

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110618\
 Data File : FE029024.D
 Signal(s) : FID1B.CH
 Acq On : 06 Nov 2018 16:03
 Operator : DD\SJ
 Sample : J5826-10
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 07 08:35:45 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE102518.M
 Quant Title :
 QLast Update : Thu Oct 25 04:58:05 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.914	2710832	15.754 ug/ml
Target Compounds			
4) N-TETRADECANE	8.501f	1293047	7.001 ug/ml
8) N-DOCOSANE	14.007	831954	4.147 ug/ml
10) N-TETRACOSANE	15.115	259013	1.334 ug/ml
11) N-HEXACOSANE	16.141	133492	0.709 ug/ml
12) N-OCTACOSANE	17.096	738613	4.051 ug/ml
13) N-TRIACONTANE	17.987	1107690	6.223 ug/ml
14) N-DOTRIACONTANE	18.822	2528981	14.426 ug/ml
15) N-TETRATRIACONTANE	19.609	233211	1.324 ug/ml
16) N-HEXATRIACONTANE	20.352	245279	1.384 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110618\
Data File : FE029024.D
Signal(s) : FID1B.CH
Acq On : 06 Nov 2018 16:03
Operator : DD\SJ
Sample : J5826-10
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 07 08:35:45 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE102518.M
Quant Title :
QLast Update : Thu Oct 25 04:58:05 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

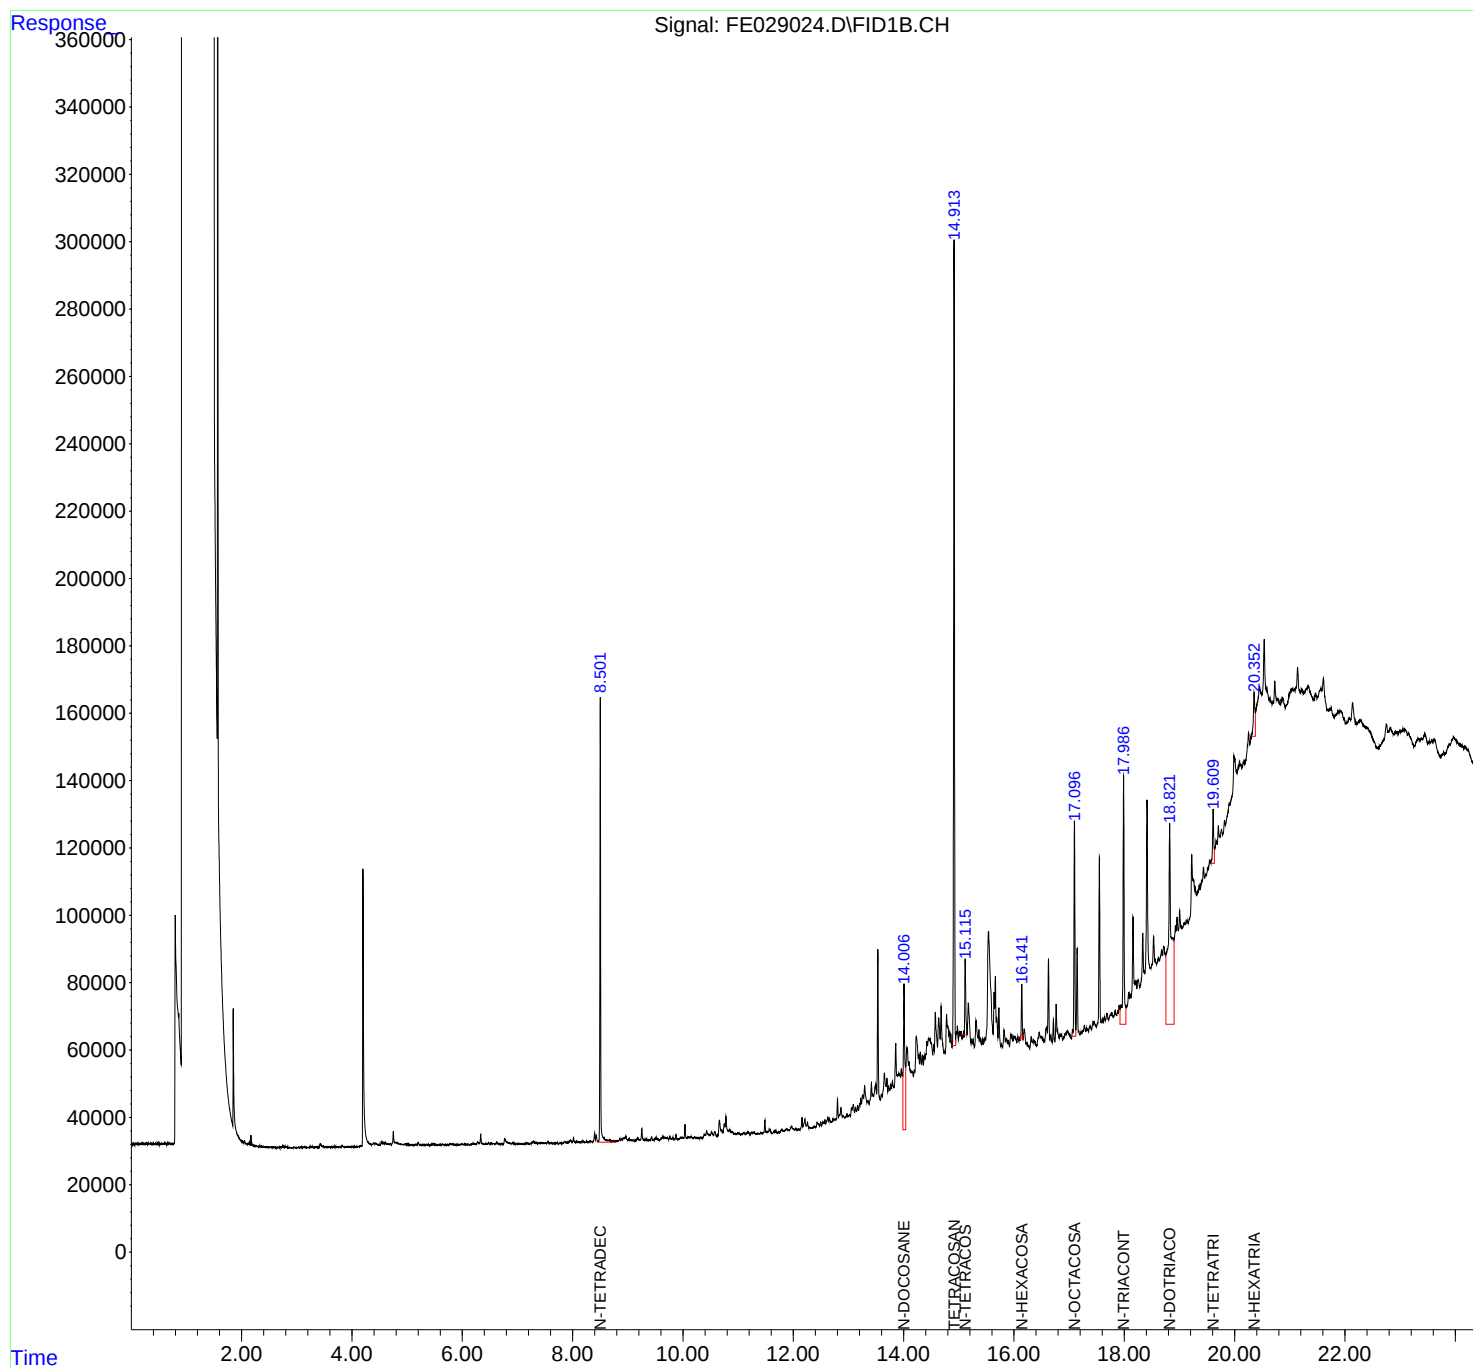

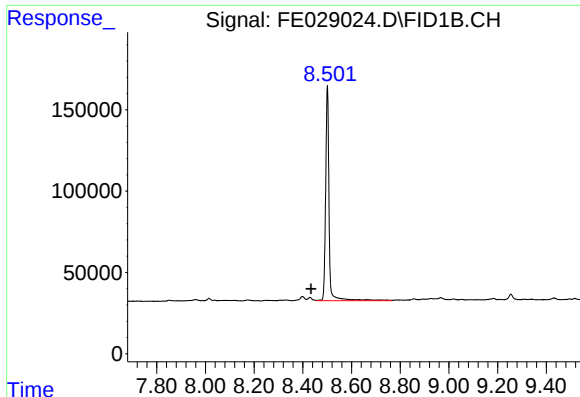


#4 N-TETRADECANE

R.T.: 8.501 min
Delta R.T.: 0.067 min
Response: 1293047
Conc: 7.00 ug/ml

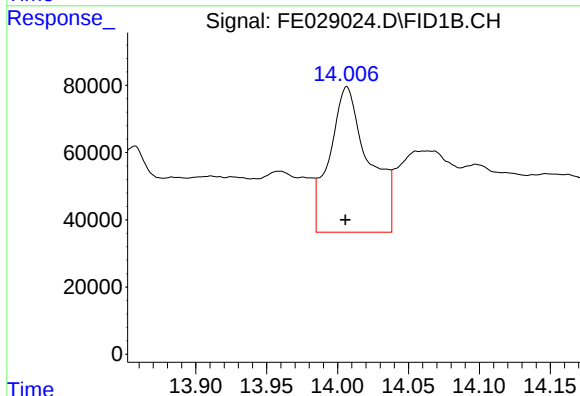


#8 N-DOCOSANE

R.T.: 14.007 min
Delta R.T.: 0.000 min
Response: 831954
Conc: 4.15 ug/ml

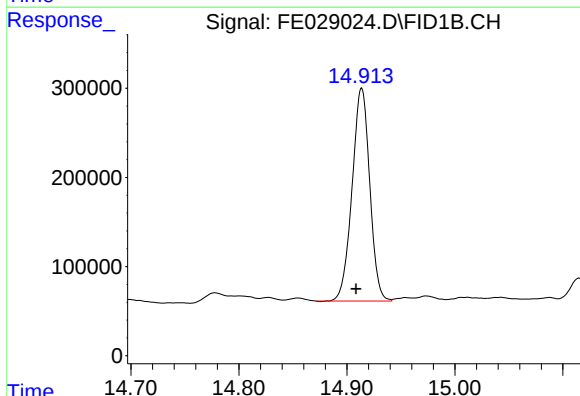


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.914 min
Delta R.T.: 0.005 min
Response: 2710832
Conc: 15.75 ug/ml

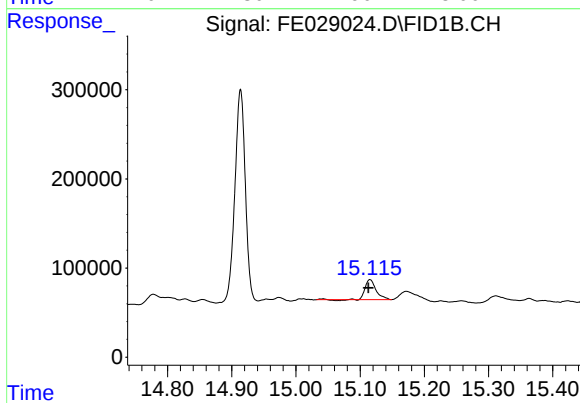


#10 N-TETRACOSANE

R.T.: 15.115 min
Delta R.T.: 0.003 min
Response: 259013
Conc: 1.33 ug/ml

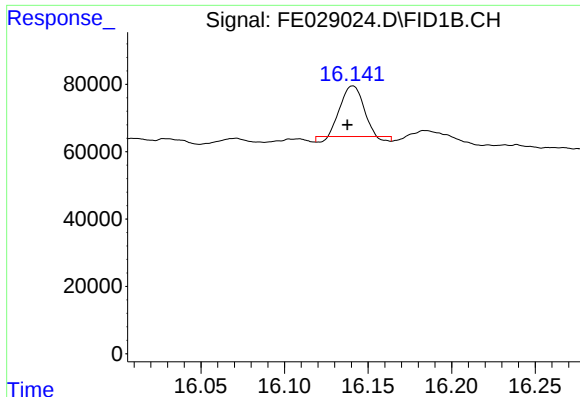


#11 N-HEXACOSANE

R.T.: 16.141 min
Delta R.T.: 0.003 min
Response: 133492
Conc: 0.71 ug/ml

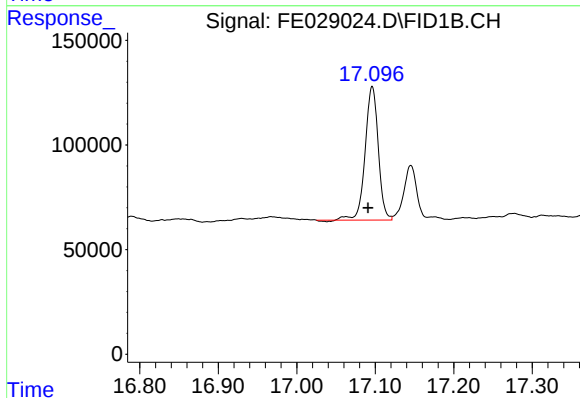


#12 N-OCTACOSANE

R.T.: 17.096 min
Delta R.T.: 0.005 min
Response: 738613
Conc: 4.05 ug/ml

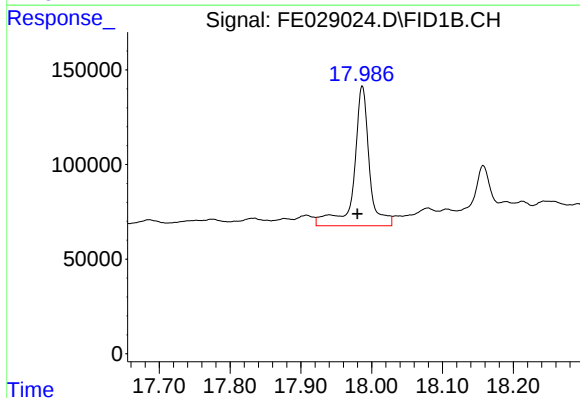


#13 N-TRIACONTANE

R.T.: 17.987 min
Delta R.T.: 0.007 min
Response: 1107690
Conc: 6.22 ug/ml

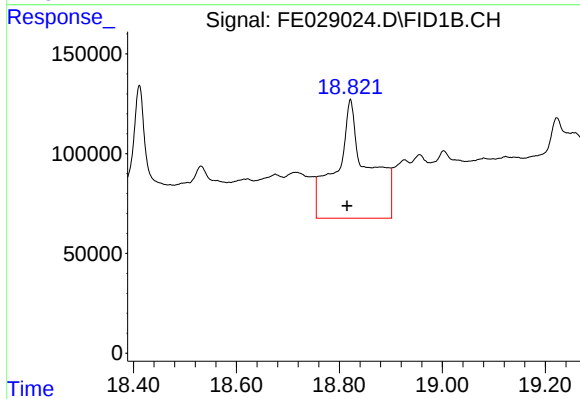


#14 N-DOTRIACONTANE

R.T.: 18.822 min
Delta R.T.: 0.007 min
Response: 2528981
Conc: 14.43 ug/ml

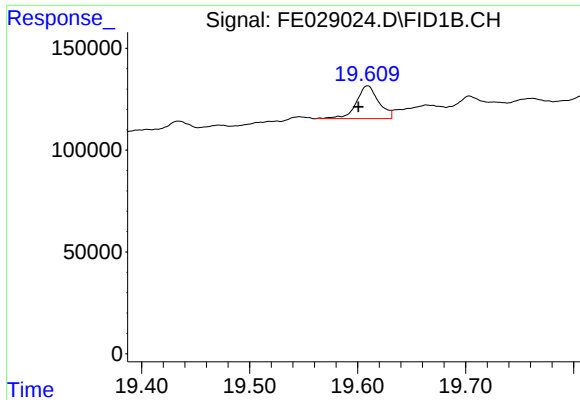

#15 N-TETRATRIACONTANE

R.T.: 19.609 min
Delta R.T.: 0.009 min
Response: 233211
Conc: 1.32 ug/ml

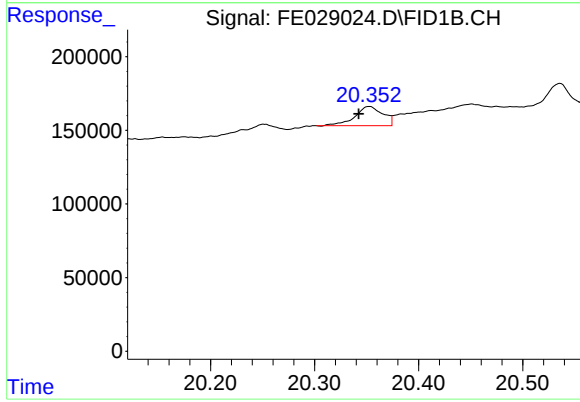

#16 N-HEXATRIACONTANE

R.T.: 20.352 min
Delta R.T.: 0.010 min
Response: 245279
Conc: 1.38 ug/ml