

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110618\
 Data File : FE029029.D
 Signal(s) : FID1B.CH
 Acq On : 06 Nov 2018 18:49
 Operator : DD\SJ
 Sample : J5826-02MSD
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 07 08:36:11 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE102518.M
 Quant Title :
 QLast Update : Thu Oct 25 04:58:05 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.910	3426725	19.915 ug/ml
Target Compounds			
2) N-DECANE	4.602	3666380	22.232 ug/ml
3) N-DODECANE	6.626	4092289	23.691 ug/ml
4) N-TETRADECANE	8.431	4113466	22.271 ug/ml
5) N-HEXADECANE	10.038	4169967	21.509 ug/ml
6) N-OCTADECANE	11.487	3995004	19.690 ug/ml
7) N-EICOSANE	12.803	4370430	21.721 ug/ml
8) N-DOCOSANE	14.008	4121345	20.543 ug/mlm
10) N-TETRACOSANE	15.117	3928217	20.232 ug/mlm
11) N-HEXACOSANE	16.142	3865753	20.526 ug/mlm
12) N-OCTACOSANE	17.096	4278587	23.465 ug/mlm


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110618\
Data File : FE029029.D
Signal(s) : FID1B.CH
Acq On : 06 Nov 2018 18:49
Operator : DD\SJ
Sample : J5826-02MSD
Misc :
ALS Vial : 14 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 07 08:36:11 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE102518.M
Quant Title :
QLast Update : Thu Oct 25 04:58:05 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

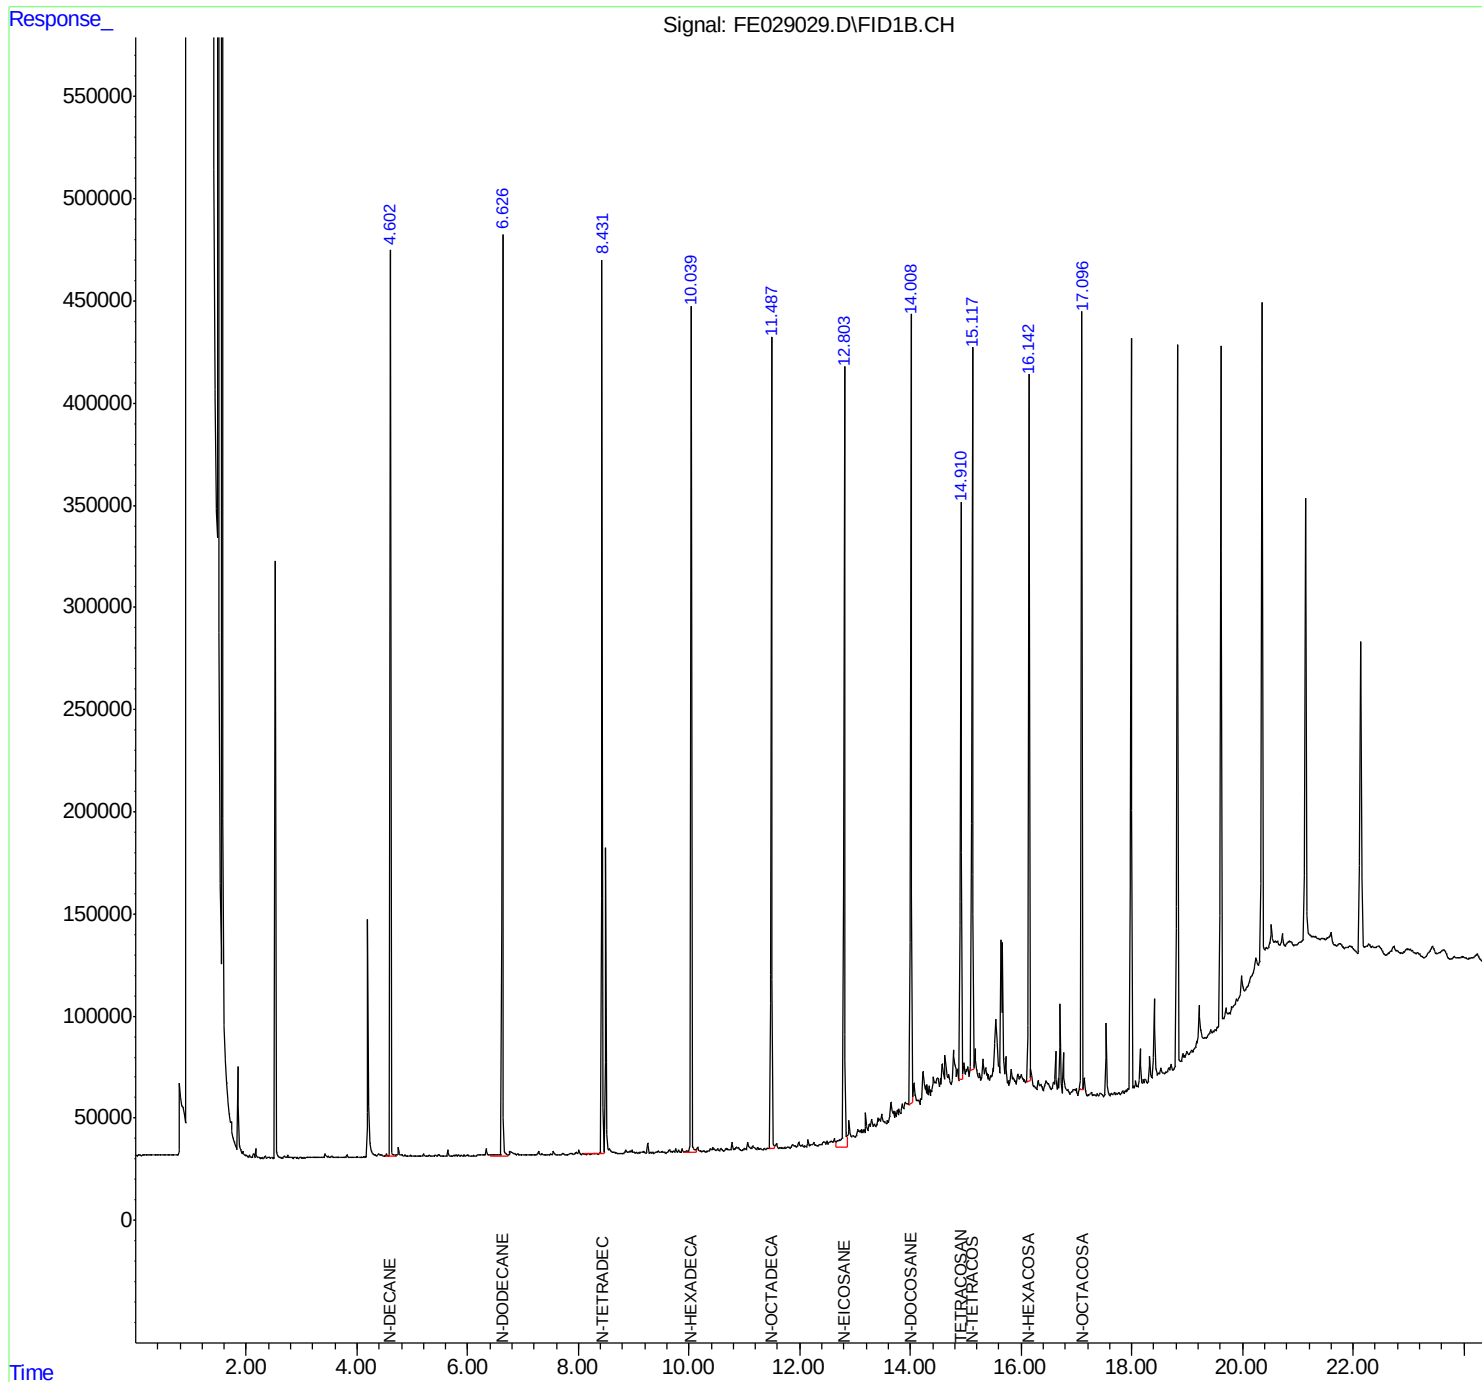

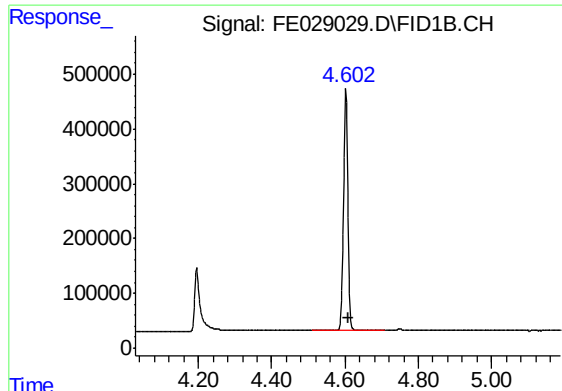


#2 N-DECANE

R.T.: 4.602 min
Delta R.T.: -0.006 min
Response: 3666380
Conc: 22.23 ug/ml

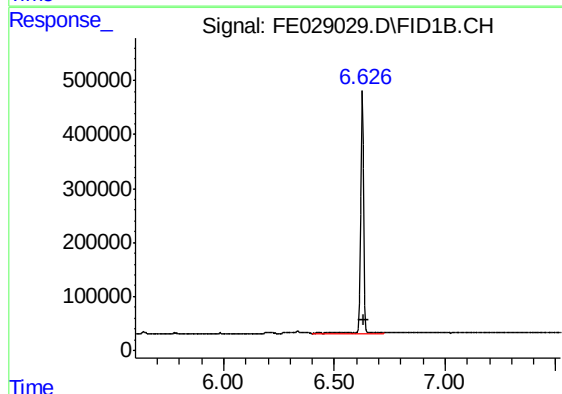


#3 N-DODECANE

R.T.: 6.626 min
Delta R.T.: -0.006 min
Response: 4092289
Conc: 23.69 ug/ml

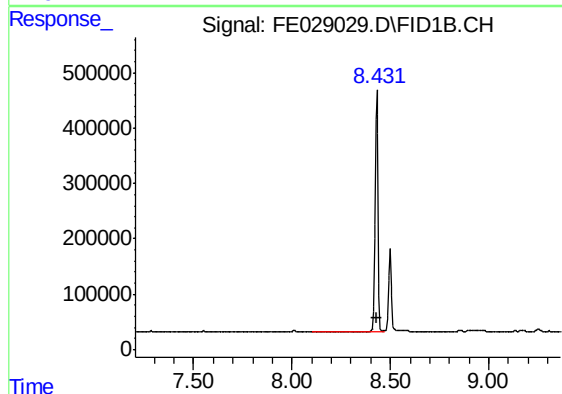


#4 N-TETRADECANE

R.T.: 8.431 min
Delta R.T.: -0.003 min
Response: 4113466
Conc: 22.27 ug/ml

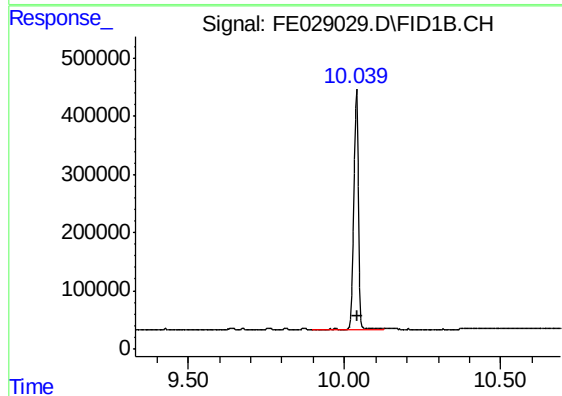


#5 N-HEXADECANE

R.T.: 10.038 min
Delta R.T.: -0.003 min
Response: 4169967
Conc: 21.51 ug/ml

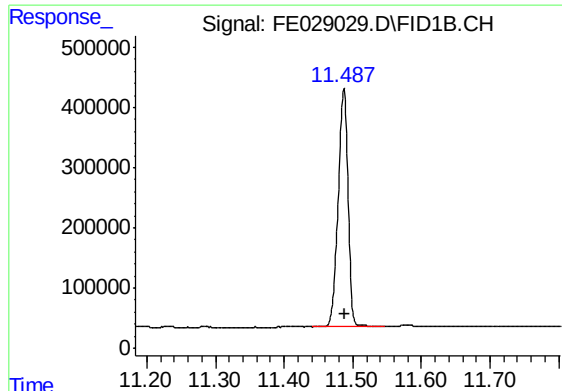


#6 N-OCTADECANE

R.T.: 11.487 min
Delta R.T.: -0.001 min
Response: 3995004
Conc: 19.69 ug/ml

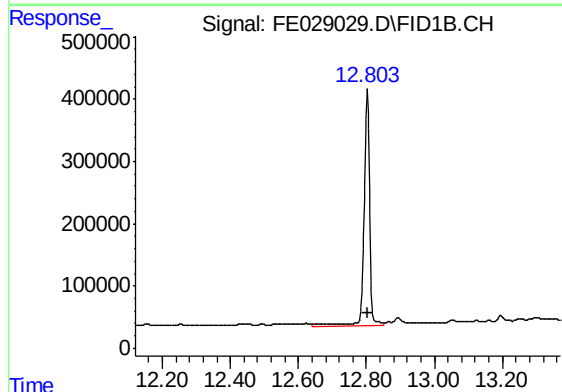


#7 N-EICOSANE

R.T.: 12.803 min
Delta R.T.: 0.000 min
Response: 4370430
Conc: 21.72 ug/ml

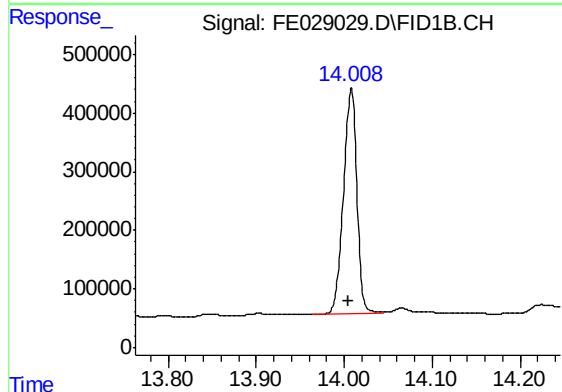


#8 N-DOCOSANE

R.T.: 14.008 min
Delta R.T.: 0.002 min
Response: 4121345
Conc: 20.54 ug/ml m

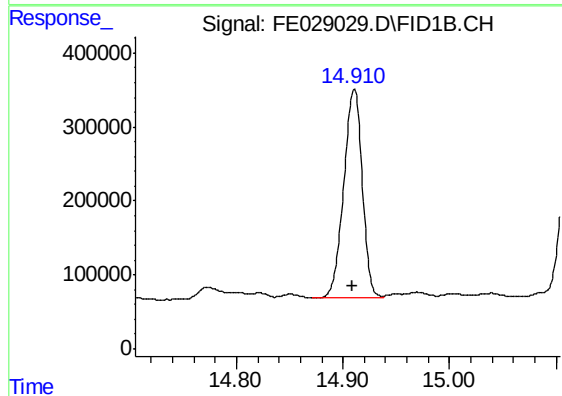


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.910 min
Delta R.T.: 0.002 min
Response: 3426725
Conc: 19.91 ug/ml

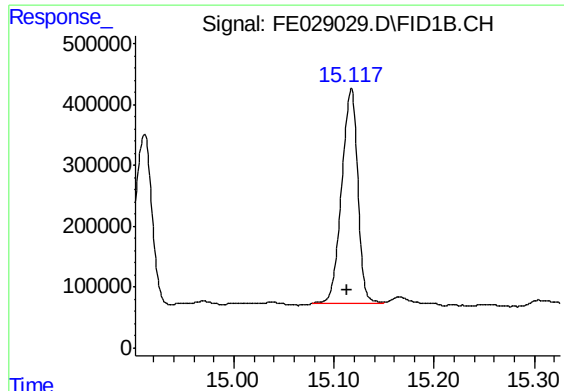


#10 N-TETRACOSANE

R.T.: 15.117 min
Delta R.T.: 0.004 min
Response: 3928217
Conc: 20.23 ug/ml m

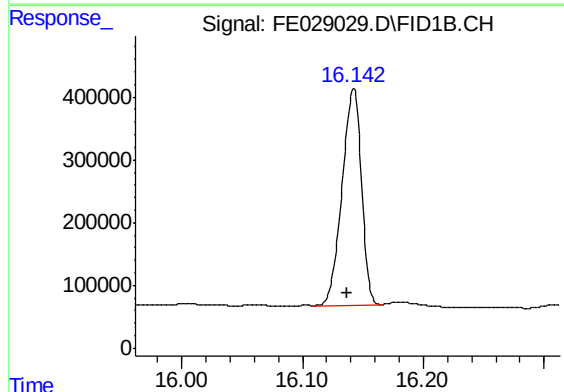

#11 N-HEXACOSANE

R.T.: 16.142 min
Delta R.T.: 0.005 min
Response: 3865753
Conc: 20.53 ug/ml m

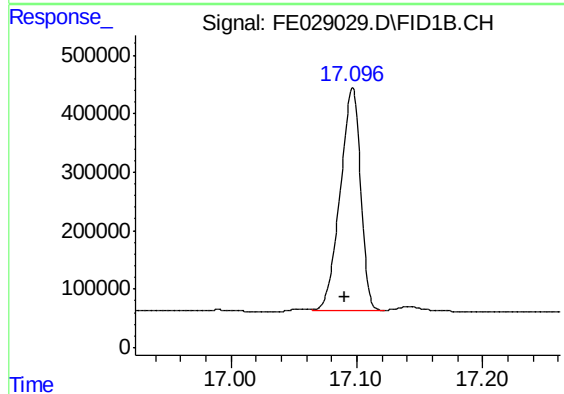

#12 N-OCTACOSANE

R.T.: 17.096 min
Delta R.T.: 0.006 min
Response: 4278587
Conc: 23.46 ug/ml m