

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110620\
 Data File : FE033124.D
 Signal(s) : FID1B.CH
 Acq On : 07 Nov 2020 3:35
 Operator : DD\AJ
 Sample : L4656-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 09 16:45:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE110620.M
 Quant Title :
 QLast Update : Mon Nov 09 16:39:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.626	7271608	24.187 ug/ml
Target Compounds			
6) N-TETRADECANE	8.256	3503384	11.184 ug/ml
7) N-HEXADECANE	9.810	487224	1.568 ug/ml
8) N-OCTADECANE	11.260	406406	1.321 ug/ml
9) N-EICOSANE	12.546	1635534	5.455 ug/ml
10) N-TETRACOSANE	14.843	9600992	32.274 ug/ml
11) N-OCTACOSANE	16.851	2863481	10.065 ug/ml
12) N-DOTRIACONTANE	18.507	1781169	6.827 ug/ml
14) N-HEXATRIACONTANE	20.029	1404267	6.254 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110620\
Data File : FE033124.D
Signal(s) : FID1B.CH
Acq On : 07 Nov 2020 3:35
Operator : DD\AJ
Sample : L4656-04
Misc :
ALS Vial : 20 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 09 16:45:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE110620.M
Quant Title :
QLast Update : Mon Nov 09 16:39:48 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

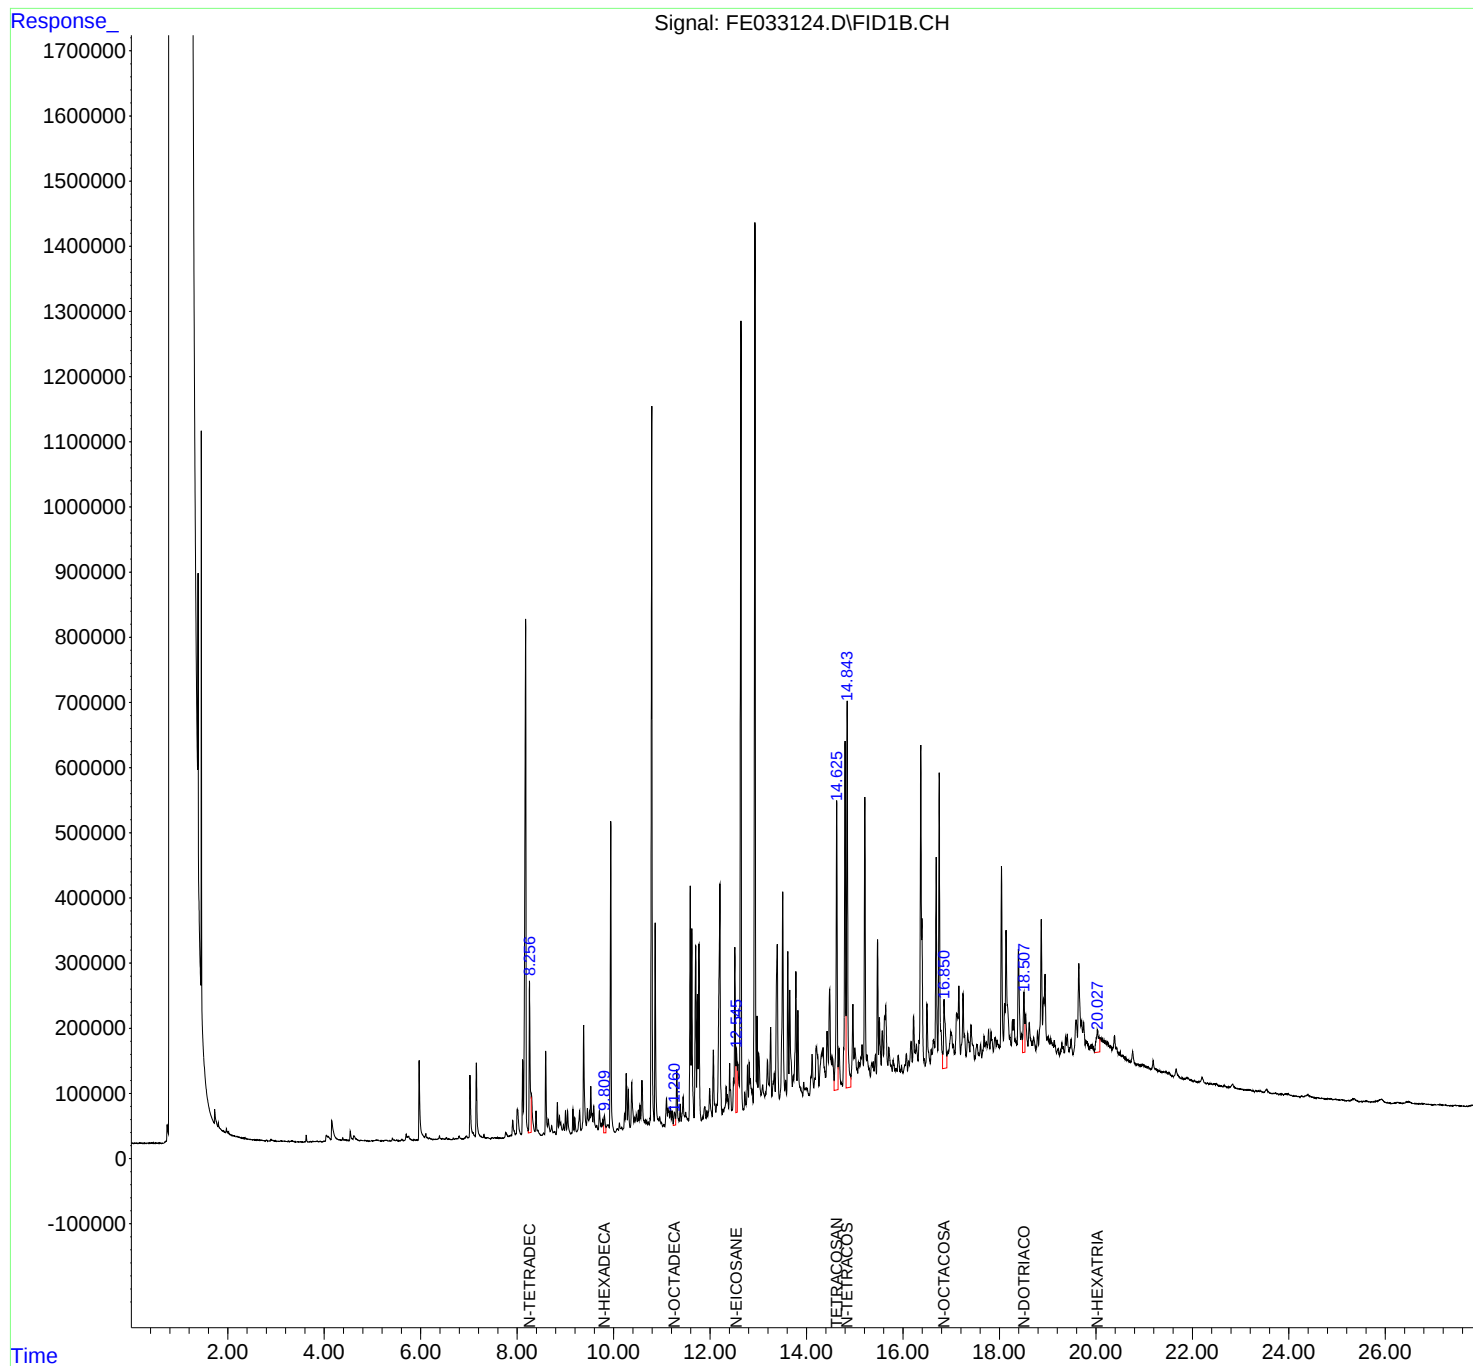

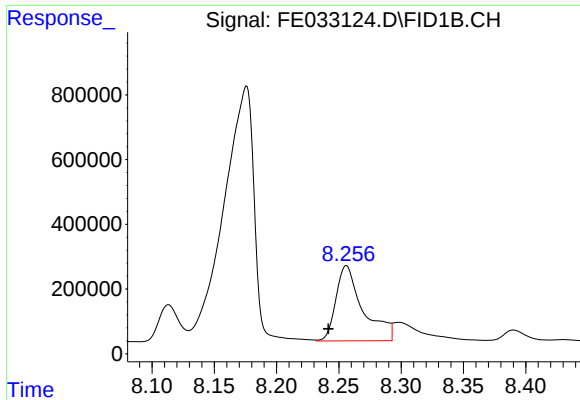


#6 N-TETRADECANE

R.T.: 8.256 min
Delta R.T.: 0.015 min
Response: 3503384
Conc: 11.18 ug/ml

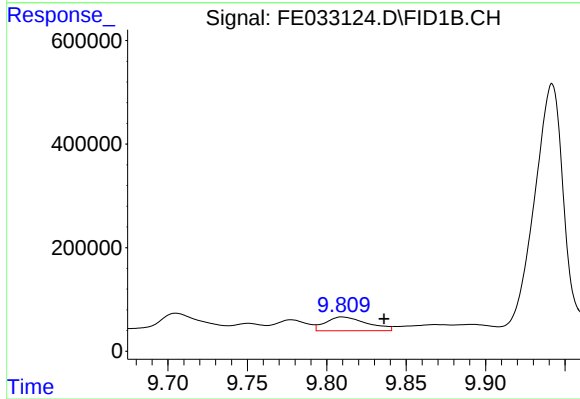


#7 N-HEXADECANE

R.T.: 9.810 min
Delta R.T.: -0.026 min
Response: 487224
Conc: 1.57 ug/ml

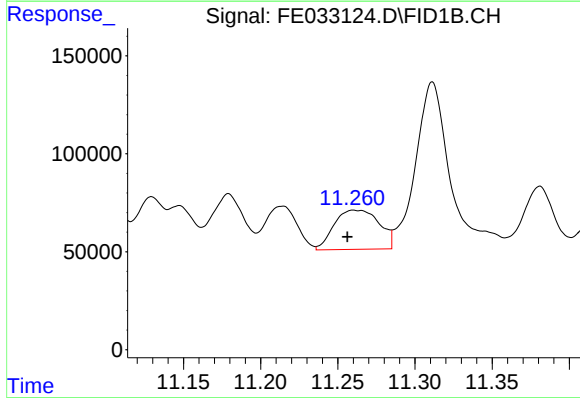


#8 N-OCTADECANE

R.T.: 11.260 min
Delta R.T.: 0.004 min
Response: 406406
Conc: 1.32 ug/ml

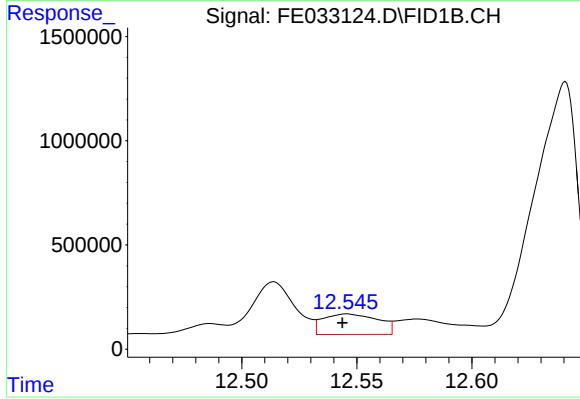


#9 N-EICOSANE

R.T.: 12.546 min
Delta R.T.: 0.002 min
Response: 1635534
Conc: 5.46 ug/ml

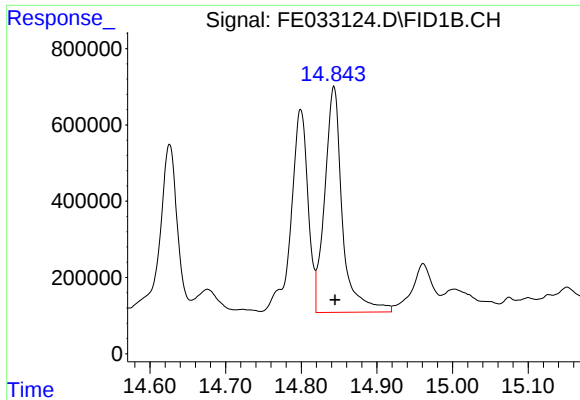


#10 N-TETRACOSANE

R.T.: 14.843 min
Delta R.T.: -0.001 min
Response: 9600992
Conc: 32.27 ug/ml

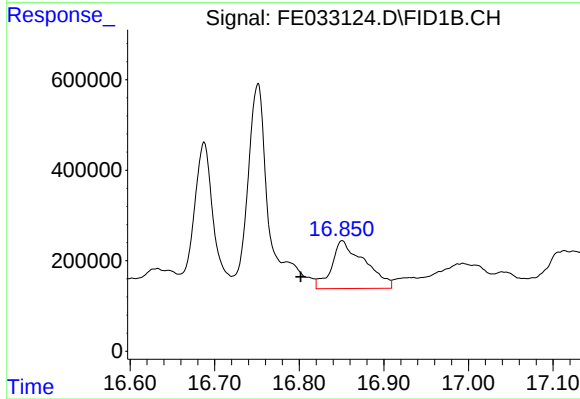


#11 N-OCTACOSANE

R.T.: 16.851 min
Delta R.T.: 0.049 min
Response: 2863481
Conc: 10.06 ug/ml

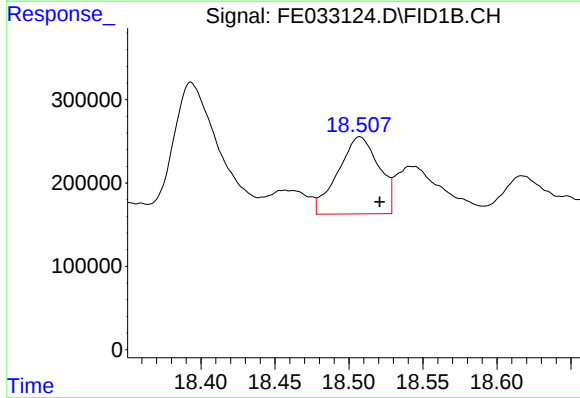


#12 N-DOTRIACONTANE

R.T.: 18.507 min
Delta R.T.: -0.013 min
Response: 1781169
Conc: 6.83 ug/ml

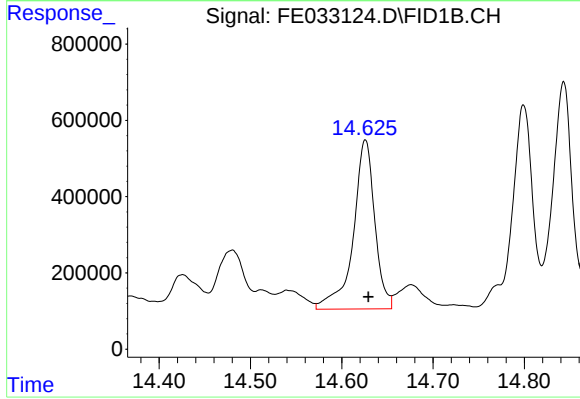

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.626 min
Delta R.T.: -0.003 min
Response: 7271608
Conc: 24.19 ug/ml

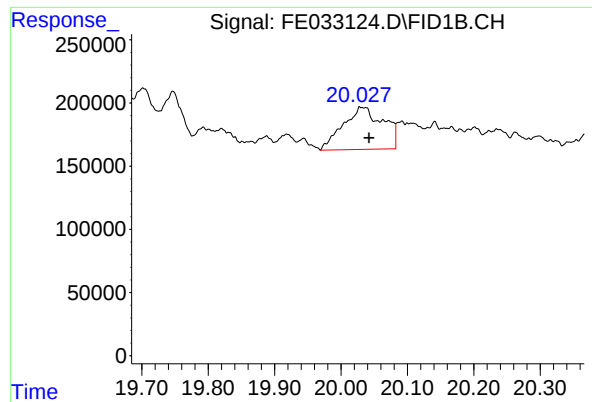

#14 N-HEXATRIACONTANE

R.T.: 20.029 min
Delta R.T.: -0.013 min
Response: 1404267
Conc: 6.25 ug/ml