

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110620\
 Data File : FE033131.D
 Signal(s) : FID1B.CH
 Acq On : 07 Nov 2020 7:59
 Operator : DD\AJ
 Sample : L4656-14
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 09 16:46:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE110620.M
 Quant Title :
 QLast Update : Mon Nov 09 16:39:48 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.624	4847805	16.125 ug/ml
Target Compounds			
6) N-TETRADECANE	8.252	1834574	5.857 ug/ml
8) N-OCTADECANE	11.309	247764	0.805 ug/ml
9) N-EICOSANE	12.524	372847	1.244 ug/ml
10) N-TETRACOSANE	14.830	3757444	12.631 ug/ml
11) N-OCTACOSANE	16.845	817448	2.873 ug/ml
12) N-DOTRIACONTANE	18.509	1256465	4.816 ug/ml
14) N-HEXATRIACONTANE	20.035	429526	1.913 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110620\
Data File : FE033131.D
Signal(s) : FID1B.CH
Acq On : 07 Nov 2020 7:59
Operator : DD\AJ
Sample : L4656-14
Misc :
ALS Vial : 27 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 09 16:46:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE110620.M
Quant Title :
QLast Update : Mon Nov 09 16:39:48 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

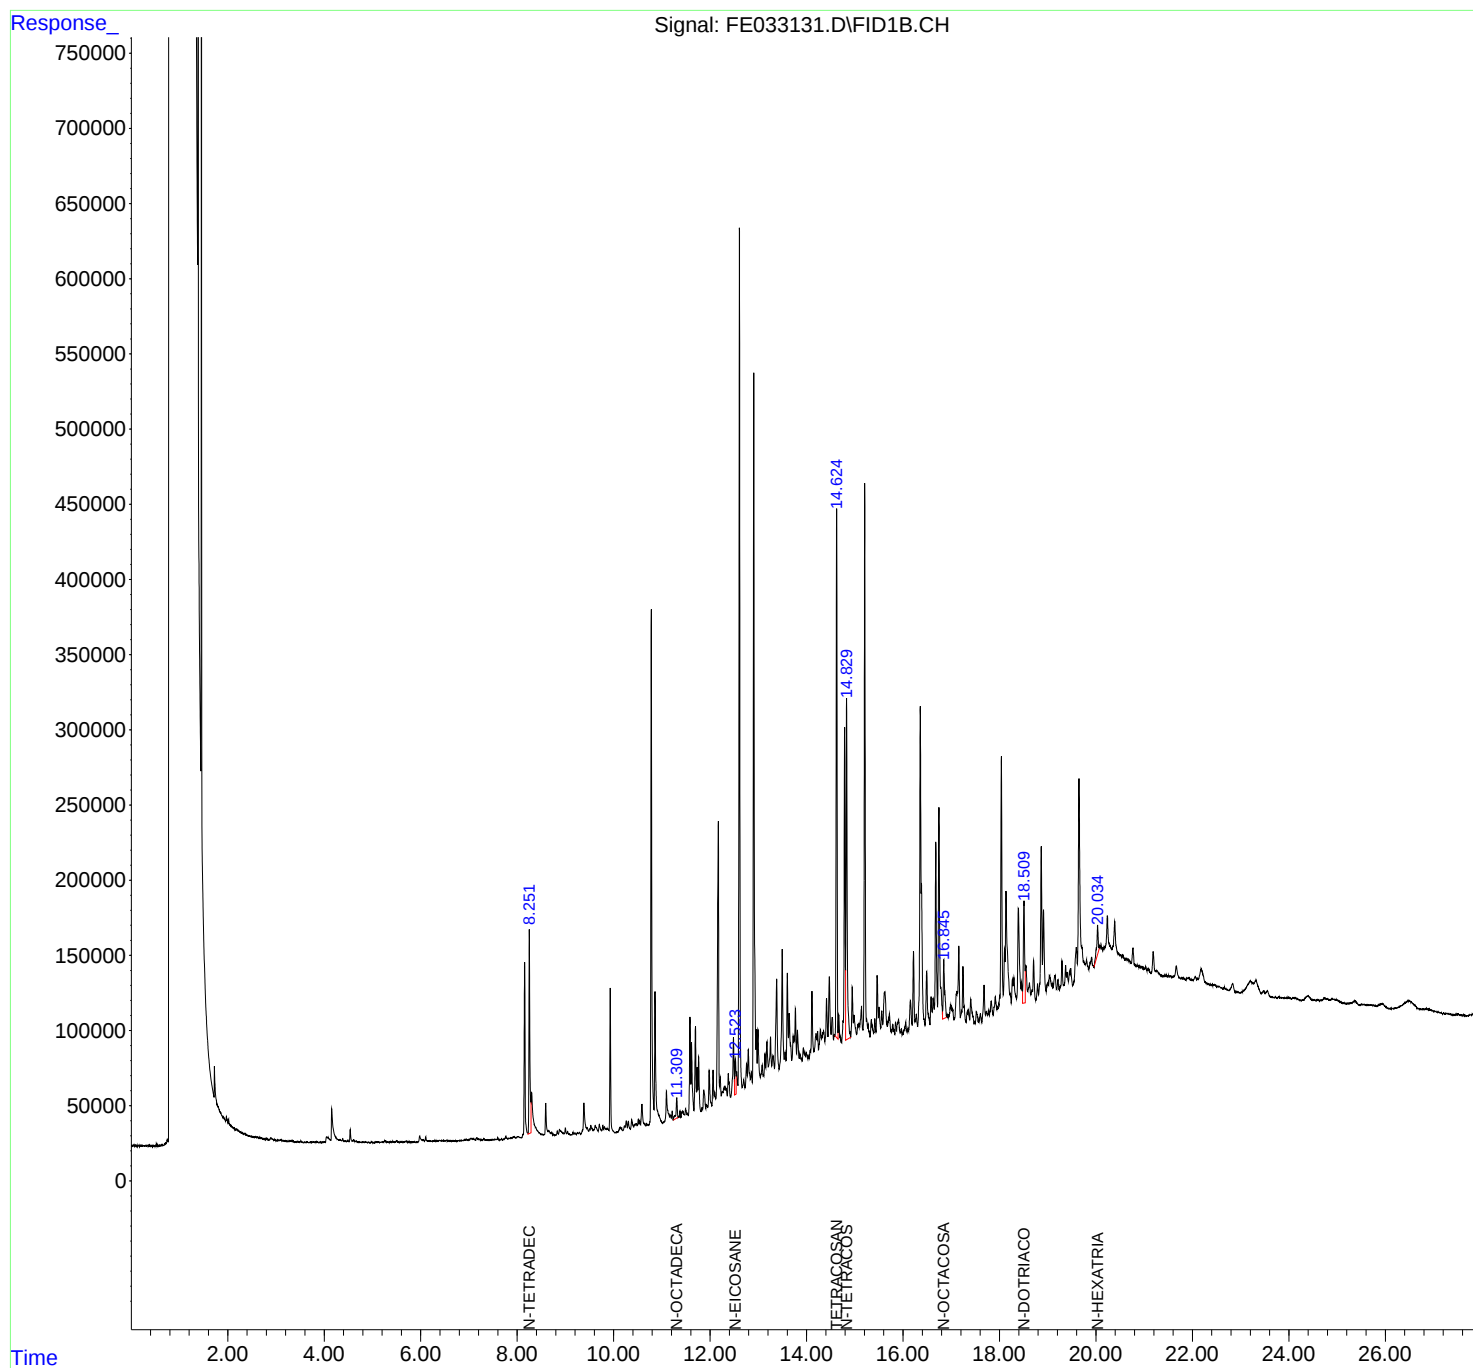

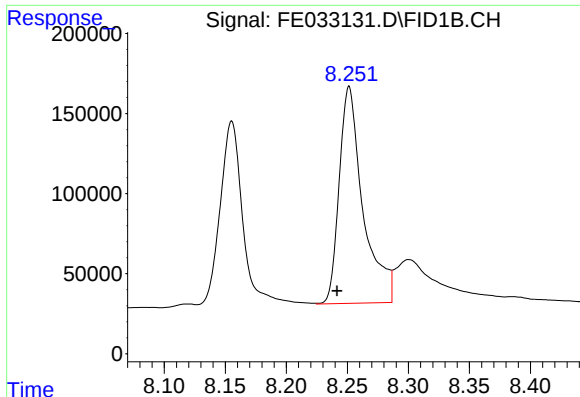


#6 N-TETRADECANE

R.T.: 8.252 min
Delta R.T.: 0.010 min
Response: 1834574
Conc: 5.86 ug/ml

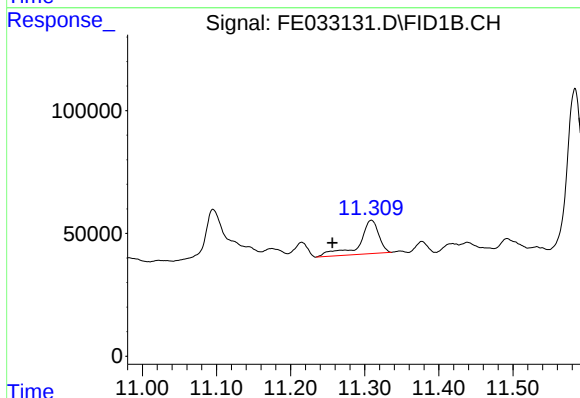


#8 N-OCTADECANE

R.T.: 11.309 min
Delta R.T.: 0.053 min
Response: 247764
Conc: 0.81 ug/ml

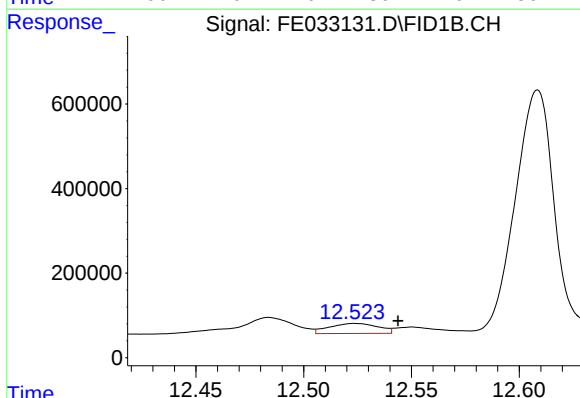


#9 N-EICOSANE

R.T.: 12.524 min
Delta R.T.: -0.020 min
Response: 372847
Conc: 1.24 ug/ml

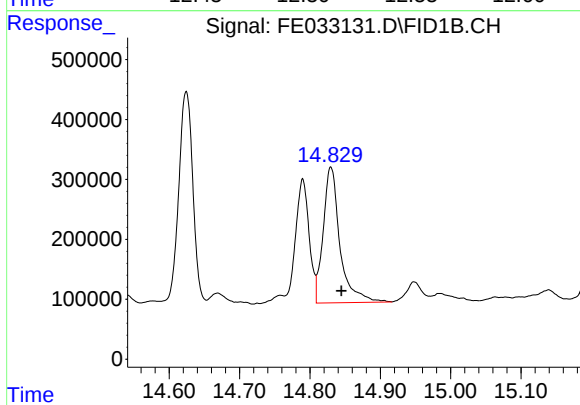


#10 N-TETRACOSANE

R.T.: 14.830 min
Delta R.T.: -0.015 min
Response: 3757444
Conc: 12.63 ug/ml

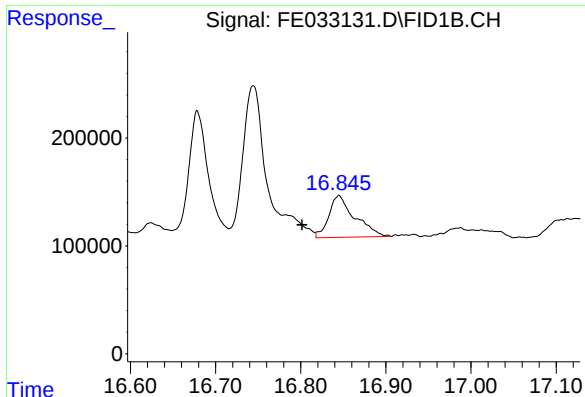


#11 N-OCTACOSANE

R.T.: 16.845 min
Delta R.T.: 0.043 min
Response: 817448
Conc: 2.87 ug/ml

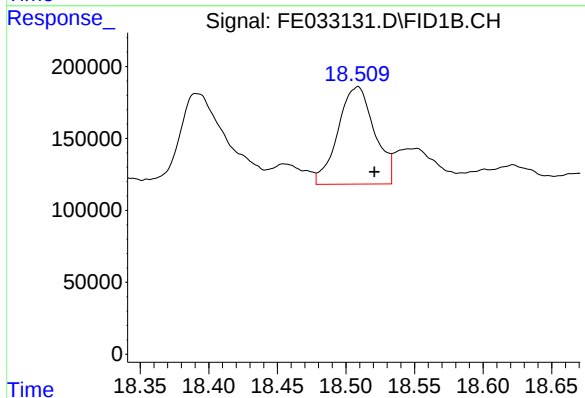


#12 N-DOTRIACONTANE

R.T.: 18.509 min
Delta R.T.: -0.012 min
Response: 1256465
Conc: 4.82 ug/ml

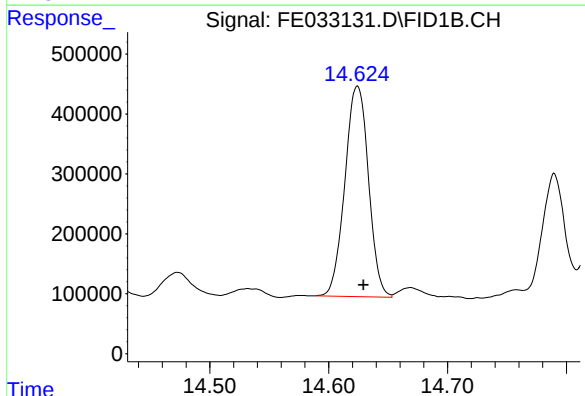

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.624 min
Delta R.T.: -0.005 min
Response: 4847805
Conc: 16.13 ug/ml

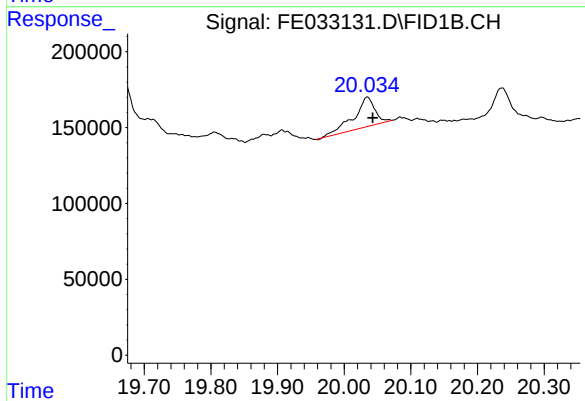

#14 N-HEXATRIACONTANE

R.T.: 20.035 min
Delta R.T.: -0.008 min
Response: 429526
Conc: 1.91 ug/ml