

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110623AL\
Data File : FE045201.D
Signal(s) : FID1B.ch
Acq On : 06 Nov 2023 08:12
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 06 11:14:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 110423.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 05:16:05 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.909	92743	0.594 ug/ml
20) T	n-Hexatriacontane (C36)	20.454	78835	0.486 ug/ml
22) T	n-Tetracontane (C40)	22.018	1724843	10.098 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110623AL\
Data File : FE045201.D
Signal(s) : FID1B.ch
Acq On : 06 Nov 2023 08:12
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 06 11:14:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 110423.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 05:16:05 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

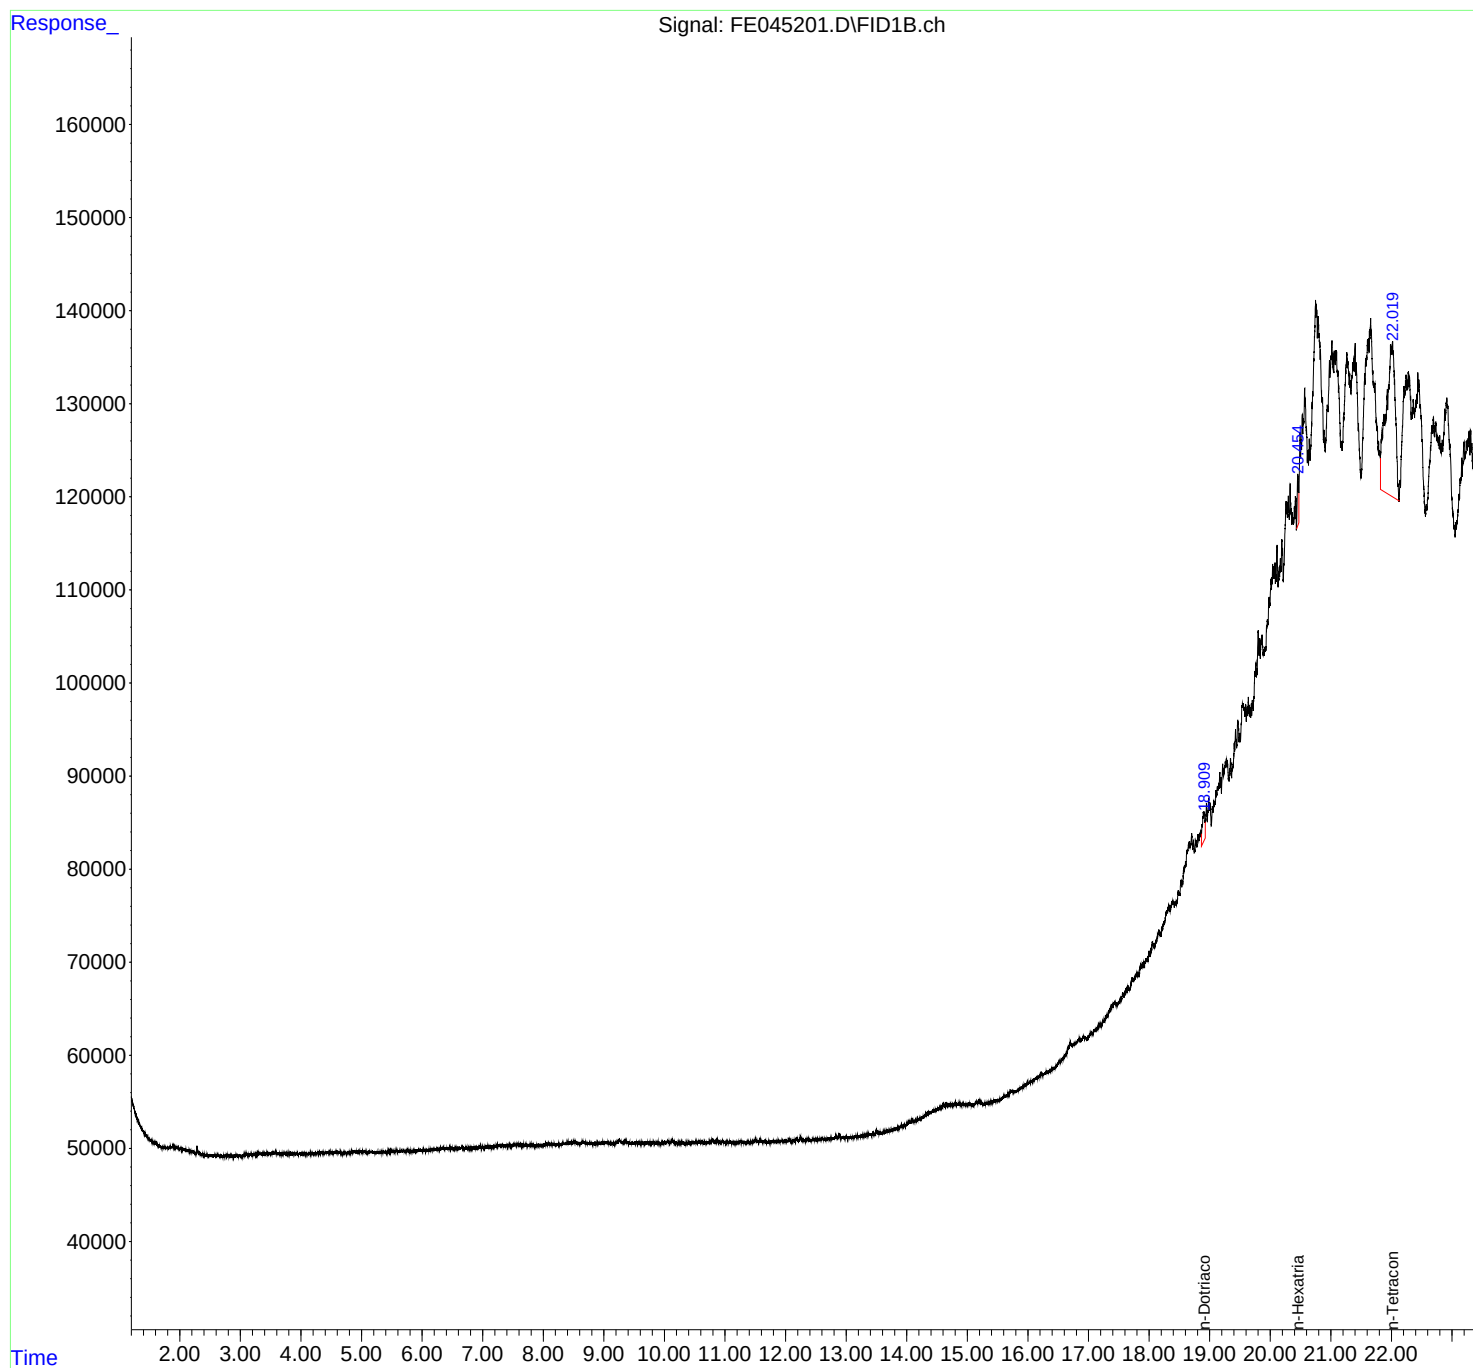


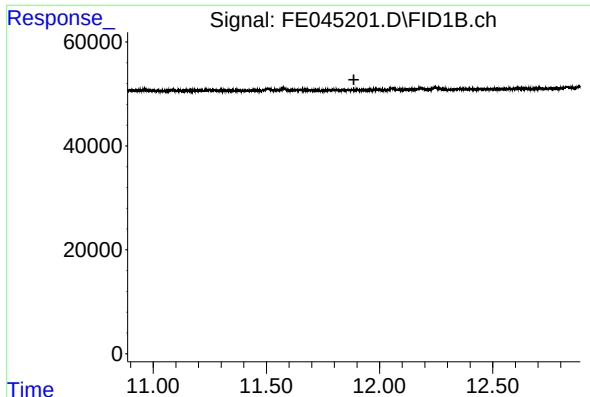

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.887 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

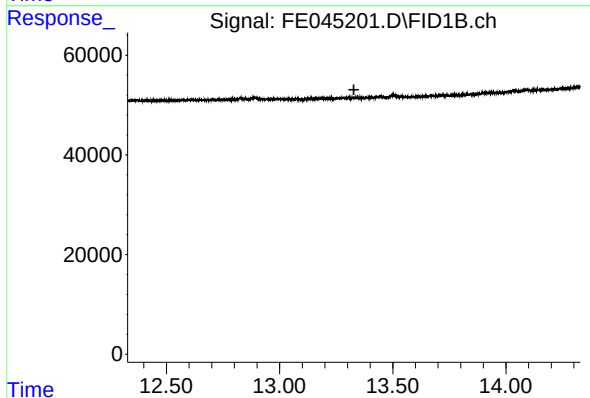


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.328 min
Response: 0
Conc: N.D.

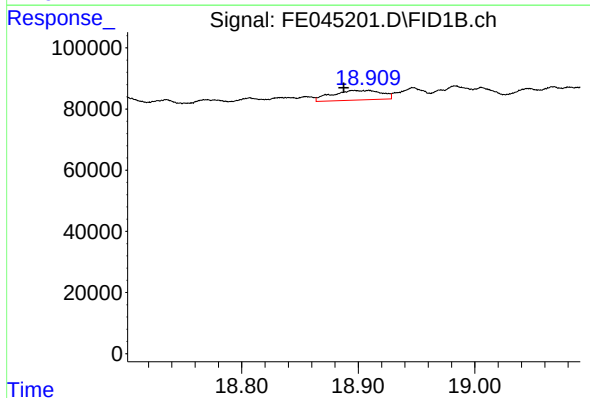


#18 n-Dotriacontane (C32)

R.T.: 18.909 min
Delta R.T.: 0.021 min
Response: 92743
Conc: 0.59 ug/ml

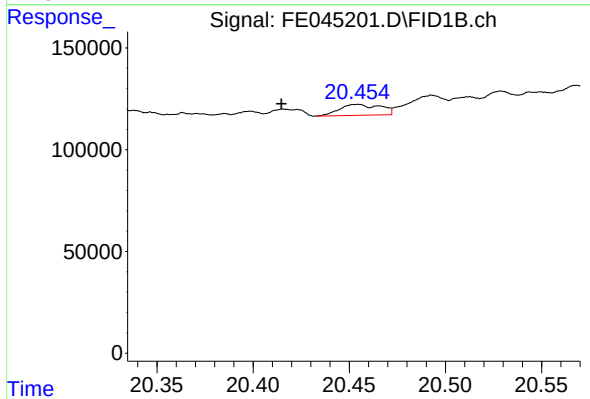

#20 n-Hexatriacontane (C36)

R.T.: 20.454 min
Delta R.T.: 0.040 min
Response: 78835
Conc: 0.49 ug/ml

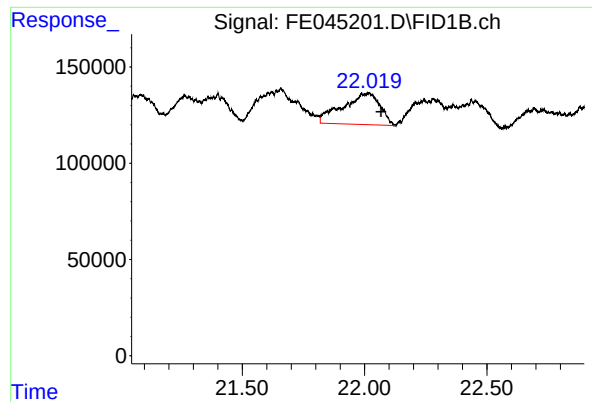

#22 n-Tetracontane (C40)

R.T.: 22.018 min
Delta R.T.: -0.049 min
Response: 1724843
Conc: 10.10 ug/ml

Instrument :

FID_E

ClientSampleId :