

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110719\
 Data File : FE030788.D
 Signal(s) : FID1B.CH
 Acq On : 07 Nov 2019 21:05
 Operator : DD\AJ
 Sample : K5675-06 50X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 TR-04-110619

Integration File: autoint1.e
 Quant Time: Nov 08 00:34:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
 Quant Title :
 QLast Update : Thu Oct 31 08:47:02 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
7) N-EICOSANE	12.628f	621991	1.702 ug/ml
8) N-DOCOSANE	13.781	342152	0.952 ug/ml
10) N-TETRACOSANE	14.869	2582204	7.260 ug/ml
12) N-OCTACOSANE	16.847	346323	1.016 ug/ml
13) N-TRIACONTANE	17.737	397420	1.197 ug/ml
14) N-DOTRIACONTANE	18.569	673163	2.109 ug/ml
15) N-TETRATRIACONTANE	19.357	134372	0.441 ug/ml
16) N-HEXATRIACONTANE	20.097	3088270	11.249 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110719\
Data File : FE030788.D
Signal(s) : FID1B.CH
Acq On : 07 Nov 2019 21:05
Operator : DD\AJ
Sample : K5675-06 50X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
TR-04-110619

Integration File: autoint1.e
Quant Time: Nov 08 00:34:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
Quant Title :
QLast Update : Thu Oct 31 08:47:02 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

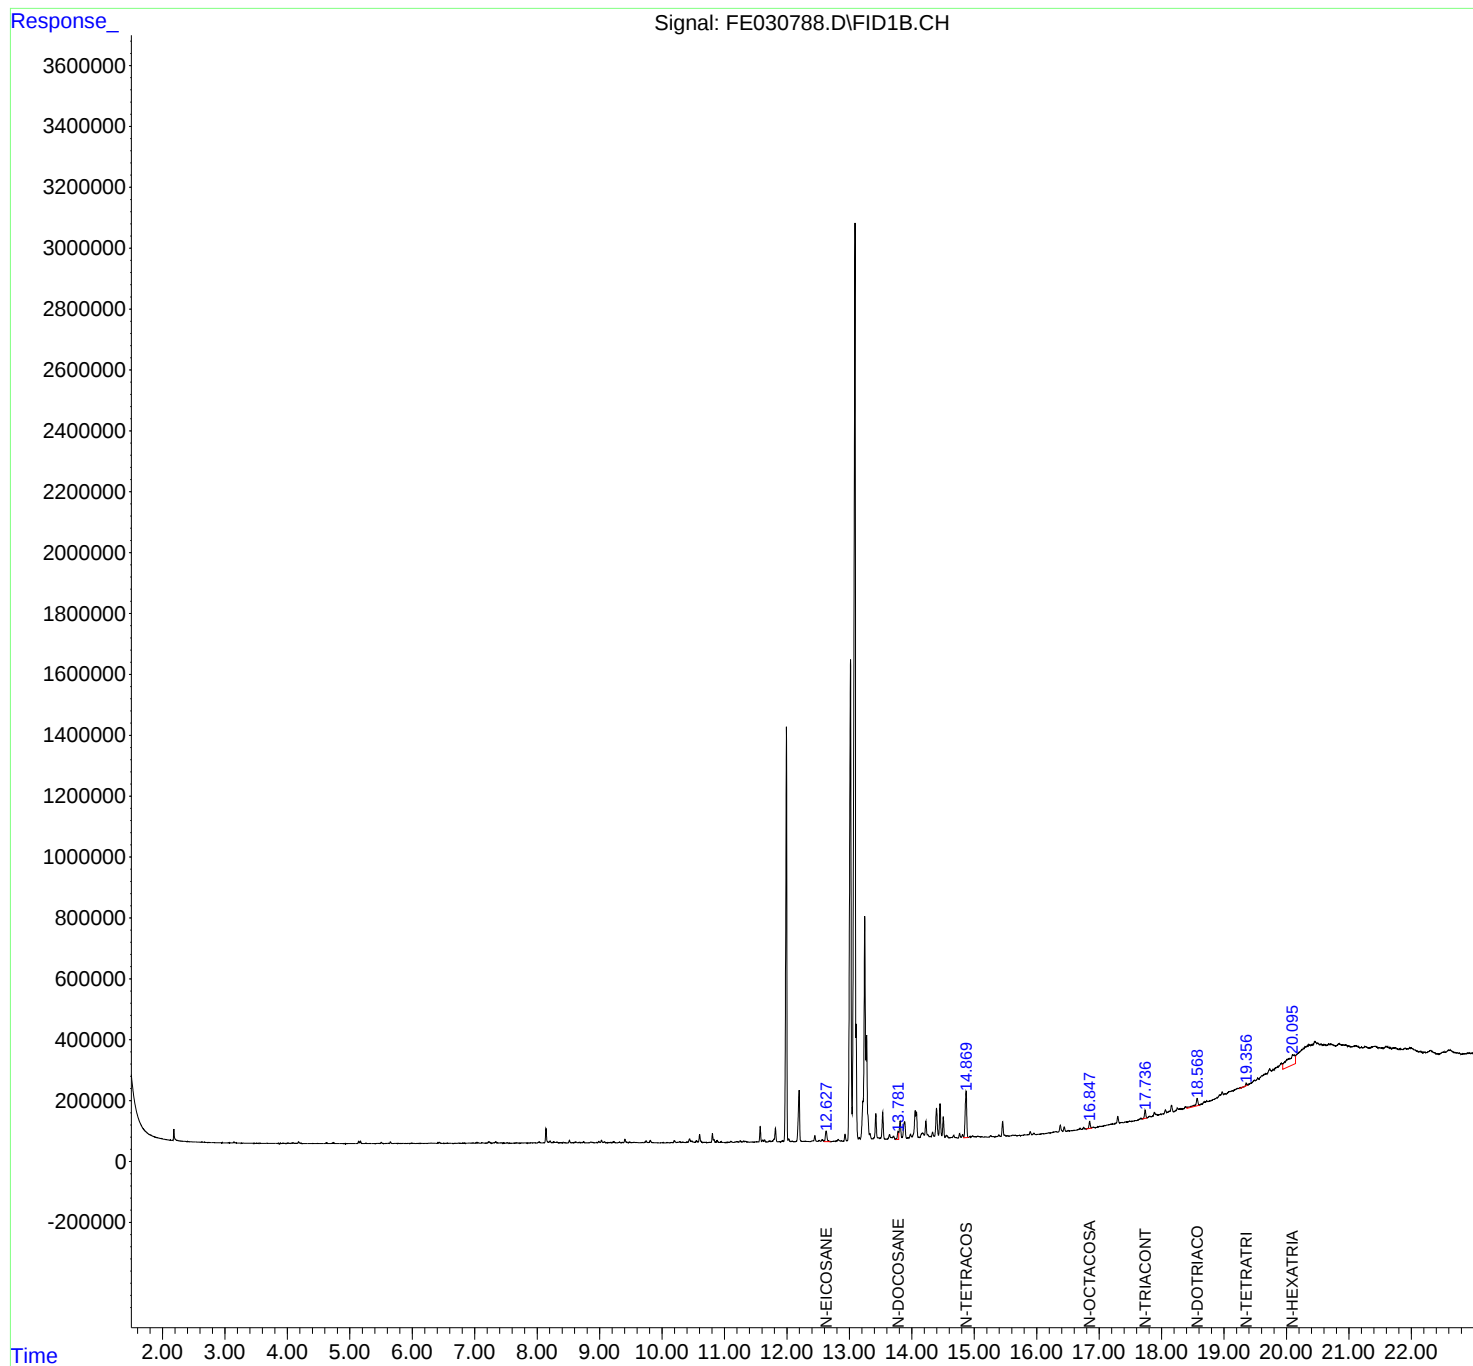


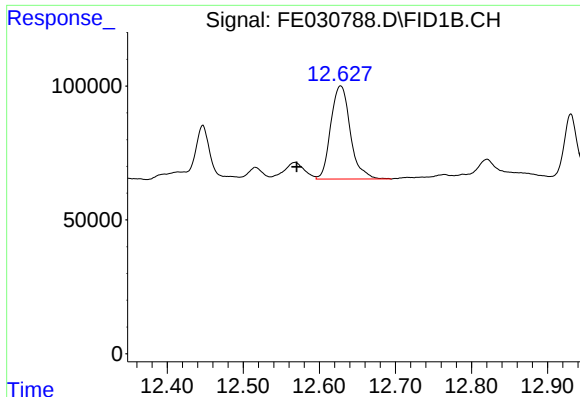

#7 N-EICOSANE


R.T.: 12.628 min
Delta R.T.: 0.058 min
Response: 621991
Conc: 1.70 ug/ml

Instrument :
FID_E
ClientSampleId :
TR-04-110619

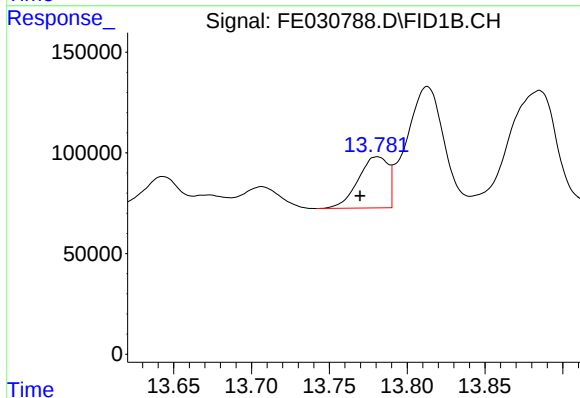


#8 N-DOCOSANE

R.T.: 13.781 min
Delta R.T.: 0.011 min
Response: 342152
Conc: 0.95 ug/ml

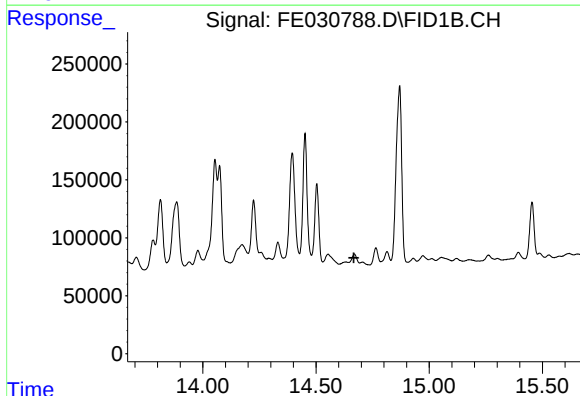


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.667 min
Response: 0
Conc: N.D.

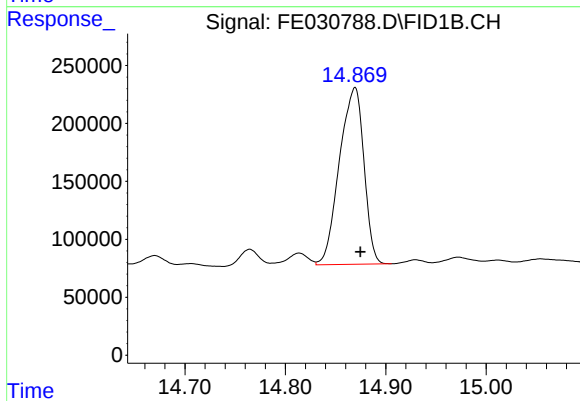

#10 N-TETRACOSANE


R.T.: 14.869 min
Delta R.T.: -0.006 min
Response: 2582204
Conc: 7.26 ug/ml

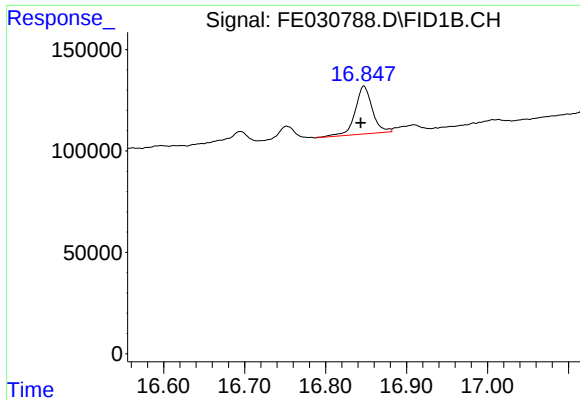

#12 N-OCTACOSANE


R.T.: 16.847 min
Delta R.T.: 0.004 min
Response: 346323
Conc: 1.02 ug/ml

Instrument :
FID_E
ClientSampleId :
TR-04-110619

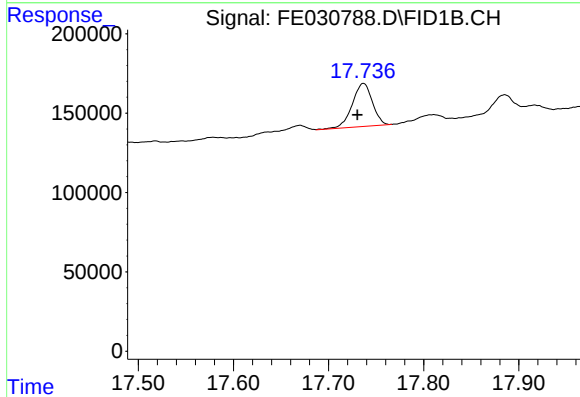


#13 N-TRIACONTANE

R.T.: 17.737 min
Delta R.T.: 0.006 min
Response: 397420
Conc: 1.20 ug/ml

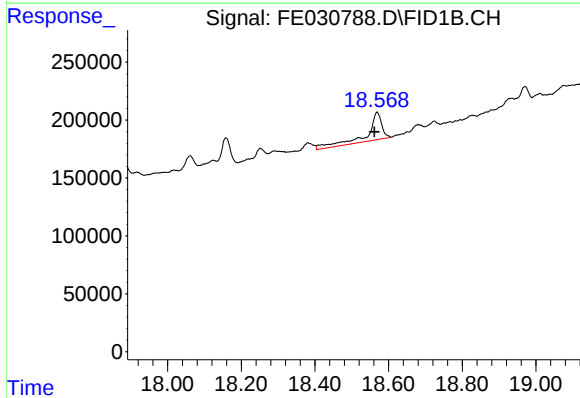


#14 N-DOTRIACONTANE

R.T.: 18.569 min
Delta R.T.: 0.007 min
Response: 673163
Conc: 2.11 ug/ml

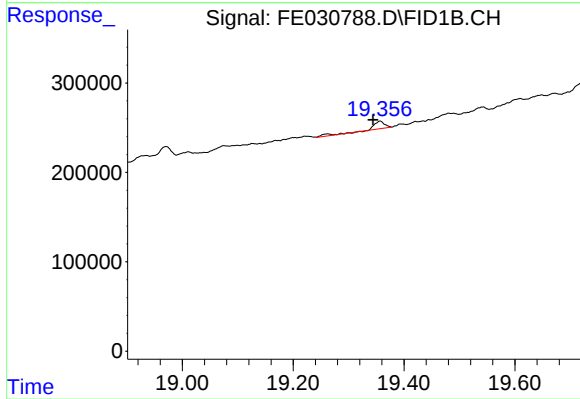

#15 N-TETRATRIACONTANE

R.T.: 19.357 min
Delta R.T.: 0.013 min
Response: 134372
Conc: 0.44 ug/ml

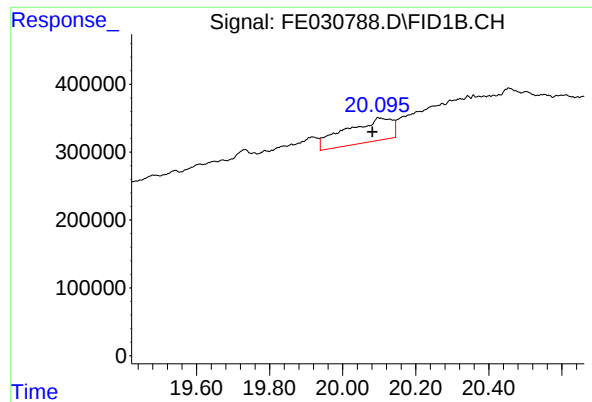

#16 N-HEXATRIACONTANE

R.T.: 20.097 min
Delta R.T.: 0.016 min
Response: 3088270
Conc: 11.25 ug/ml

Instrument :
FID_E
ClientSampleId :
TR-04-110619