

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110719\
Data File : FE030788.D
Signal(s) : FID1B.CH
Acq On : 07 Nov 2019 21:05
Operator : DD\AJ
Sample : K5675-06 50X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
TR-04-110619

Integration File: autoint1.e
Quant Time: Nov 08 00:34:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
Quant Title :
QLast Update : Thu Oct 31 08:47:02 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110719\
Data File : FE030788.D
Signal(s) : FID1B.CH
Acq On : 07 Nov 2019 21:05
Operator : DD\AJ
Sample : K5675-06 50X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
TR-04-110619

Integration File: autoint1.e
Quant Time: Nov 08 00:34:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
Quant Title :
QLast Update : Thu Oct 31 08:47:02 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

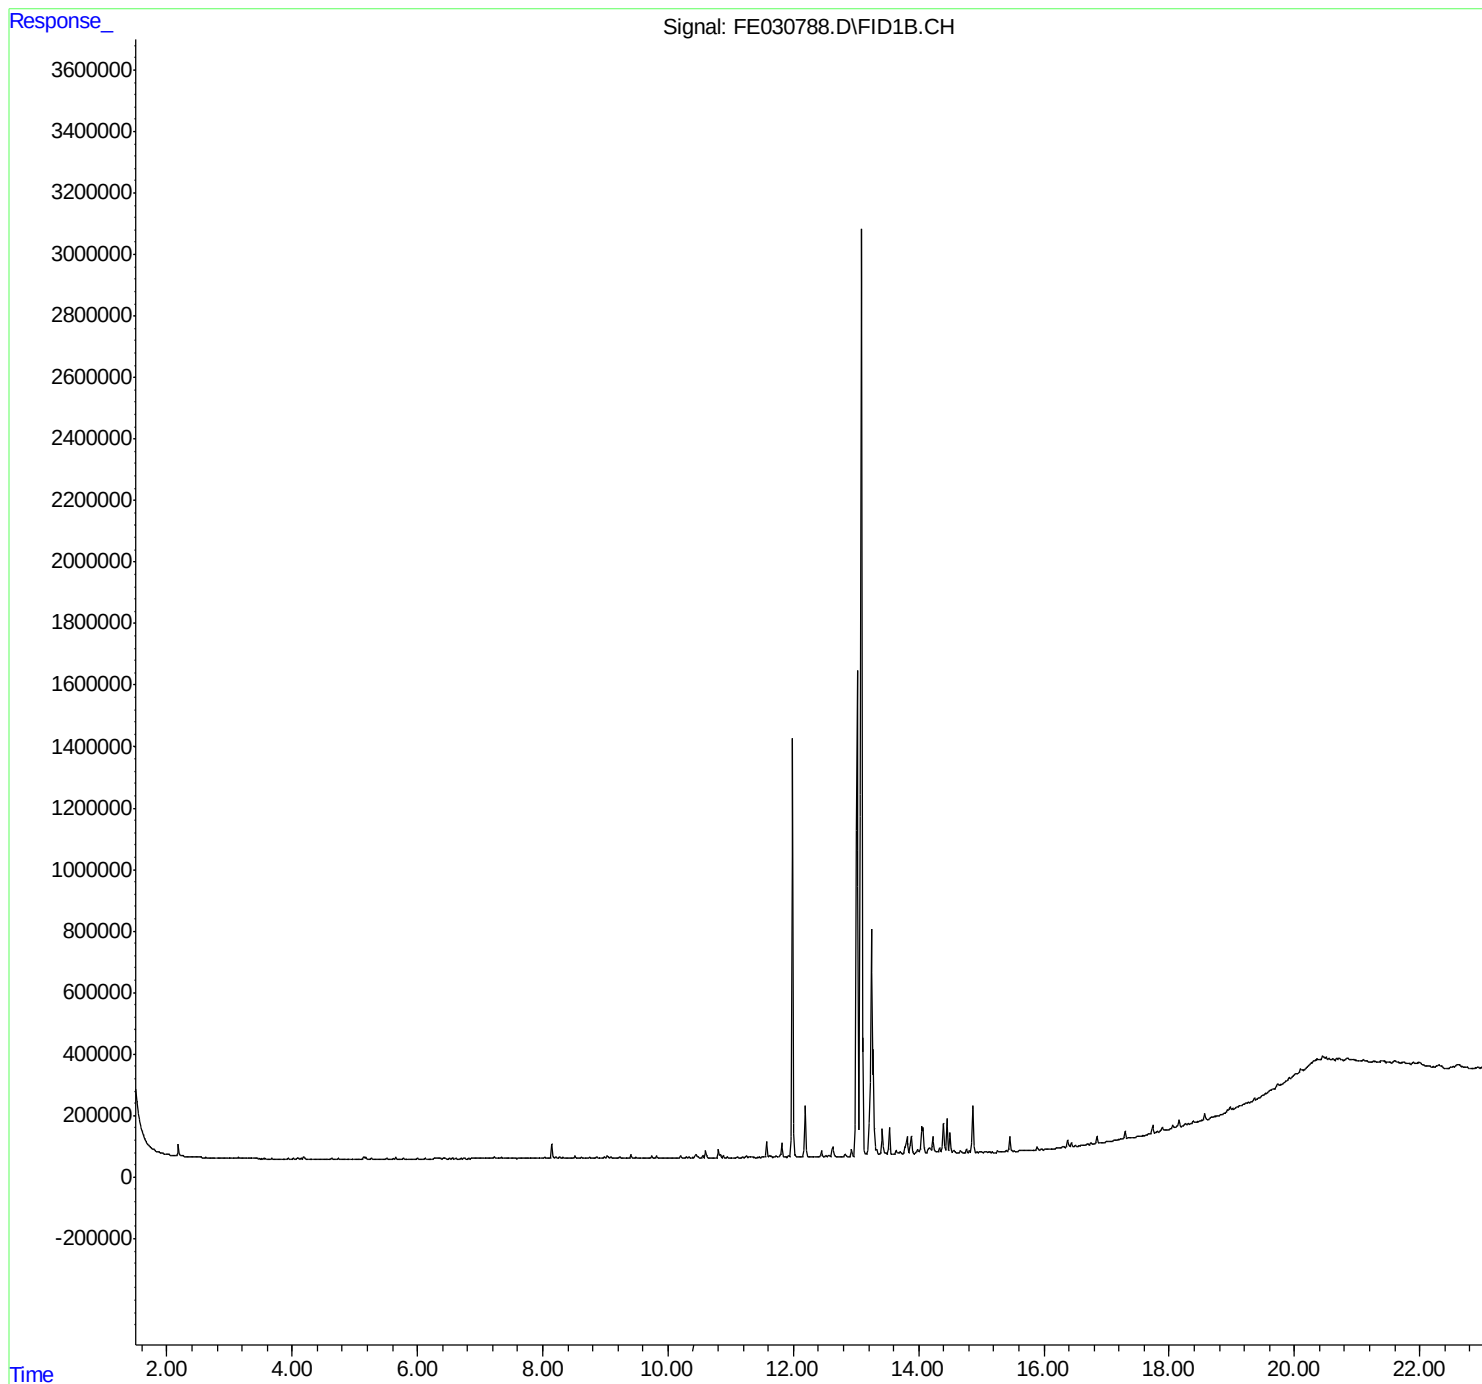

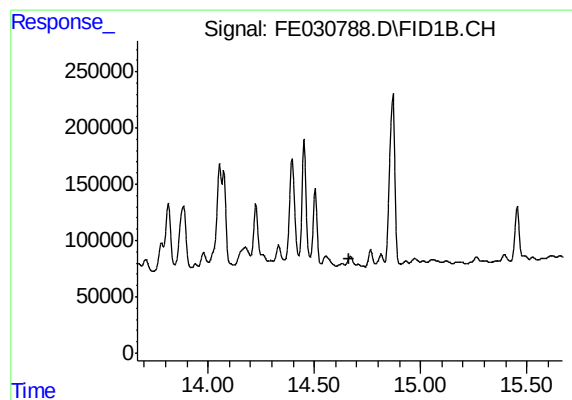

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.667 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
TR-04-110619