

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE110818\  
Data File : FE029061.D  
Signal(s) : FID1B.CH  
Acq On : 07 Nov 2018 13:51  
Operator : DD\SJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Nov 08 09:03:16 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE102518.M  
Quant Title :  
QLast Update : Thu Oct 25 04:58:05 2018  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound | R.T. | Response | Conc Units |
|----------|------|----------|------------|
|----------|------|----------|------------|

-----  
System Monitoring Compounds

Target Compounds

|     |                 |        |         |              |
|-----|-----------------|--------|---------|--------------|
| 3)  | N-DODECANE      | 6.613  | 4168435 | 24.131 ug/ml |
| 12) | N-OCTACOSANE    | 17.074 | 4185622 | 22.955 ug/ml |
| 13) | N-TRIACONTANE   | 17.956 | 204041  | 1.146 ug/ml  |
| 14) | N-DOTRIACONTANE | 18.793 | 196076  | 1.118 ug/ml  |
| 18) | N-TETRACONTANE  | 22.088 | 669452  | 4.159 ug/ml  |


-----  
(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE110818\  
Data File : FE029061.D  
Signal(s) : FID1B.CH  
Acq On : 07 Nov 2018 13:51  
Operator : DD\SJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Nov 08 09:03:16 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE102518.M  
Quant Title :  
QLast Update : Thu Oct 25 04:58:05 2018  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

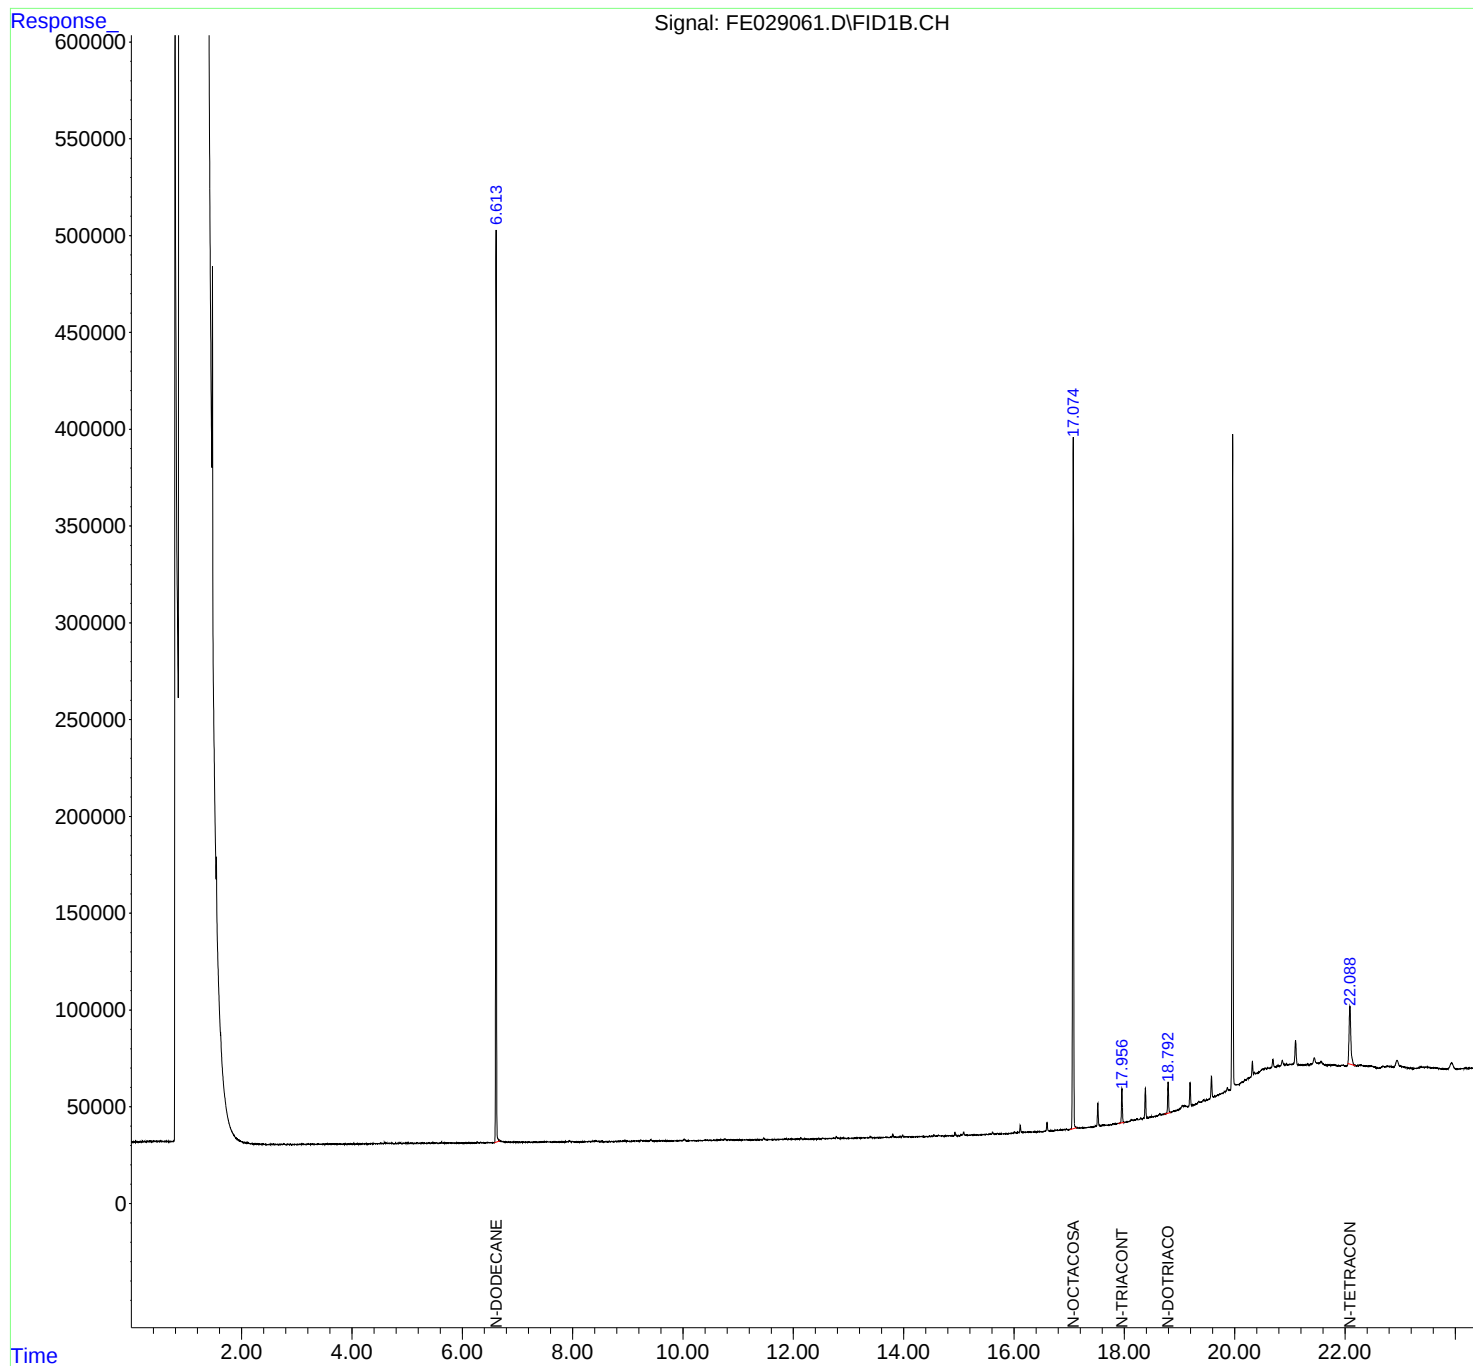

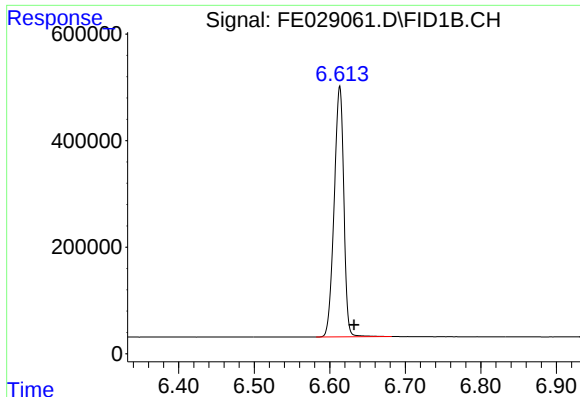


#3 N-DODECANE

R.T.: 6.613 min  
Delta R.T.: -0.019 min  
Response: 4168435  
Conc: 24.13 ug/ml

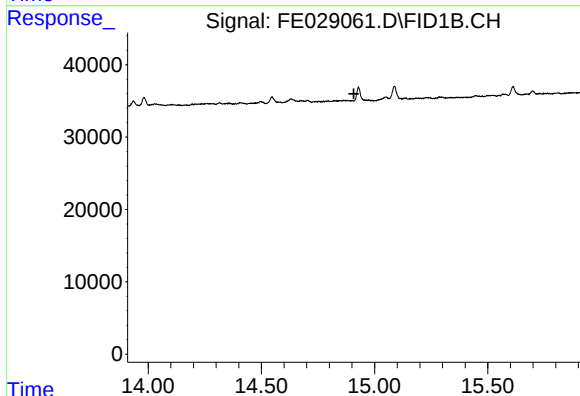


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T.: 14.908 min  
Response: 0  
Conc: N.D.

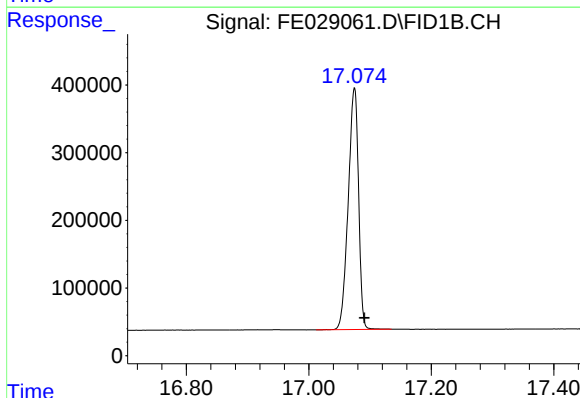


#12 N-OCTACOSANE

R.T.: 17.074 min  
Delta R.T.: -0.016 min  
Response: 4185622  
Conc: 22.95 ug/ml

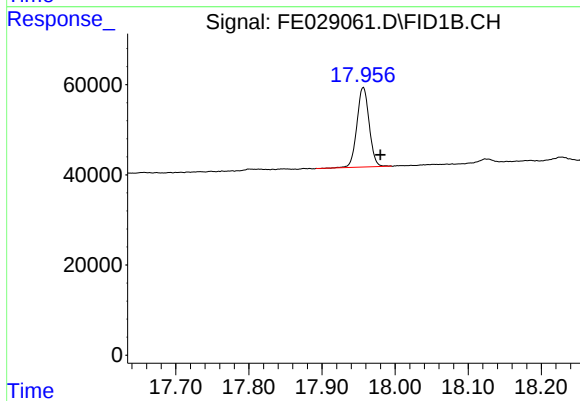


#13 N-TRIACONTANE

R.T.: 17.956 min  
Delta R.T.: -0.024 min  
Response: 204041  
Conc: 1.15 ug/ml

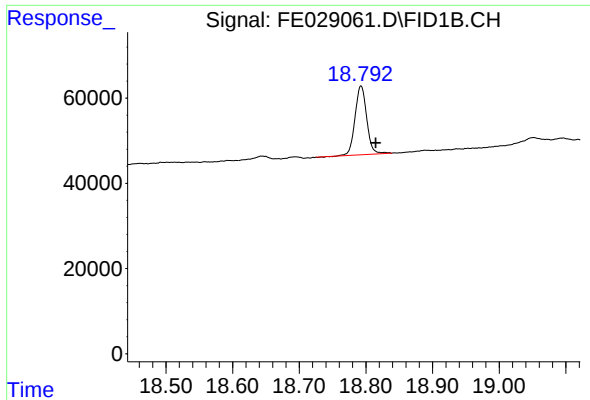

#14 N-DOTRIACONTANE

R.T.: 18.793 min  
Delta R.T.: -0.022 min  
Response: 196076  
Conc: 1.12 ug/ml

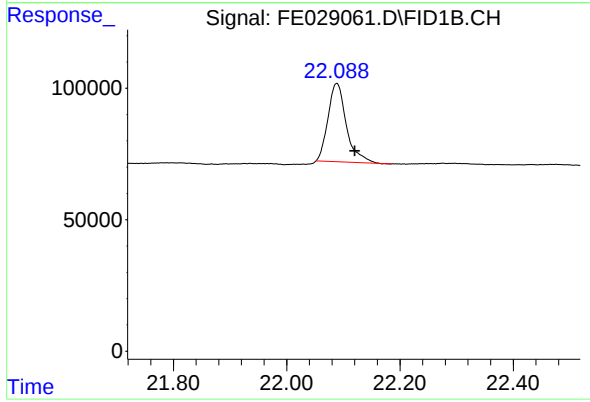

#18 N-TETRACONTANE

R.T.: 22.088 min  
Delta R.T.: -0.032 min  
Response: 669452  
Conc: 4.16 ug/ml