

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110819\
 Data File : FE030795.D
 Signal(s) : FID1B.CH
 Acq On : 08 Nov 2019 8:49
 Operator : DD\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 MECL2

Integration File: autoint1.e
 Quant Time: Nov 08 23:30:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
 Quant Title :
 QLast Update : Thu Oct 31 08:47:02 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) N-DOTRIACONTANE	18.584	181263	0.568 ug/ml
15) N-TETRATRIACONTANE	19.300	1561343	5.128 ug/ml
16) N-HEXATRIACONTANE	20.113	2264838	8.249 ug/ml
17) N-OCTATRIACONTANE	20.812	2366775	9.360 ug/ml
18) N-TETRACONTANE	21.763	537320	2.045 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110819\
Data File : FE030795.D
Signal(s) : FID1B.CH
Acq On : 08 Nov 2019 8:49
Operator : DD\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Nov 08 23:30:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
Quant Title :
QLast Update : Thu Oct 31 08:47:02 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

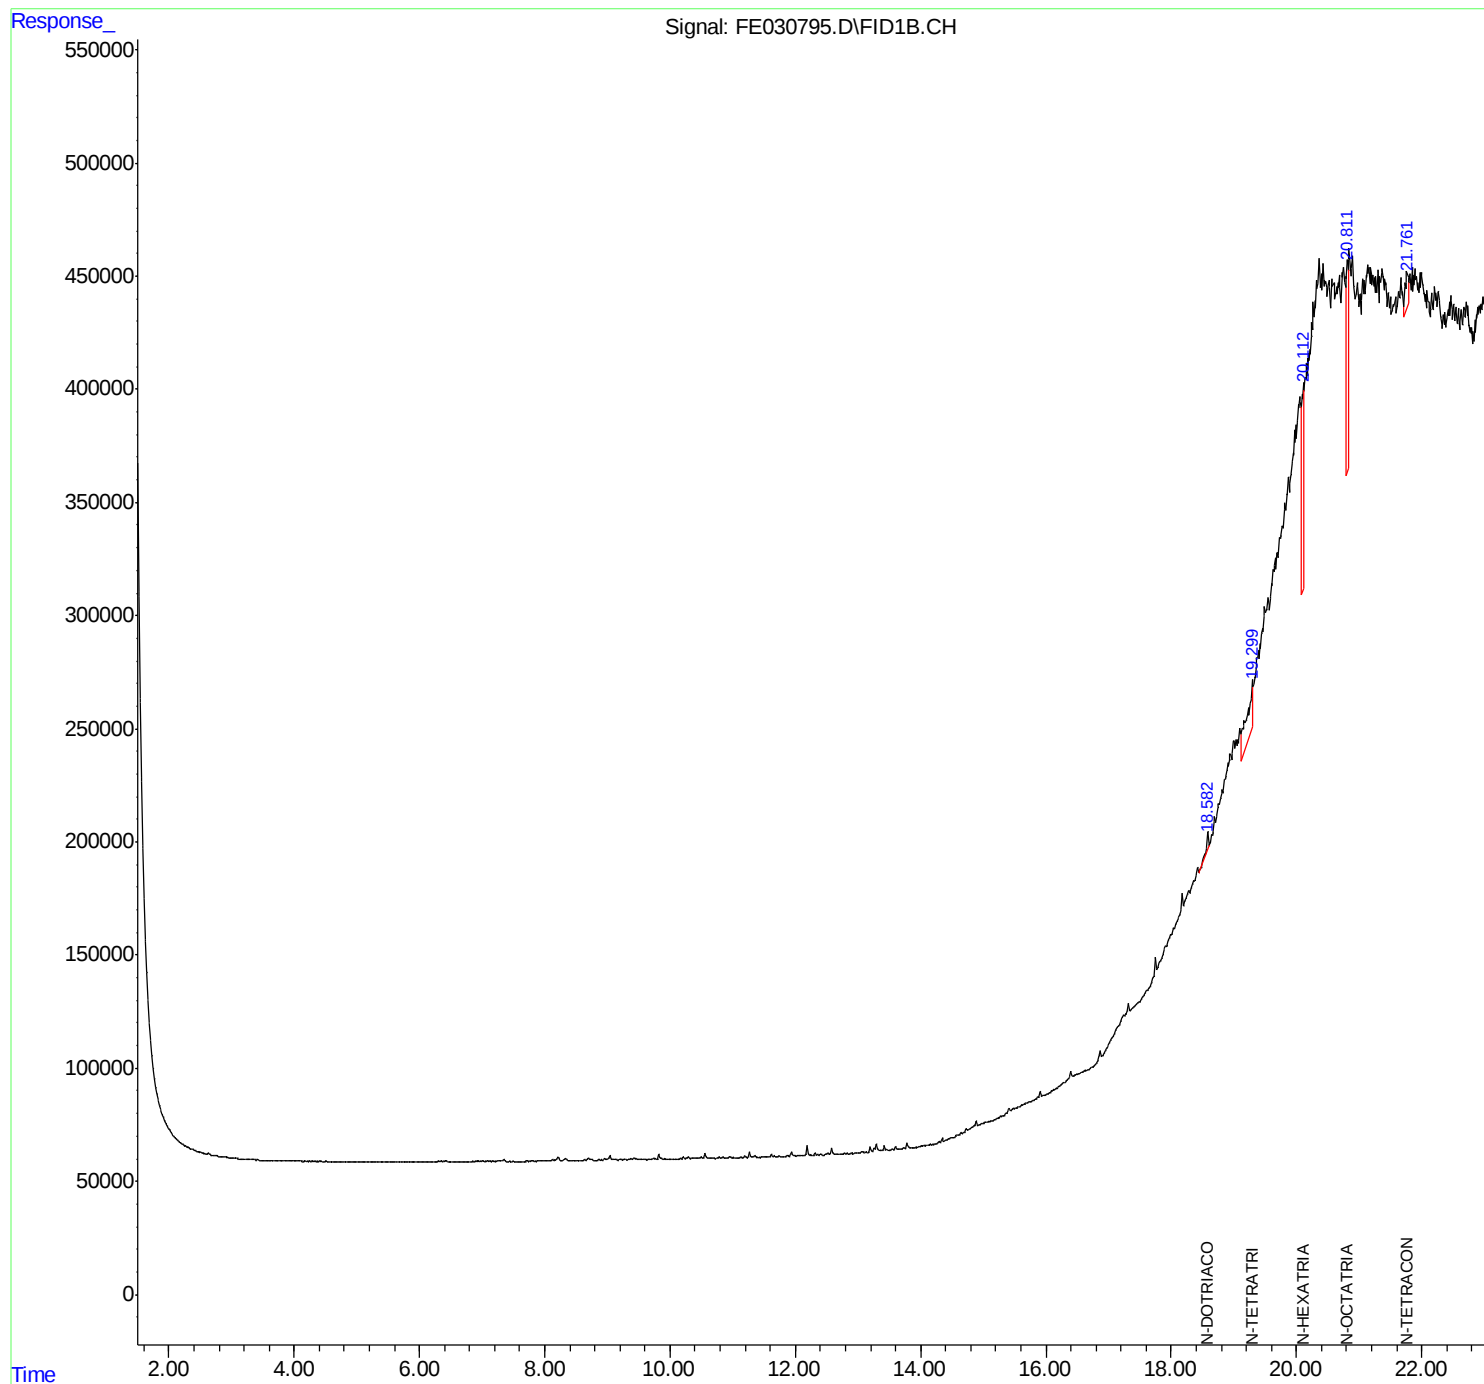


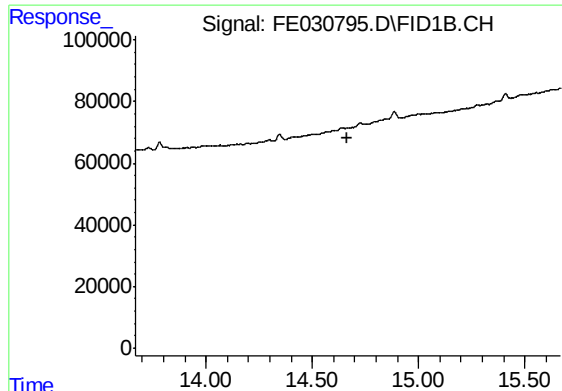

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.667 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
MECL2

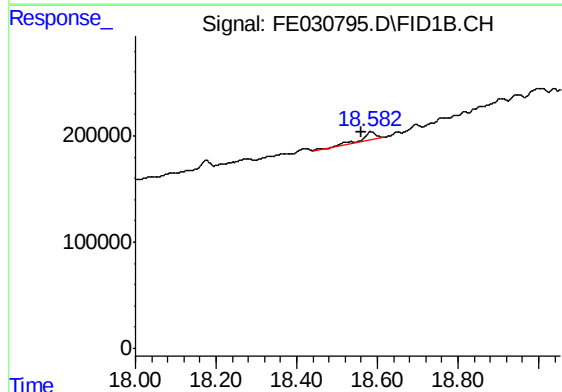


#14 N-DOTRIACONTANE

R.T.: 18.584 min
Delta R.T.: 0.023 min
Response: 181263
Conc: 0.57 ug/ml

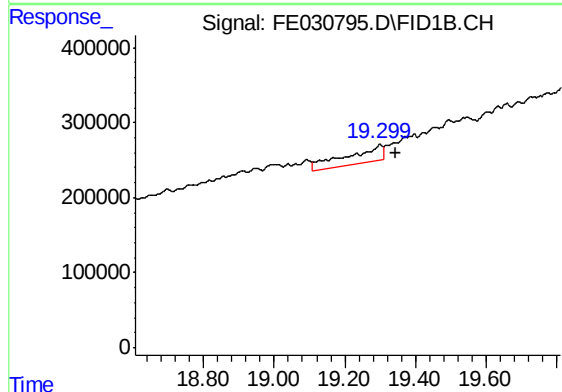


#15 N-TETRATRIACONTANE

R.T.: 19.300 min
Delta R.T.: -0.044 min
Response: 1561343
Conc: 5.13 ug/ml

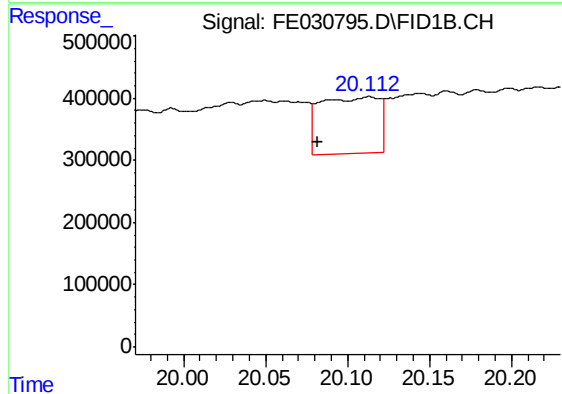

#16 N-HEXATRIACONTANE


R.T.: 20.113 min
Delta R.T.: 0.032 min
Response: 2264838
Conc: 8.25 ug/ml

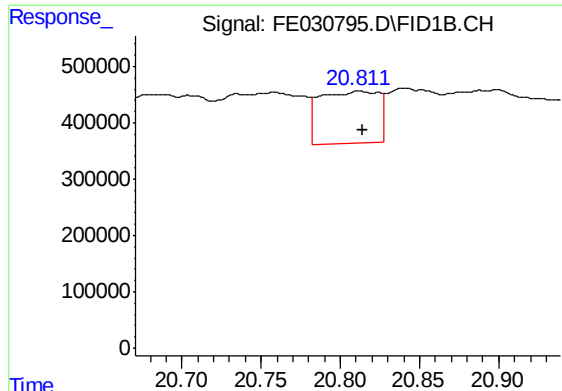

#17 N-OCTATRIACONTANE

R.T.: 20.812 min
Delta R.T.: -0.002 min
Response: 2366775
Conc: 9.36 ug/ml

Instrument :
FID_E
ClientSampleId :
MECL2

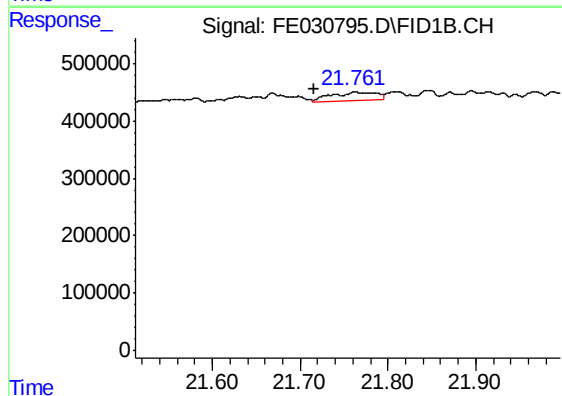

#18 N-TETRACONTANE

R.T.: 21.763 min
Delta R.T.: 0.047 min
Response: 537320
Conc: 2.05 ug/ml