

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110819\
 Data File : FE030807.D
 Signal(s) : FID1B.CH
 Acq On : 08 Nov 2019 18:31
 Operator : DD\AJ
 Sample : PB124648BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 PB124648BL

Integration File: autoint1.e
 Quant Time: Nov 08 23:52:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
 Quant Title :
 QLast Update : Thu Oct 31 08:47:02 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
2) N-DECANE	4.400	7015181	18.437 ug/ml
3) N-DODECANE	6.412	7345026	19.304 ug/ml
4) N-TETRADECANE	8.208	7590474	20.270 ug/ml
5) N-HEXADECANE	9.811	7864125	21.085 ug/ml
6) N-OCTADECANE	11.256	8269501	22.617 ug/ml
7) N-EICOSANE	12.568	8416598	23.030 ug/ml
8) N-DOCOSANE	13.769	8319010	23.141 ug/ml
10) N-TETRACOSANE	14.874	8199309	23.051 ug/ml
11) N-HEXACOSANE	15.896	8076929	23.160 ug/ml
12) N-OCTACOSANE	16.847	8060932	23.644 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE110819\
Data File : FE030807.D
Signal(s) : FID1B.CH
Acq On : 08 Nov 2019 18:31
Operator : DD\AJ
Sample : PB124648BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB124648BL

Integration File: autoint1.e
Quant Time: Nov 08 23:52:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
Quant Title :
QLast Update : Thu Oct 31 08:47:02 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

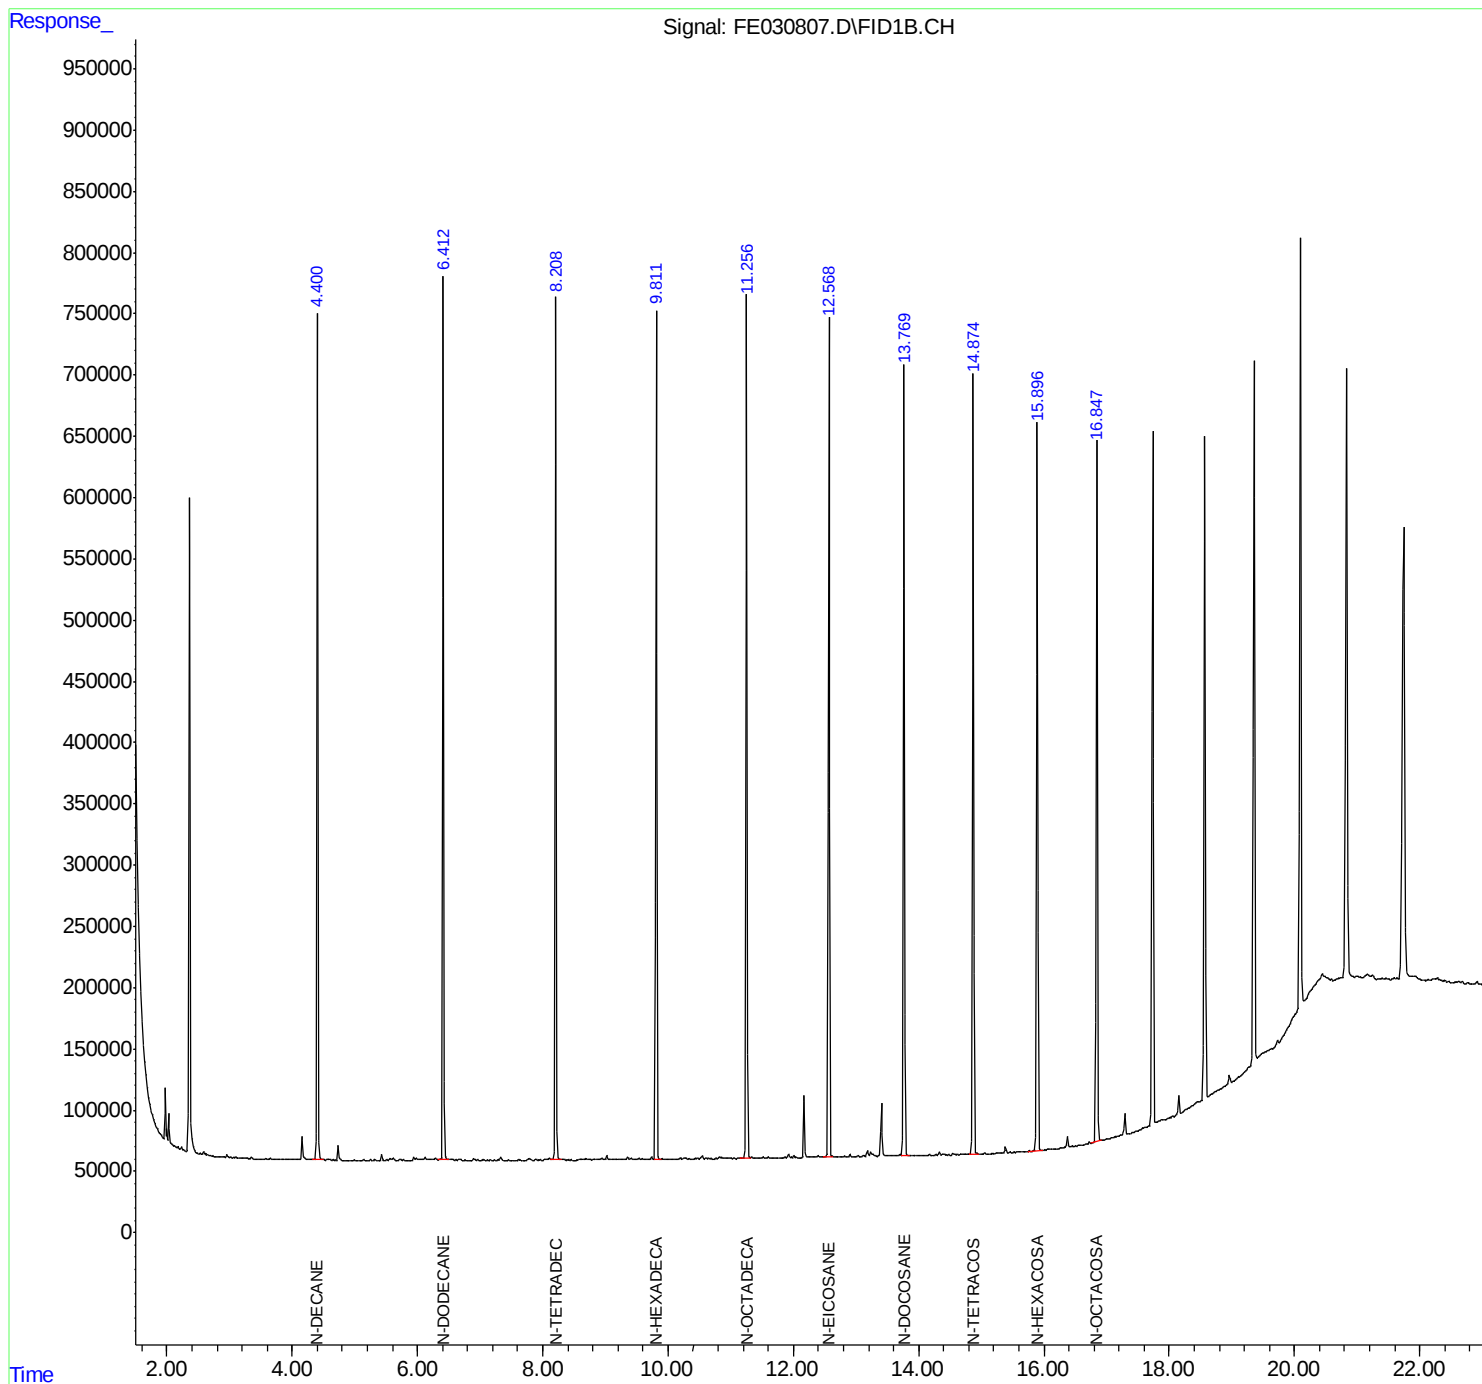


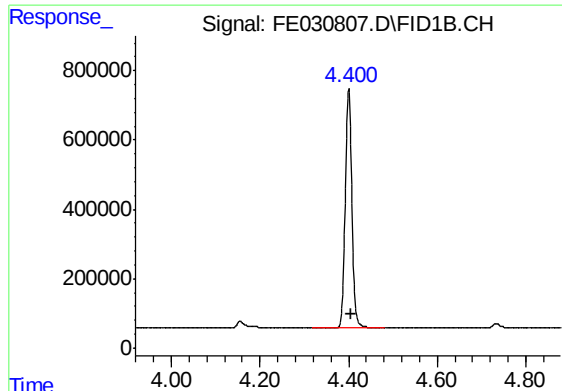

#2 N-DECANE


R.T.: 4.400 min
Delta R.T.: -0.004 min
Response: 7015181
Conc: 18.44 ug/ml

Instrument :
FID_E
ClientSampleId :
PB124648BL

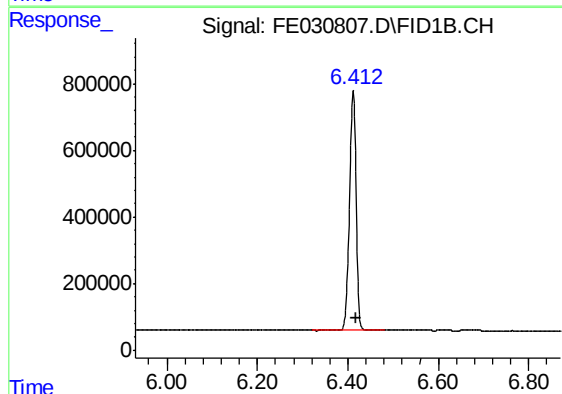


#3 N-DODECANE

R.T.: 6.412 min
Delta R.T.: -0.007 min
Response: 7345026
Conc: 19.30 ug/ml

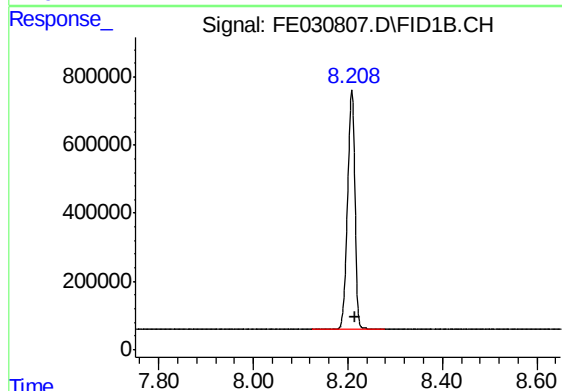


#4 N-TETRADECANE

R.T.: 8.208 min
Delta R.T.: -0.006 min
Response: 7590474
Conc: 20.27 ug/ml

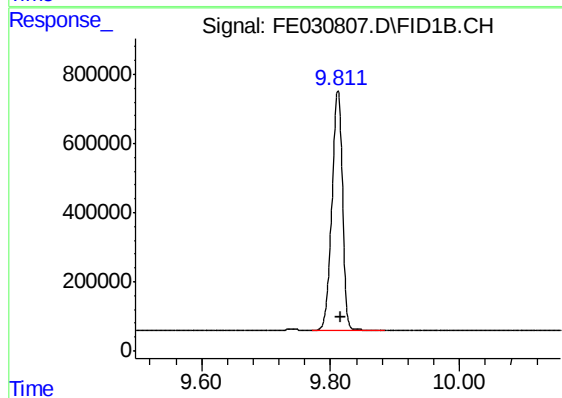

#5 N-HEXADECANE


R.T.: 9.811 min
Delta R.T.: -0.005 min
Response: 7864125
Conc: 21.09 ug/ml

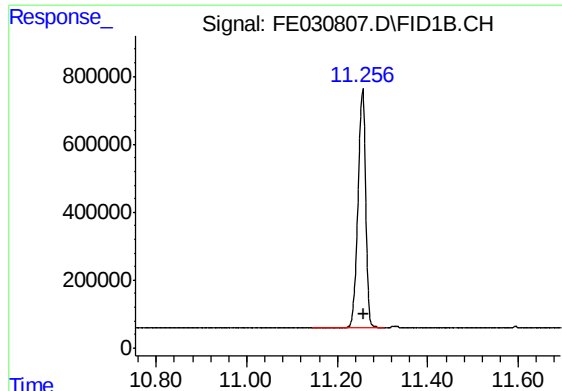

#6 N-OCTADECANE


R.T.: 11.256 min
Delta R.T.: -0.004 min
Response: 8269501
Conc: 22.62 ug/ml

Instrument :
FID_E
ClientSampleId :
PB124648BL

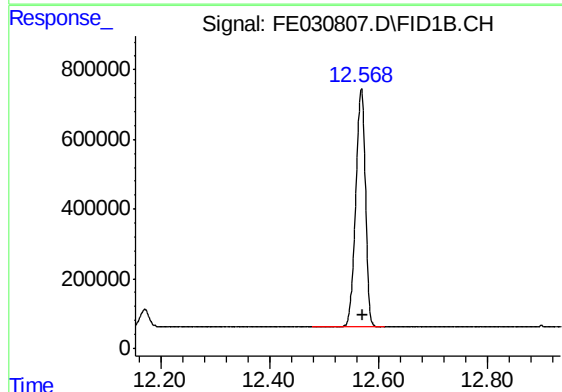


#7 N-EICOSANE

R.T.: 12.568 min
Delta R.T.: -0.002 min
Response: 8416598
Conc: 23.03 ug/ml

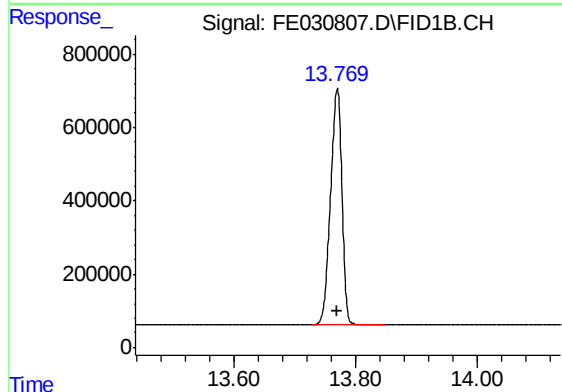


#8 N-DOCOSANE

R.T.: 13.769 min
Delta R.T.: 0.000 min
Response: 8319010
Conc: 23.14 ug/ml

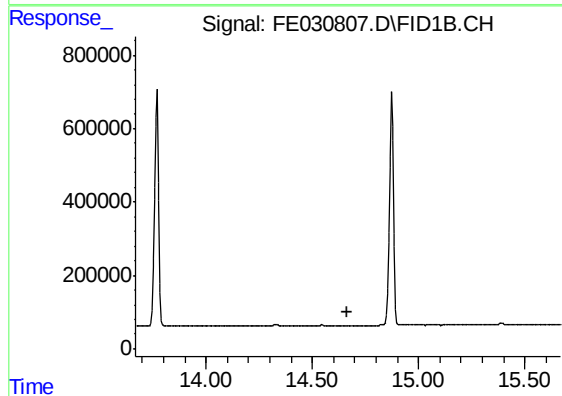

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T. : 14.667 min
Response: 0
Conc: N.D.

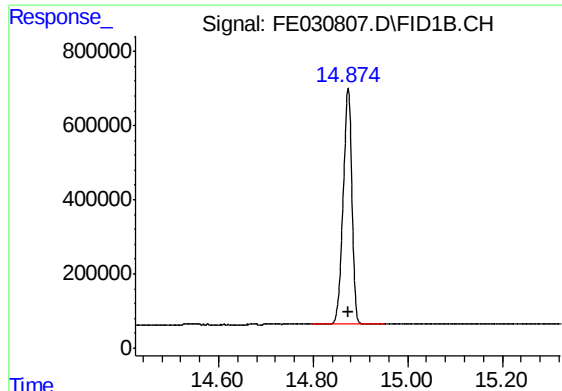

#10 N-TETRACOSANE


R.T.: 14.874 min
Delta R.T.: 0.000 min
Response: 8199309
Conc: 23.05 ug/ml

Instrument :
FID_E
ClientSampleId :
PB124648BL

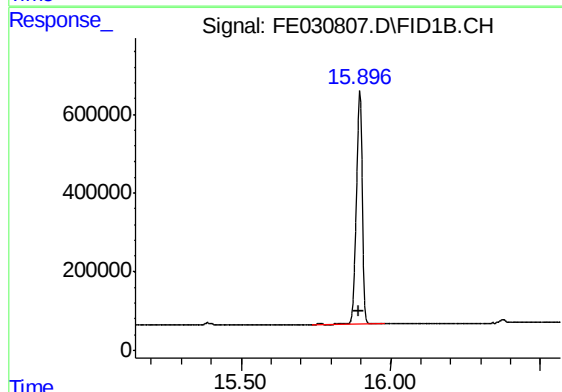

#11 N-HEXACOSANE

R.T.: 15.896 min
Delta R.T.: 0.002 min
Response: 8076929
Conc: 23.16 ug/ml

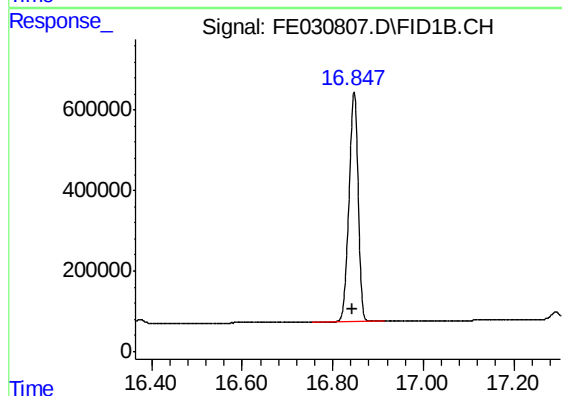

#12 N-OCTACOSANE

R.T.: 16.847 min
Delta R.T.: 0.004 min
Response: 8060932
Conc: 23.64 ug/ml