

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE110922AL\  
 Data File : FE038667.D  
 Signal(s) : FID1B.ch  
 Acq On : 09 Nov 2022 13:17  
 Operator : YP\AJ  
 Sample : N5505-01DL 5X  
 Misc :  
 ALS Vial : 11 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 HD-2-110722DL

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 11/10/2022  
 Supervised By :Ankita Jodhani 11/10/2022

Integration File: autoint1.e  
 Quant Time: Nov 10 04:54:51 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_D\methods\Aliphatic EPH 102522.M  
 Quant Title : GC Extractables  
 QLast Update : Wed Oct 26 04:49:29 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response | Conc Units     |
|--------------------------------|--------|----------|----------------|
| -----                          |        |          |                |
| System Monitoring Compounds    |        |          |                |
| 9) S ortho-Terphenyl (SURR)    | 11.962 | 791567   | 4.600 ug/mlm   |
| Spiked Amount                  | 50.000 | Recovery | = 9.20%        |
| 12) S 1-chlorooctadecane (S... | 13.395 | 24371911 | 178.025 ug/mlm |
| Spiked Amount                  | 50.000 | Recovery | = 356.05%      |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE110922AL\  
Data File : FE038667.D  
Signal(s) : FID1B.ch  
Acq On : 09 Nov 2022 13:17  
Operator : YP\AJ  
Sample : N5505-01DL 5X  
Misc :  
ALS Vial : 11 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
HD-2-110722DL


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 11/10/2022  
Supervised By :Ankita Jodhani 11/10/2022

Integration File: autoint1.e  
Quant Time: Nov 10 04:54:51 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_D\methods\Aliphatic EPH 102522.M  
Quant Title : GC Extractables  
QLast Update : Wed Oct 26 04:49:29 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

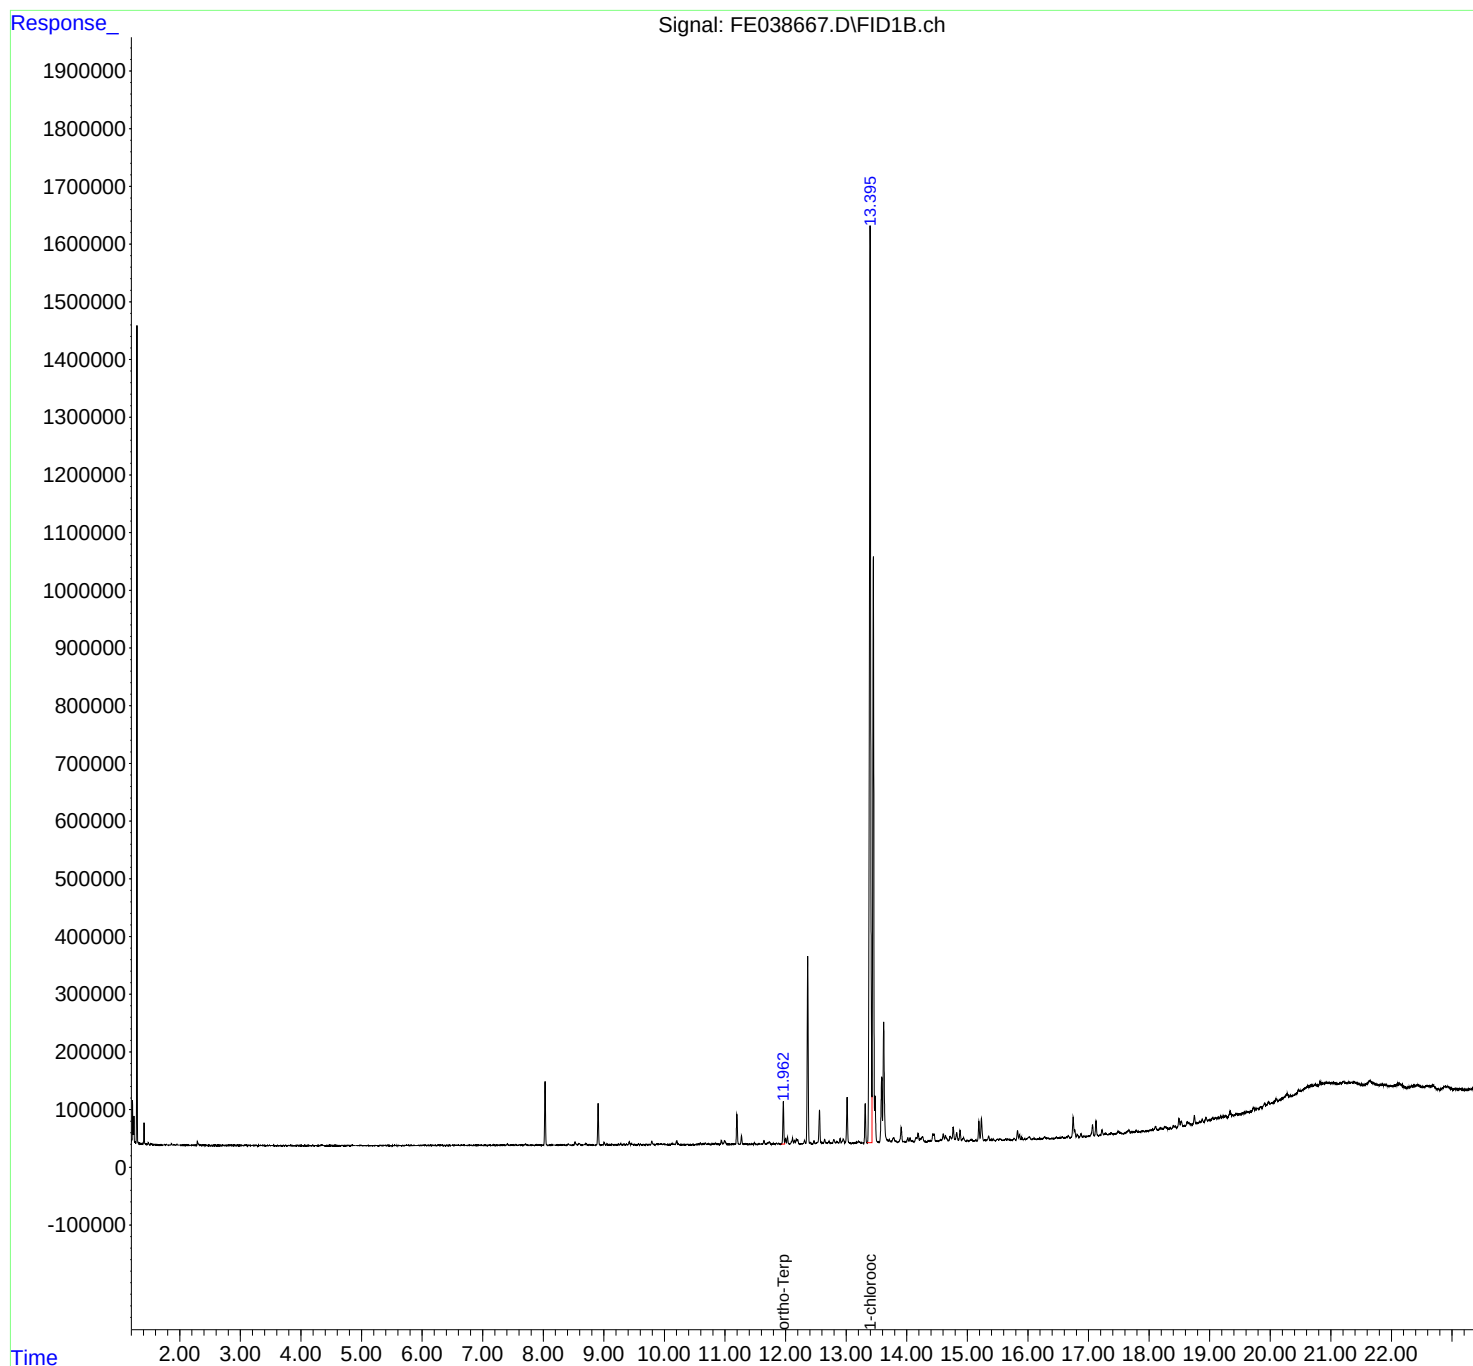

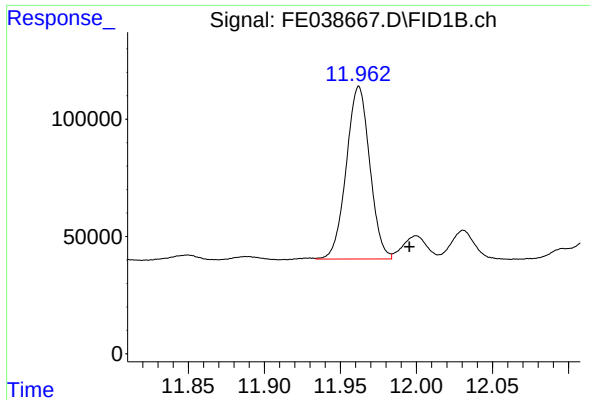


#9 ortho-Terphenyl (SURR)

R.T.: 11.962 min  
Delta R.T.: -0.034 min  
Response: 791567  
Conc: 4.60 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
HD-2-110722DL

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 11/10/2022  
Supervised By :Ankita Jodhani 11/10/2022

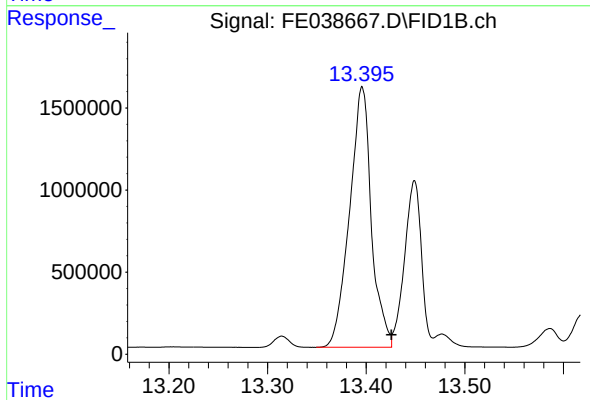

#12 1-chlorooctadecane (SURR)

R.T.: 13.395 min  
Delta R.T.: -0.030 min  
Response: 24371911  
Conc: 178.03 ug/ml m