

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE110924AL\  
 Data File : FE051110.D  
 Signal(s) : FID1B.ch  
 Acq On : 08 Nov 2024 09:36  
 Operator : YP\AJ  
 Sample : P4734-01DL 5X  
 Misc :  
 ALS Vial : 14 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 EO-03-11062024DL

Integration File: sample.E  
 Quant Time: Nov 08 12:09:54 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 110724.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Nov 07 04:56:04 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 9) S ortho-Terphenyl (SURR)    | 11.853 | 1030034    | 6.863 ug/ml  |
| Spiked Amount 50.000           |        | Recovery = | 13.73%       |
| 12) S 1-chlorooctadecane (S... | 13.276 | 3038156    | 26.761 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 53.52%       |

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE110924AL\  
Data File : FE051110.D  
Signal(s) : FID1B.ch  
Acq On : 08 Nov 2024 09:36  
Operator : YP\AJ  
Sample : P4734-01DL 5X  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
EO-03-11062024DL

Integration File: sample.E  
Quant Time: Nov 08 12:09:54 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 110724.M  
Quant Title : GC Extractables  
QLast Update : Thu Nov 07 04:56:04 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 uL  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

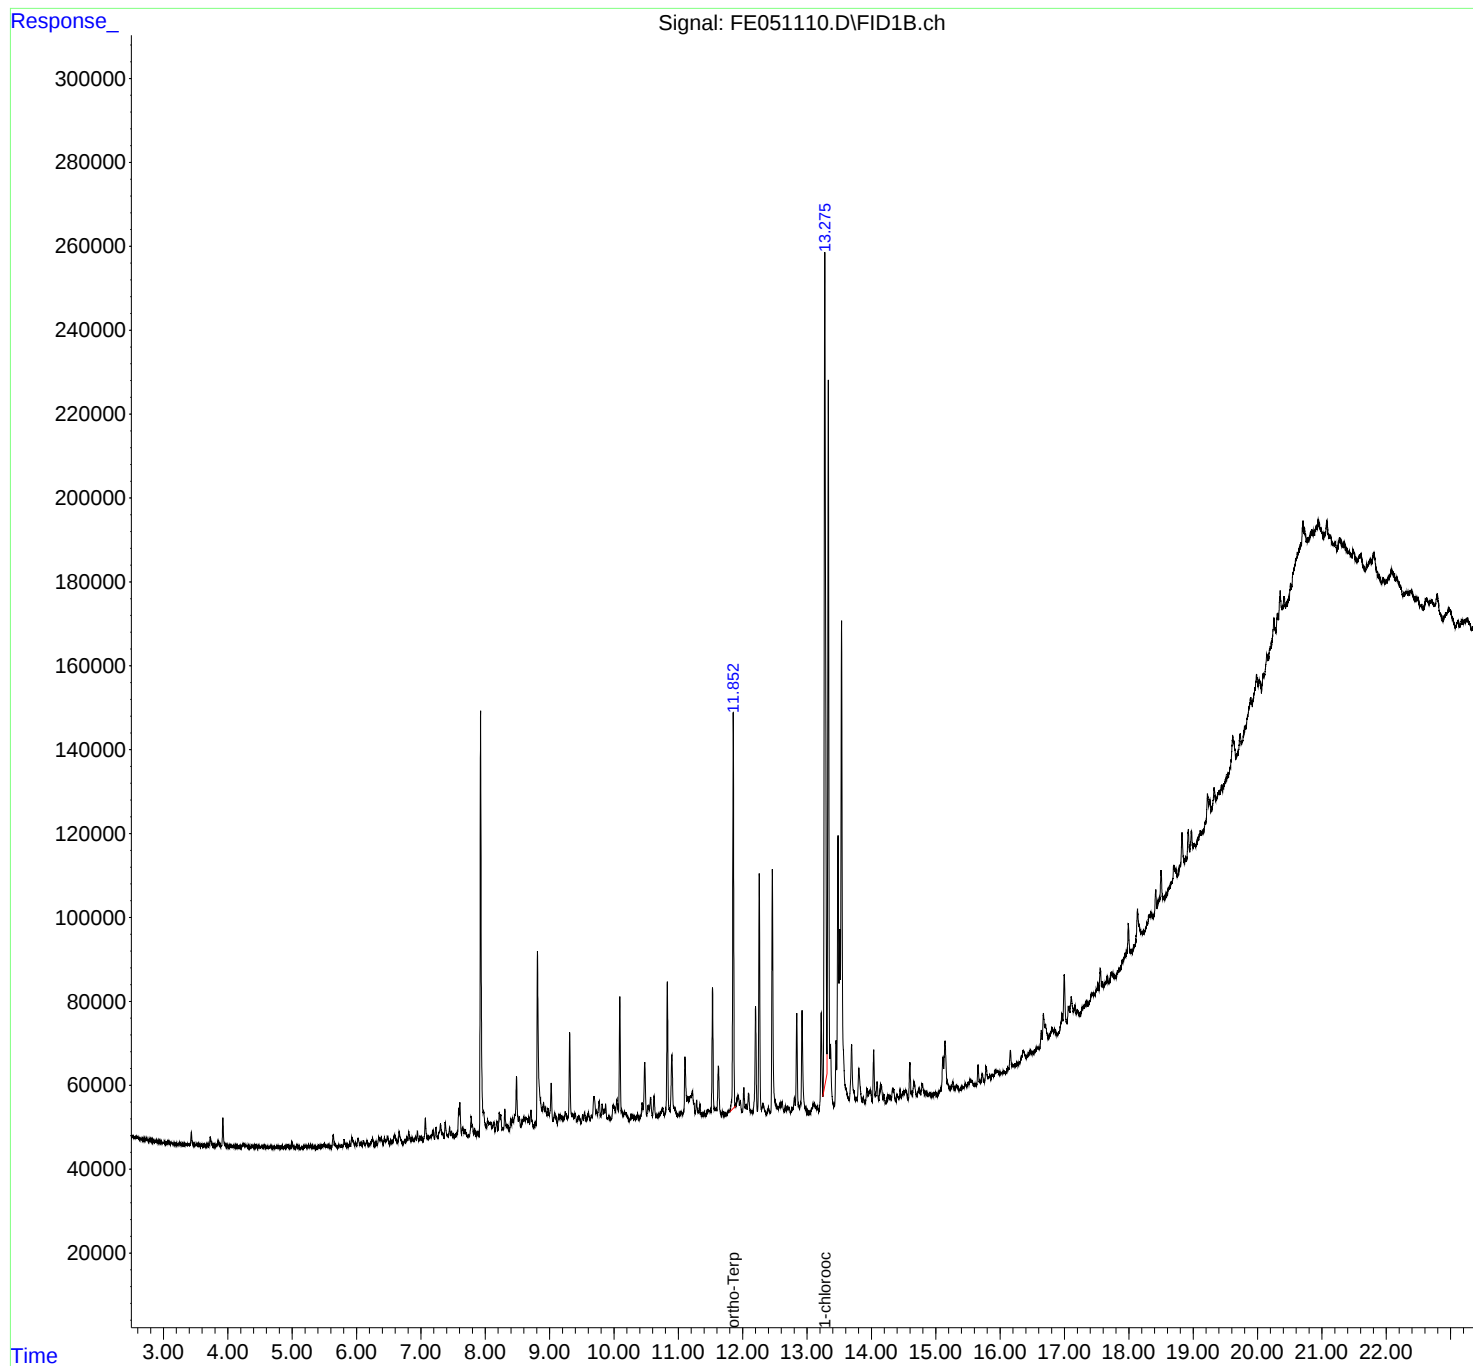


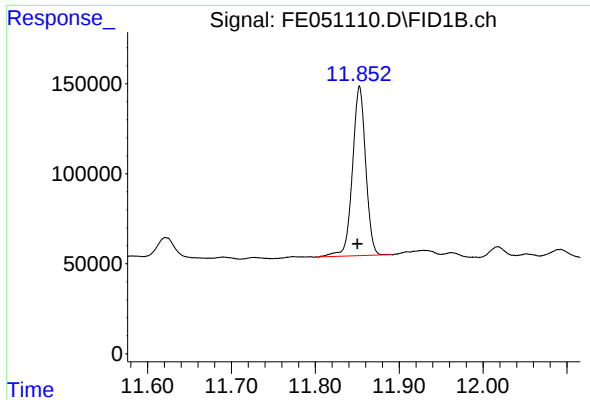

#9 ortho-Terphenyl (SURR)

R.T.: 11.853 min  
Delta R.T.: 0.002 min  
Response: 1030034  
Conc: 6.86 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
EO-03-11062024DL

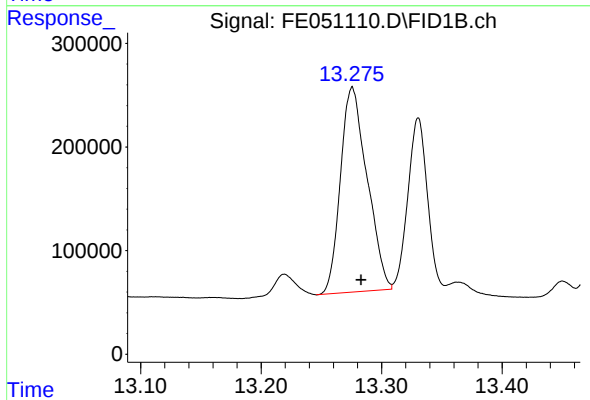

#12 1-chlorooctadecane (SURR)

R.T.: 13.276 min  
Delta R.T.: -0.007 min  
Response: 3038156  
Conc: 26.76 ug/ml