

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE111022AL\  
 Data File : FE038720.D  
 Signal(s) : FID1B.ch  
 Acq On : 10 Nov 2022 19:50  
 Operator : YP\AJ  
 Sample : N5520-01  
 Misc :  
 ALS Vial : 22 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 124035

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 11/11/2022  
 Supervised By :Ankita Jodhani 11/11/2022

Integration File: autoint1.e  
 Quant Time: Nov 11 03:46:49 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_D\methods\Aliphatic EPH 102522.M  
 Quant Title : GC Extractables  
 QLast Update : Wed Oct 26 04:49:29 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units    |
|--------------------------------|--------|------------|---------------|
| -----                          |        |            |               |
| System Monitoring Compounds    |        |            |               |
| 9) S ortho-Terphenyl (SURR)    | 11.961 | 3581122    | 20.812 ug/ml  |
| Spiked Amount 50.000           |        | Recovery = | 41.62%        |
| 12) S 1-chlorooctadecane (S... | 13.394 | 3112507    | 22.735 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 45.47%        |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE111022AL\  
Data File : FE038720.D  
Signal(s) : FID1B.ch  
Acq On : 10 Nov 2022 19:50  
Operator : YP\AJ  
Sample : N5520-01  
Misc :  
ALS Vial : 22 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
124035


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 11/11/2022  
Supervised By :Ankita Jodhani 11/11/2022

Integration File: autoint1.e  
Quant Time: Nov 11 03:46:49 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_D\methods\Aliphatic EPH 102522.M  
Quant Title : GC Extractables  
QLast Update : Wed Oct 26 04:49:29 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

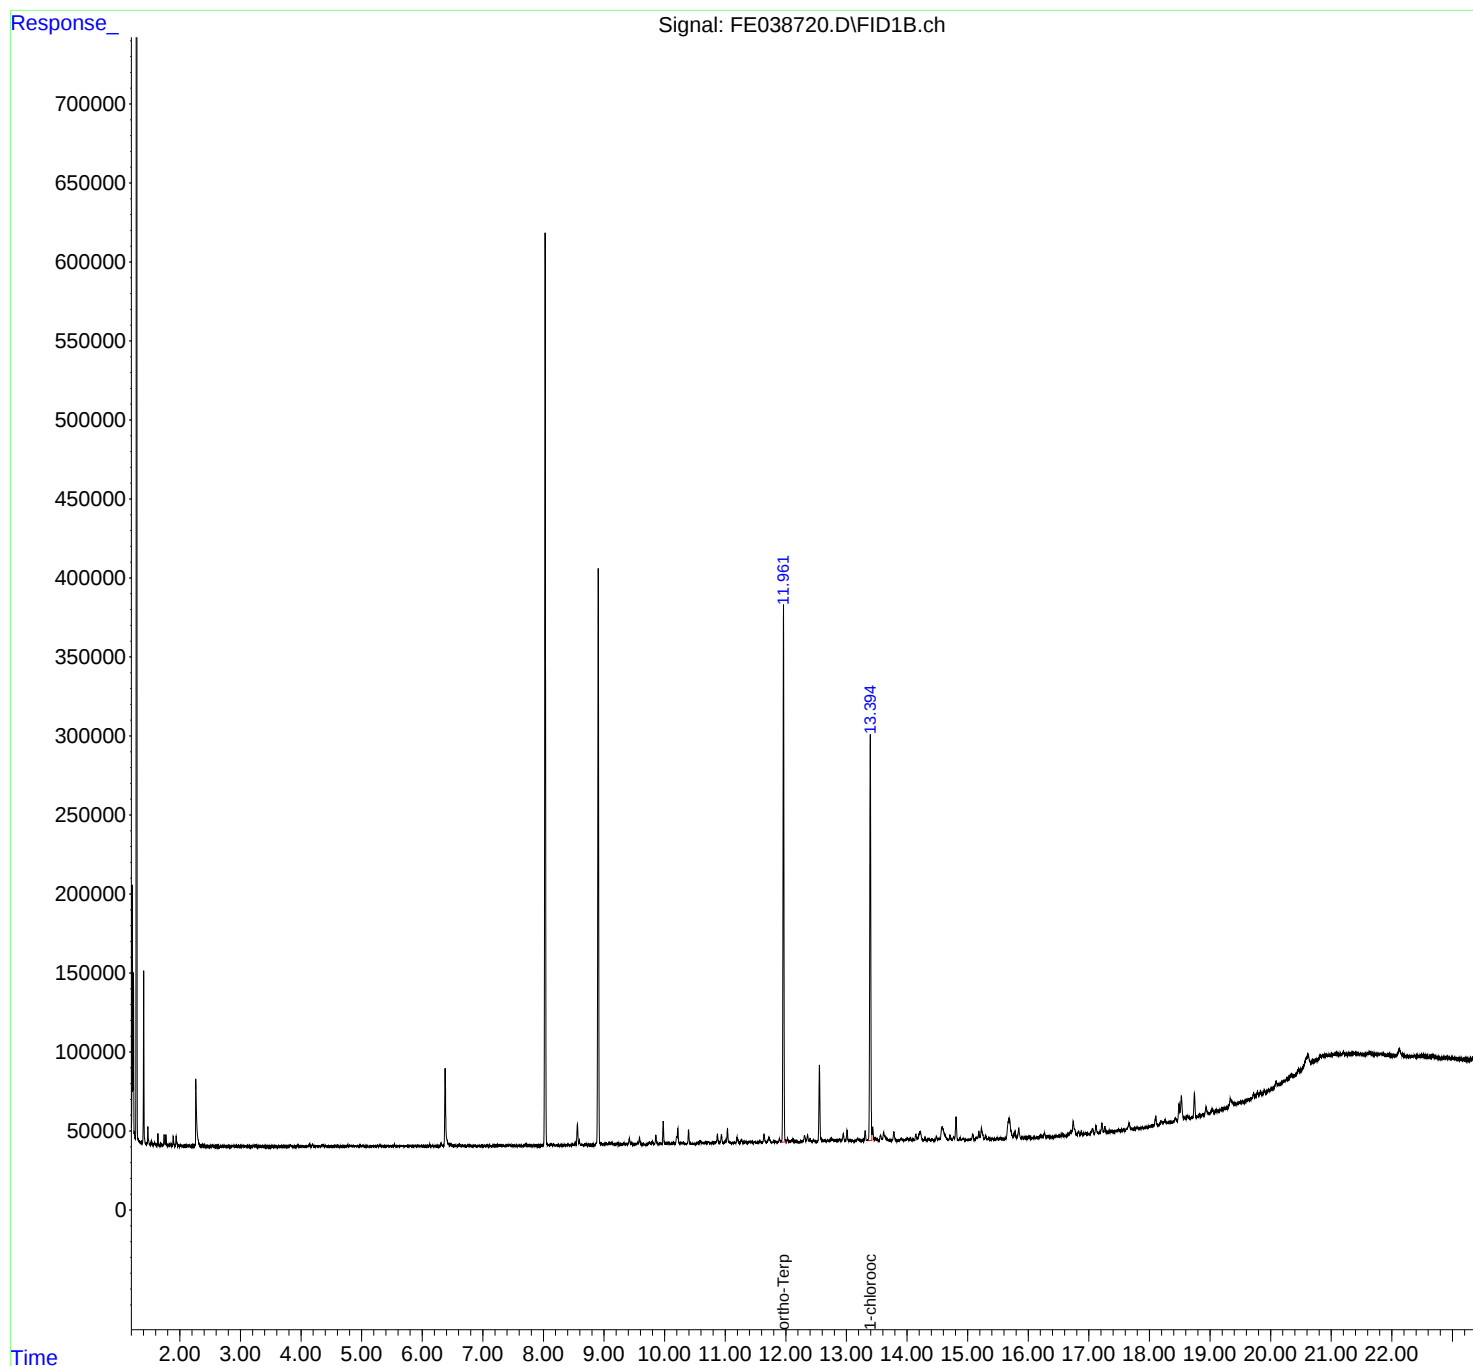

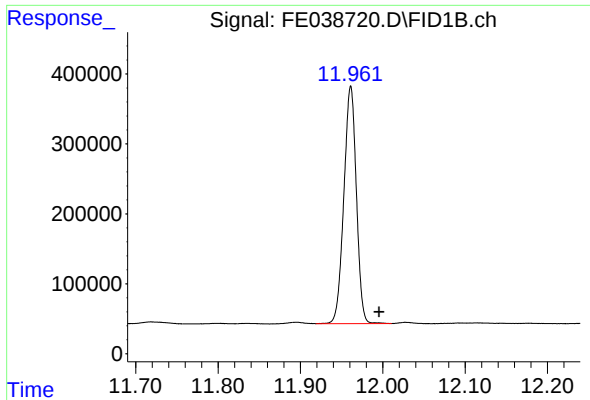


#9 ortho-Terphenyl (SURR)

R.T.: 11.961 min  
Delta R.T.: -0.034 min  
Response: 3581122  
Conc: 20.81 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
124035

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 11/11/2022  
Supervised By :Ankita Jodhani 11/11/2022

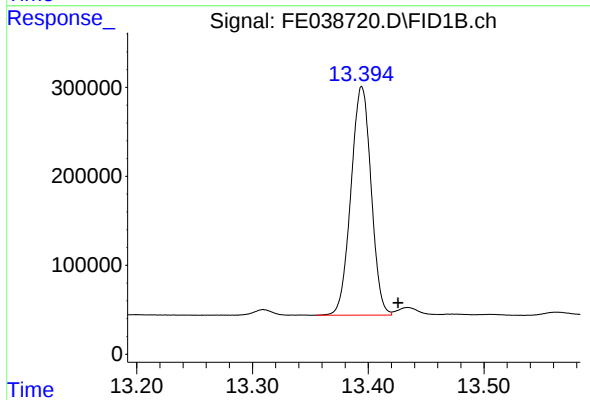

#12 1-chlorooctadecane (SURR)

R.T.: 13.394 min  
Delta R.T.: -0.032 min  
Response: 3112507  
Conc: 22.74 ug/ml m