

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB111025\  
Data File : FB032335.D  
Signal(s) : FID2B.CH  
Acq On : 10 Nov 2025 9:13  
Operator : YP/AJ  
Sample : VBF1110W1  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Nov 11 03:37:43 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB102725.M  
Quant Title :  
QLast Update : Tue Oct 28 04:57:39 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

| Compound                     | R.T.   | Response | Conc Units   |
|------------------------------|--------|----------|--------------|
| -----                        |        |          |              |
| System Monitoring Compounds  |        |          |              |
| 5) s AAA-TFT                 | 8.798  | 395890   | 19.519 ng/ml |
| Target Compounds             |        |          |              |
| 6) t Toluene                 | 10.627 | 10322    | 0.288 ng/ml  |
| 8) t m-Xylene                | 13.194 | 8978     | 0.270 ng/ml  |
| 9) t O-Xylene                | 13.927 | 8414     | 0.262 ng/ml  |
| 10) t 1,2,4-Trimethylbenzene | 16.201 | 16049    | 0.580 ng/ml  |
| -----                        |        |          |              |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_B\Data\FB111025\  
Data File : FB032335.D  
Signal(s) : FID2B.CH  
Acq On : 10 Nov 2025 9:13  
Operator : YP/AJ  
Sample : VBF1110W1  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: Calibration.e  
Quant Time: Nov 11 03:37:43 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_B\Method\FB102725.M  
Quant Title :  
QLast Update : Tue Oct 28 04:57:39 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 5 g/ml  
Signal Phase : RTX-502.2  
Signal Info : 60mx0.53mmx3.00um

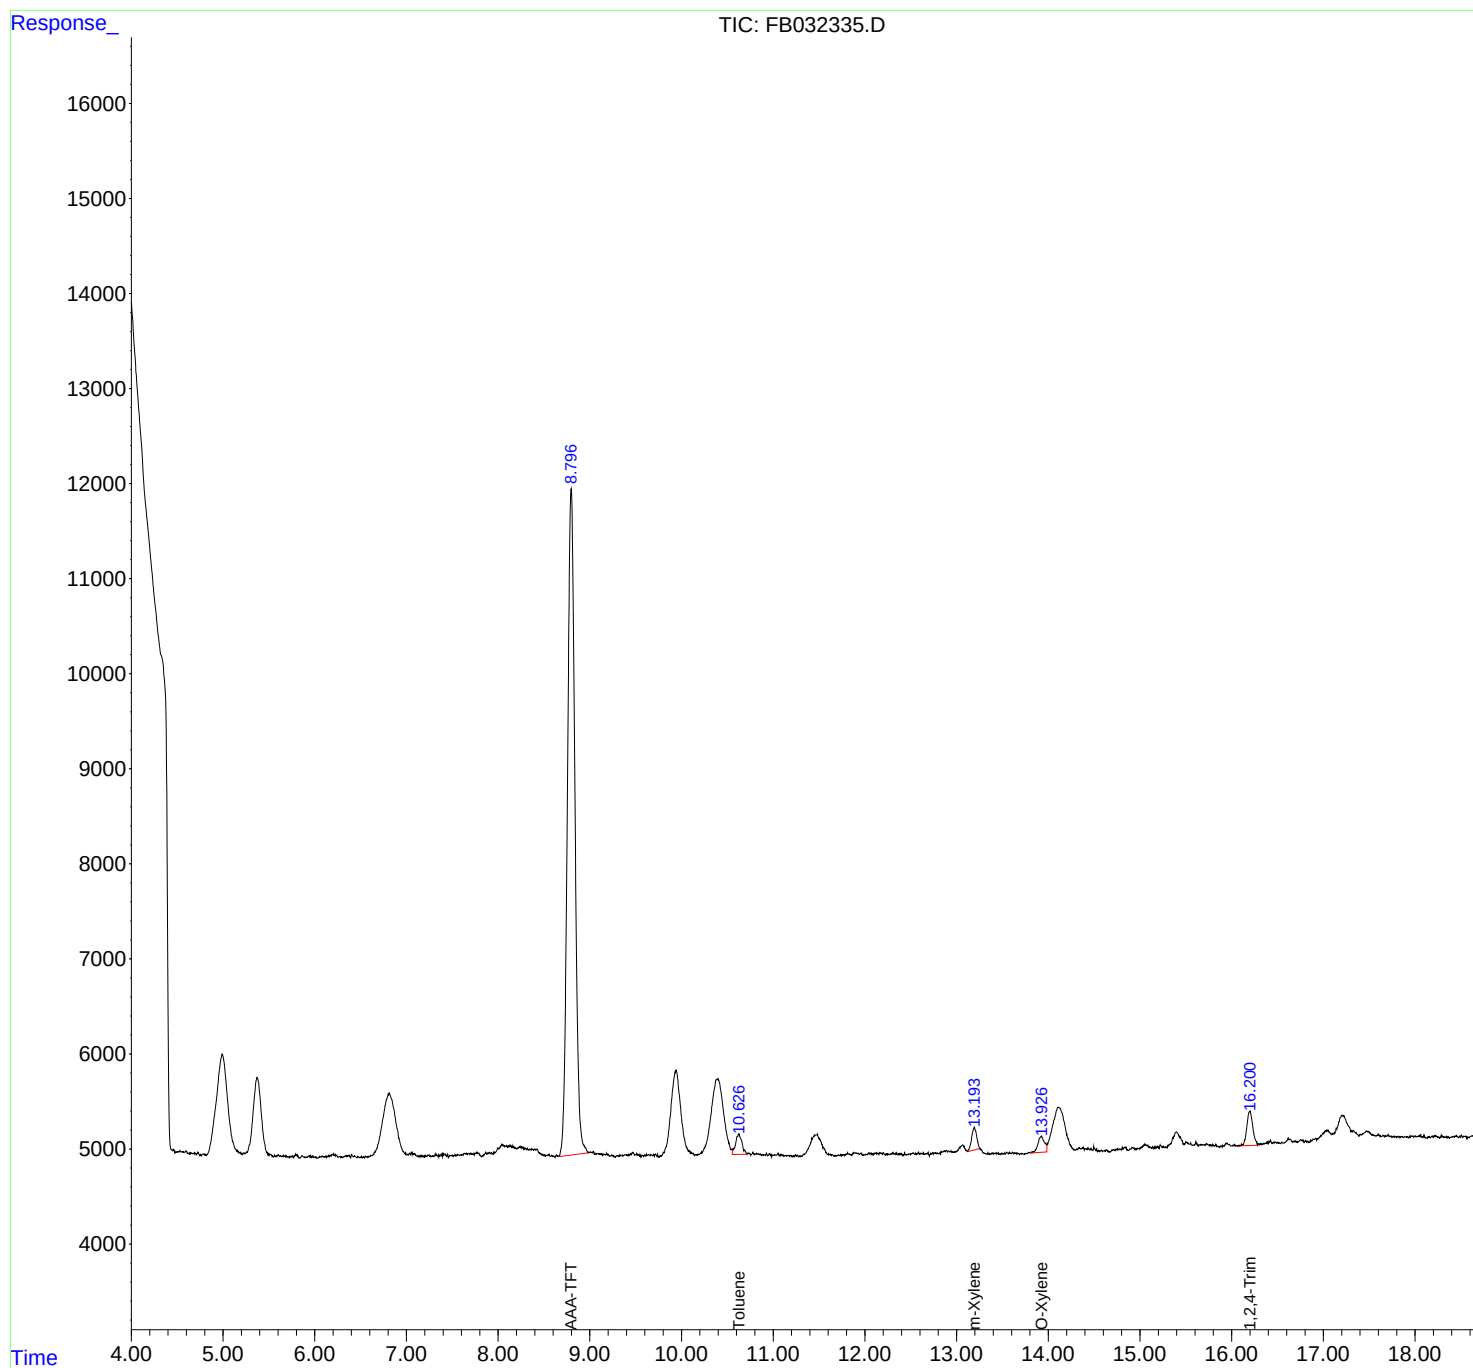


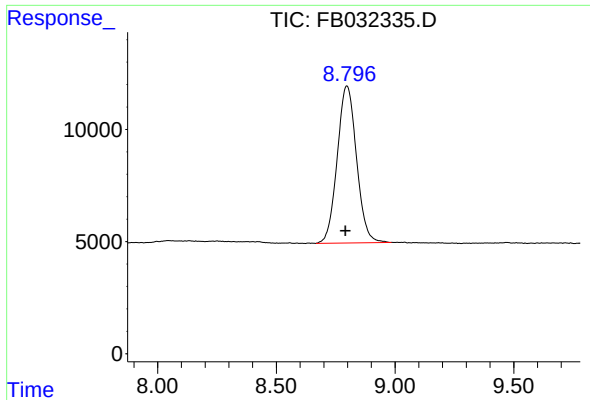

#5 AAA-TFT


R.T.: 8.798 min  
Delta R.T.: 0.007 min  
Response: 395890  
Conc: 19.52 ng/ml

Instrument :  
FID\_E  
ClientSampleId :

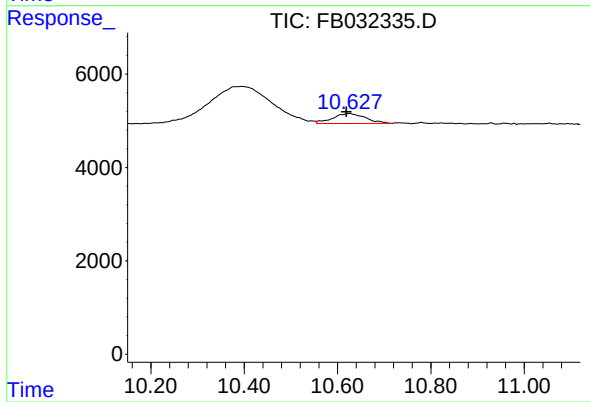


#6 Toluene

R.T.: 10.627 min  
Delta R.T.: 0.008 min  
Response: 10322  
Conc: 0.29 ng/ml

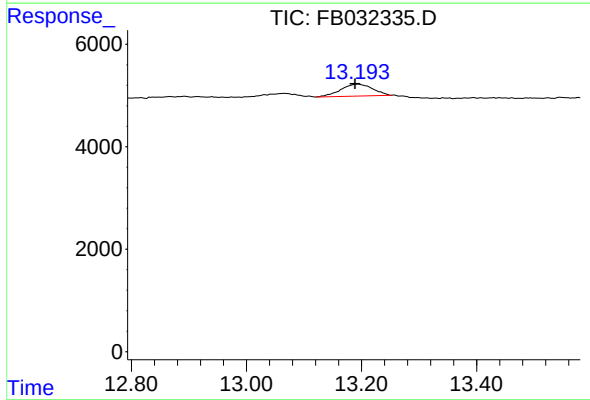


#8 m-Xylene

R.T.: 13.194 min  
Delta R.T.: 0.006 min  
Response: 8978  
Conc: 0.27 ng/ml

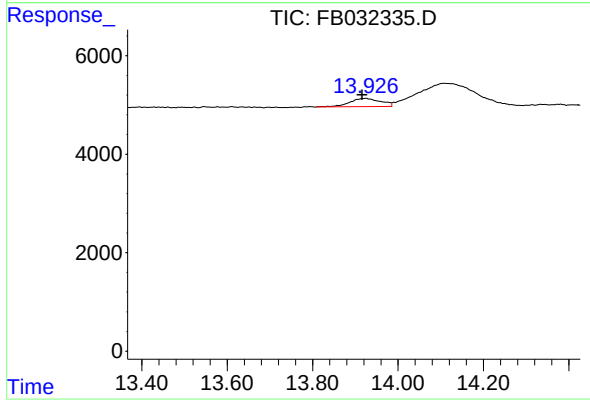

#9 O-Xylene

R.T.: 13.927 min  
Delta R.T.: 0.011 min  
Response: 8414  
Conc: 0.26 ng/ml

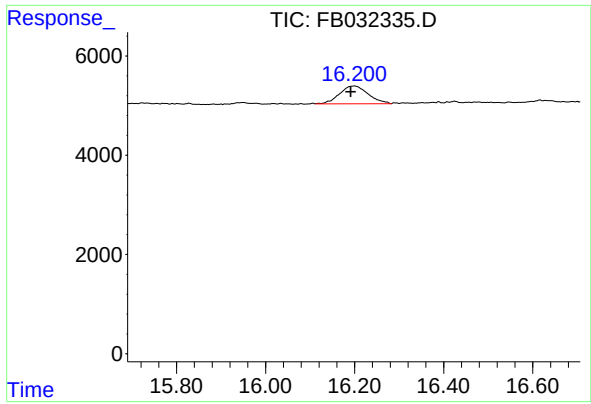

#10 1,2,4-Trimethylbenzene

R.T.: 16.201 min  
Delta R.T.: 0.010 min  
Response: 16049  
Conc: 0.58 ng/ml

Instrument :  
FID\_E  
ClientSampleId :