

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111025\
Data File : FB032339.D
Signal(s) : FID2B.CH
Acq On : 10 Nov 2025 12:18
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 11 03:38:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Quant Title :
QLast Update : Tue Oct 28 04:57:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.798	1963425	96.802 ng/ml
Target Compounds				
7) t	Ethylbenzene	13.076	74055	2.329 ng/ml
8) t	m-Xylene	13.207	109298	3.282 ng/ml
9) t	O-Xylene	13.920	159350	4.962 ng/ml
10) t	1,2,4-Trimethylbenzene	16.196	7341	0.265 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111025\
Data File : FB032339.D
Signal(s) : FID2B.CH
Acq On : 10 Nov 2025 12:18
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 11 03:38:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Quant Title :
QLast Update : Tue Oct 28 04:57:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

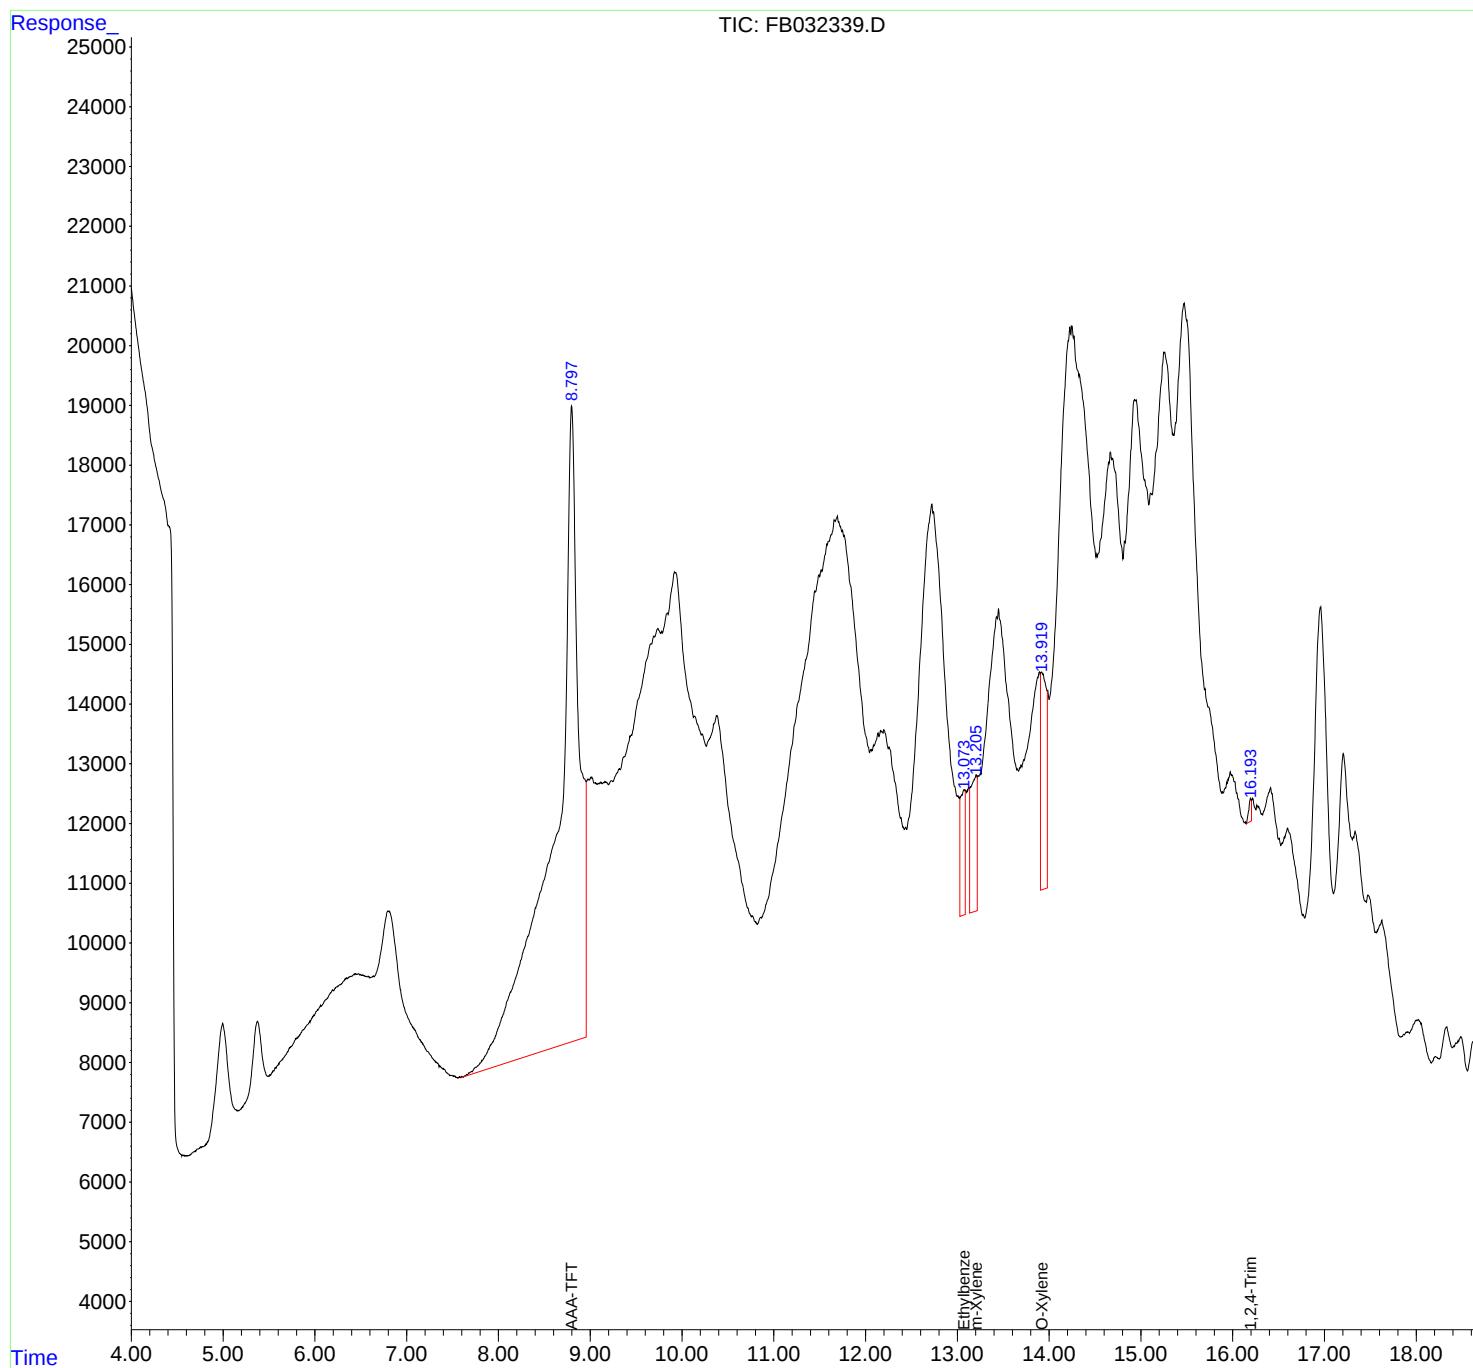


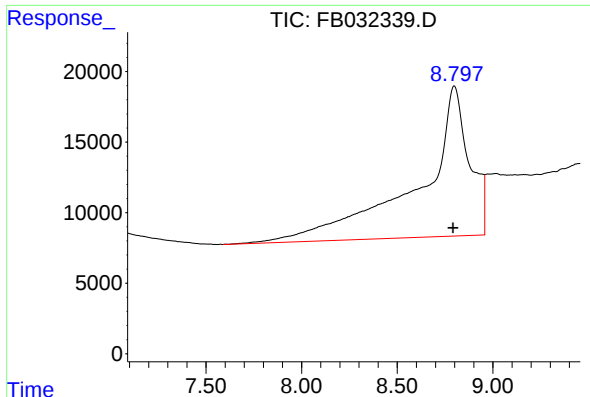

#5 AAA-TFT


R.T.: 8.798 min
Delta R.T.: 0.007 min
Response: 1963425
Conc: 96.80 ng/ml

Instrument :
FID_E
ClientSampleId :

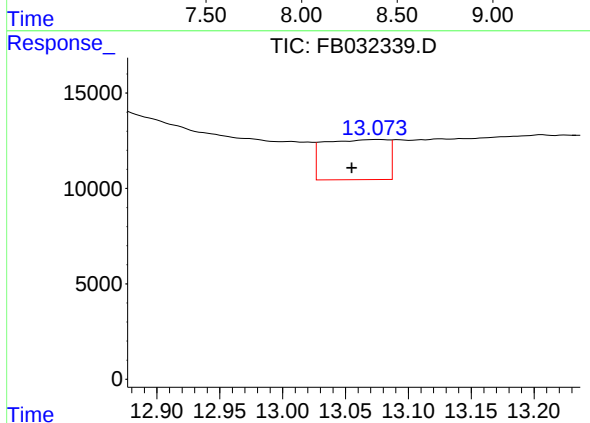


#7 Ethylbenzene

R.T.: 13.076 min
Delta R.T.: 0.021 min
Response: 74055
Conc: 2.33 ng/ml

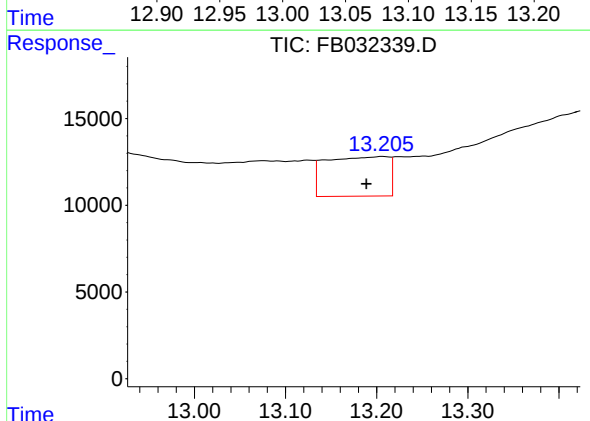


#8 m-Xylene

R.T.: 13.207 min
Delta R.T.: 0.018 min
Response: 109298
Conc: 3.28 ng/ml

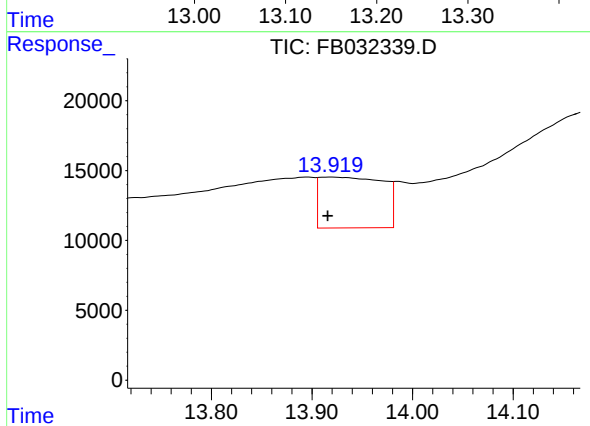

#9 O-Xylene

R.T.: 13.920 min
Delta R.T.: 0.004 min
Response: 159350
Conc: 4.96 ng/ml

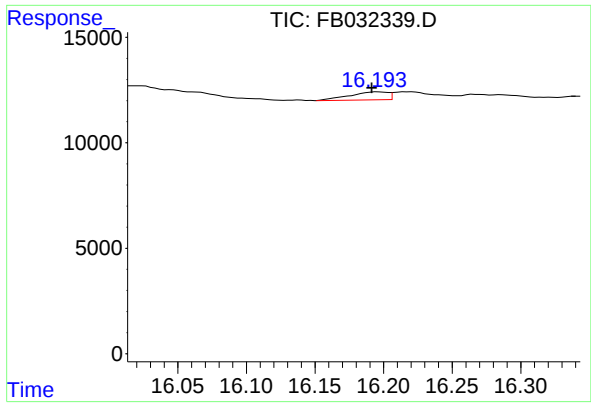

#10 1,2,4-Trimethylbenzene

R.T.: 16.196 min
Delta R.T.: 0.004 min
Response: 7341
Conc: 0.27 ng/ml

Instrument :
FID_E
ClientSampleId :