

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111025AL\
 Data File : FE056707.D
 Signal(s) : FID1B.ch
 Acq On : 10 Nov 2025 09:12
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 10 13:34:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 103025.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 30 12:50:27 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

11) T	n-Heneicosane (C21)	13.620	140449	0.764 ug/ml
17) T	n-Tricontane (C30)	18.131	993318	4.954 ug/ml
18) T	n-Dotriacontane (C32)	18.967	3681585	18.722 ug/ml
19) T	n-Tetratriacontane (C34)	19.754	5277719	30.576 ug/ml
20) T	n-Hexatriacontane (C36)	20.496	4840636	33.463 ug/ml
21) T	n-Octatriacontane (C38)	21.247	3328417	26.445 ug/ml
22) T	n-Tetracontane (C40)	22.187	2121195	18.347 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111025AL\
Data File : FE056707.D
Signal(s) : FID1B.ch
Acq On : 10 Nov 2025 09:12
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 10 13:34:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 103025.M
Quant Title : GC Extractables
QLast Update : Thu Oct 30 12:50:27 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

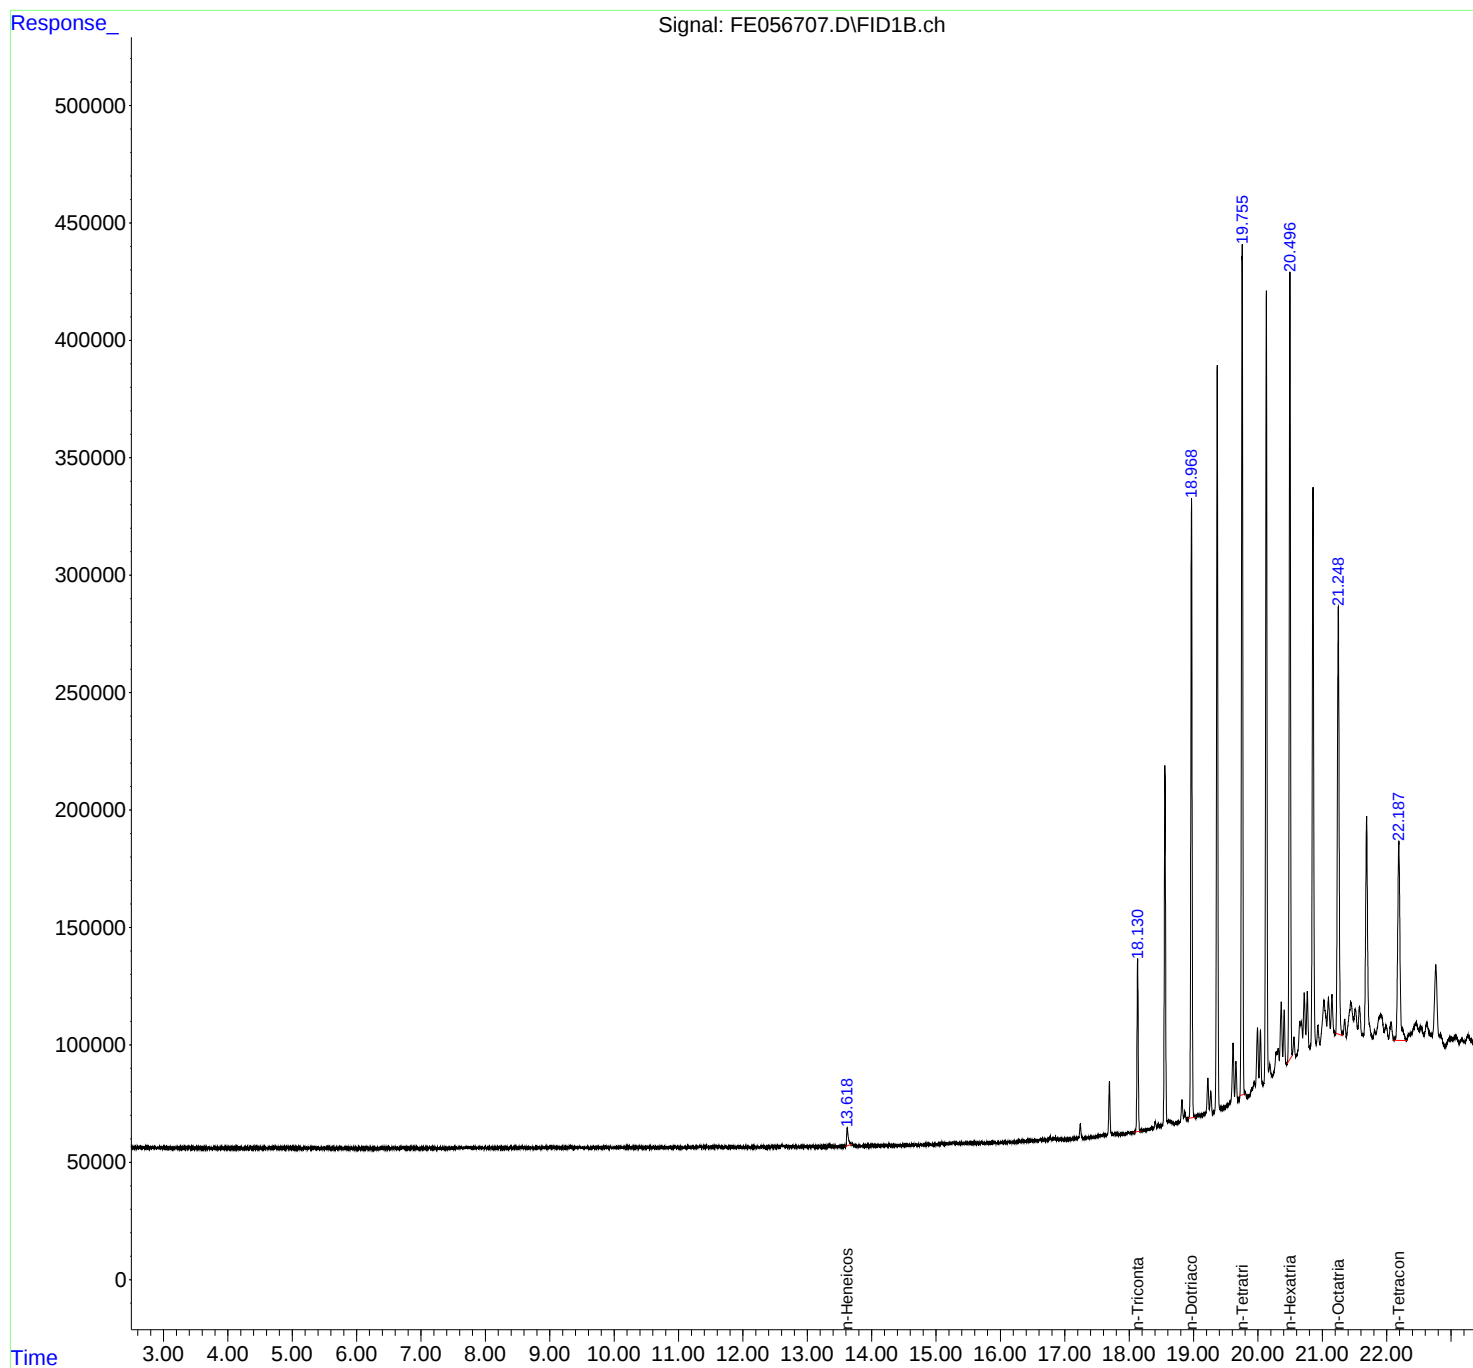


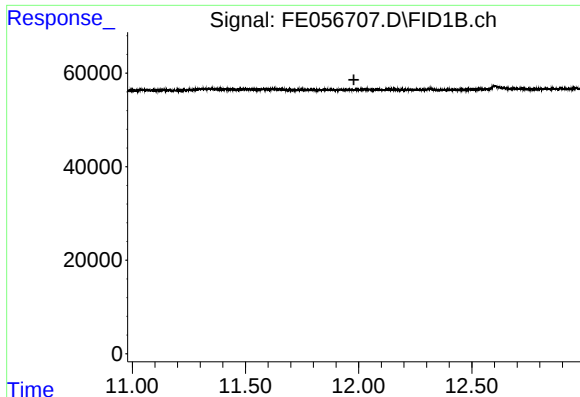

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.979 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

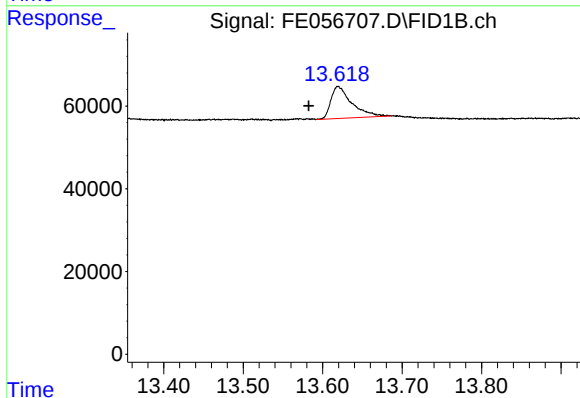


#11 n-Heneicosane (C21)

R.T.: 13.620 min
Delta R.T.: 0.038 min
Response: 140449
Conc: 0.76 ug/ml

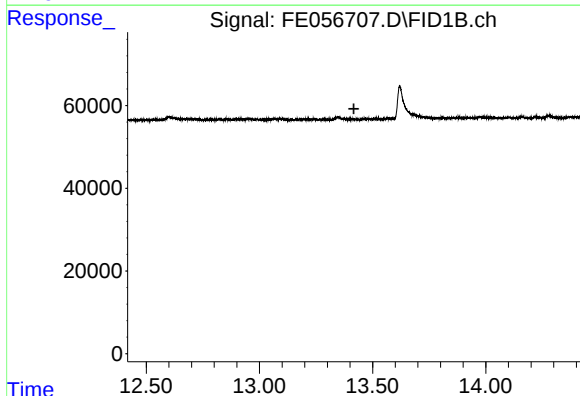


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.417 min
Response: 0
Conc: N.D.

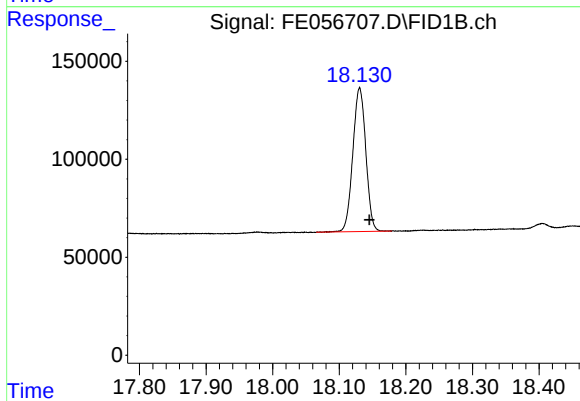

#17 n-Tricontane (C30)


R.T.: 18.131 min
Delta R.T.: -0.014 min
Response: 993318
Conc: 4.95 ug/ml

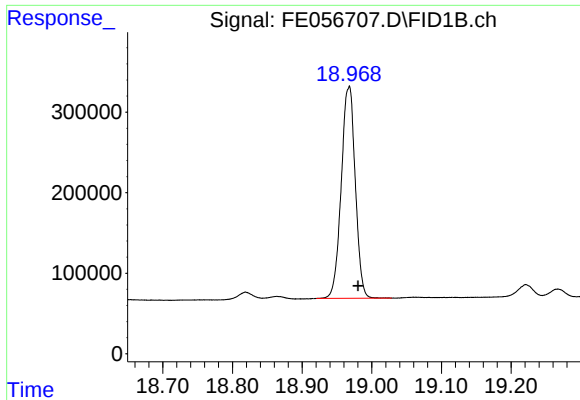

#18 n-Dotriacontane (C32)


R.T.: 18.967 min
Delta R.T.: -0.014 min
Response: 3681585
Conc: 18.72 ug/ml

Instrument :
FID_E
ClientSampleId :

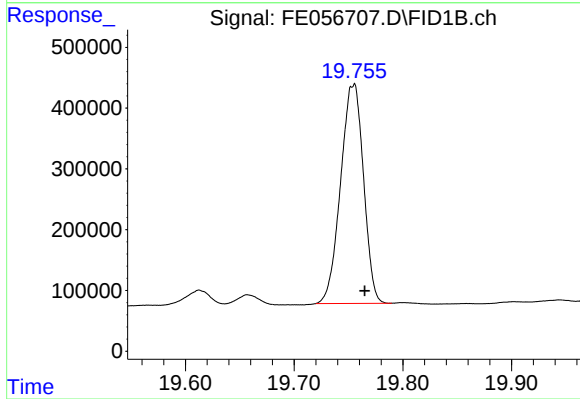


#19 n-Tetratriacontane (C34)

R.T.: 19.754 min
Delta R.T.: -0.011 min
Response: 5277719
Conc: 30.58 ug/ml

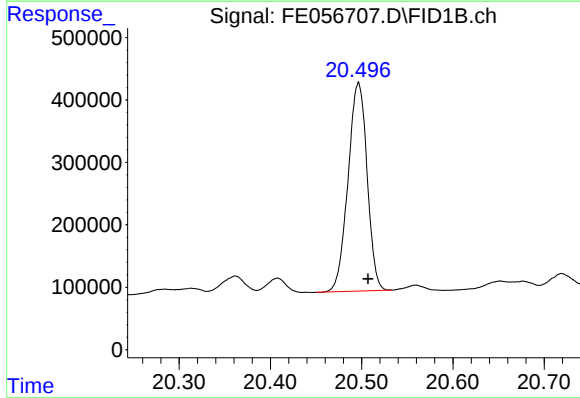


#20 n-Hexatriacontane (C36)

R.T.: 20.496 min
Delta R.T.: -0.010 min
Response: 4840636
Conc: 33.46 ug/ml

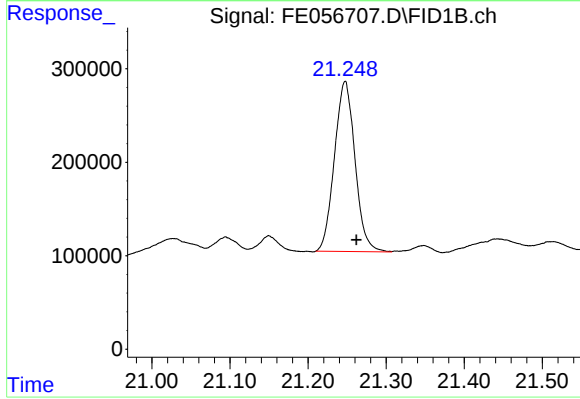

#21 n-Octatriacontane (C38)

R.T.: 21.247 min
Delta R.T.: -0.015 min
Response: 3328417
Conc: 26.45 ug/ml

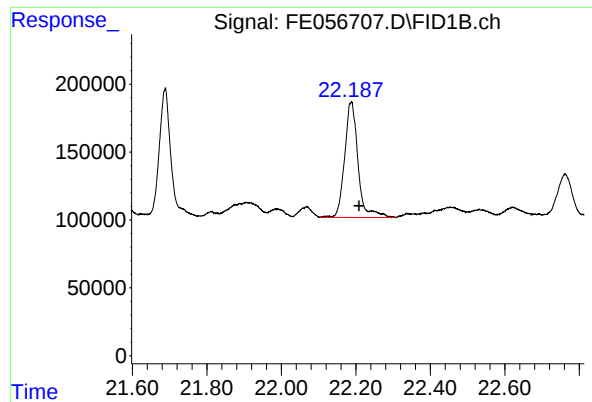

#22 n-Tetracontane (C40)

R.T.: 22.187 min
Delta R.T.: -0.022 min
Response: 2121195
Conc: 18.35 ug/ml

Instrument :
FID_E
ClientSampleId :