

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111319\
 Data File : FE030845.D
 Signal(s) : FID1B.CH
 Acq On : 13 Nov 2019 15:26
 Operator : DD\AJ
 Sample : PB124745BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 14 00:50:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
 Quant Title :
 QLast Update : Thu Oct 31 08:47:02 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.664	6248454	20.105 ug/ml
Target Compounds			
4) N-TETRADECANE	8.259	150041	0.401 ug/ml
8) N-DOCOSANE	13.758	243542	0.677 ug/ml
11) N-HEXACOSANE	15.885	256405	0.735 ug/ml
12) N-OCTACOSANE	16.838	789989	2.317 ug/ml
13) N-TRIACONTANE	17.726	967867	2.914 ug/ml
14) N-DOTRIACONTANE	18.558	593700	1.860 ug/ml
15) N-TETRATRIACONTANE	19.345	197842	0.650 ug/ml
16) N-HEXATRIACONTANE	20.084	379302	1.382 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111319\
Data File : FE030845.D
Signal(s) : FID1B.CH
Acq On : 13 Nov 2019 15:26
Operator : DD\AJ
Sample : PB124745BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 14 00:50:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
Quant Title :
QLast Update : Thu Oct 31 08:47:02 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

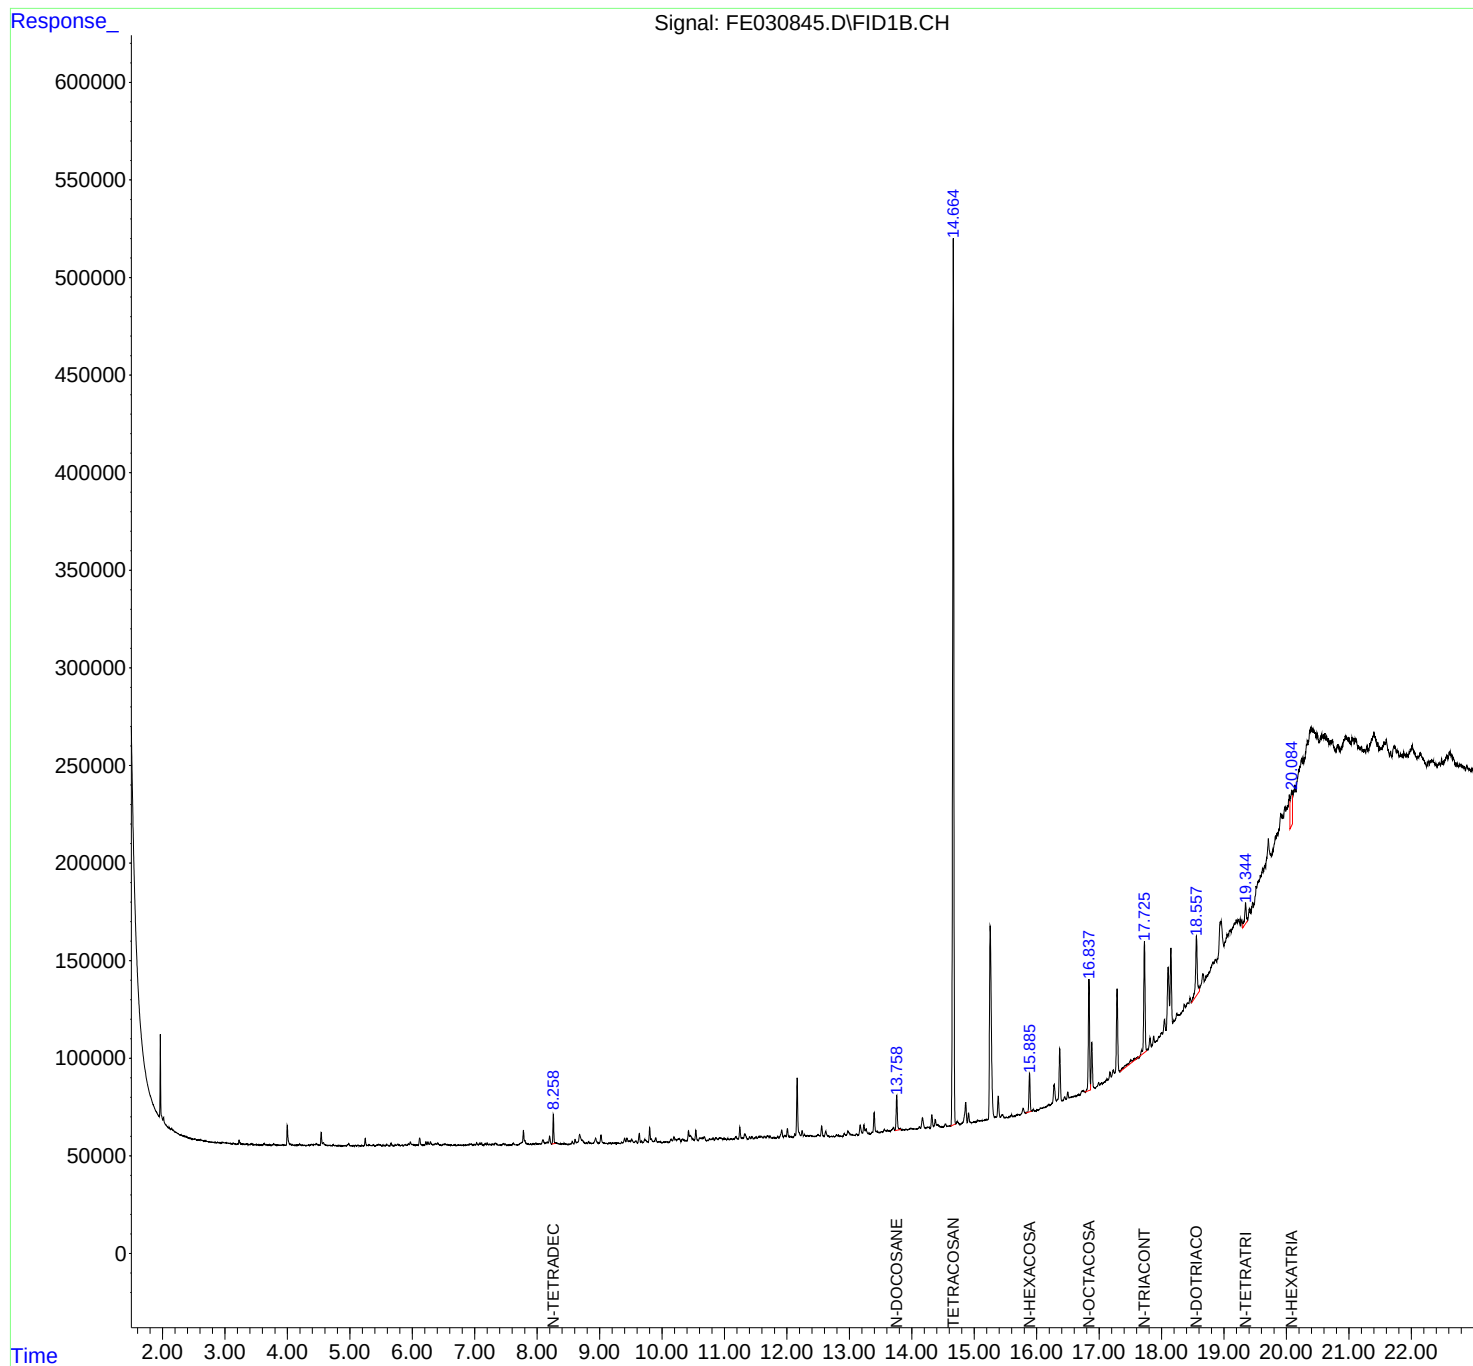


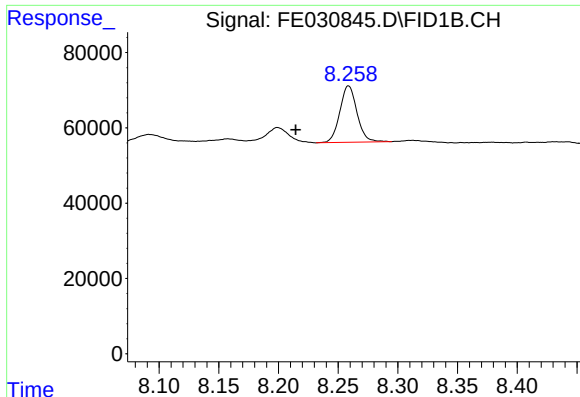

#4 N-TETRADECANE


R.T.: 8.259 min
Delta R.T.: 0.044 min
Response: 150041
Conc: 0.40 ug/ml

Instrument :
FID_E
ClientSampleId :

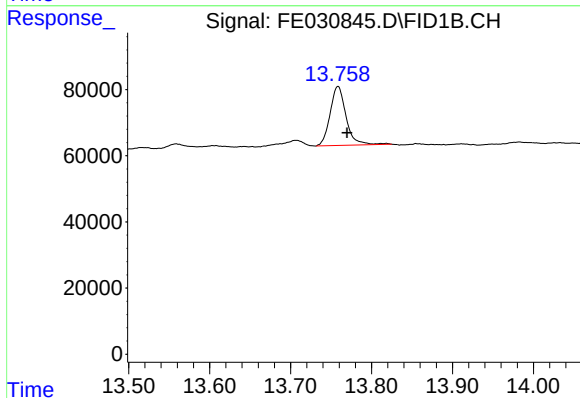


#8 N-DOCOSANE

R.T.: 13.758 min
Delta R.T.: -0.011 min
Response: 243542
Conc: 0.68 ug/ml

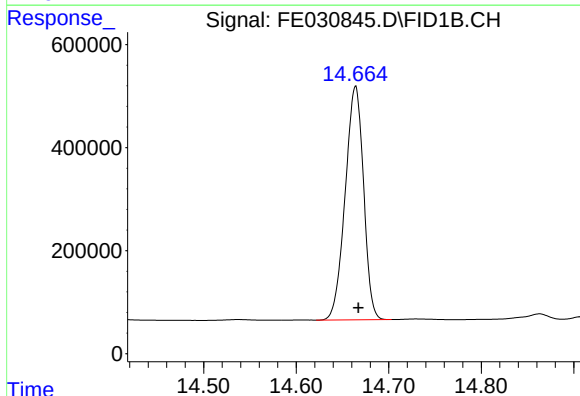


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.664 min
Delta R.T.: -0.003 min
Response: 6248454
Conc: 20.11 ug/ml

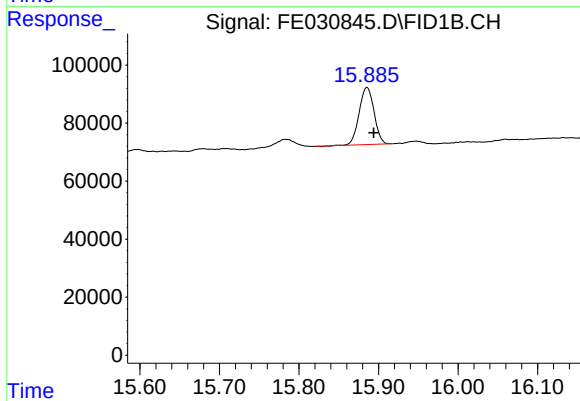

#11 N-HEXACOSANE


R.T.: 15.885 min
Delta R.T.: -0.009 min
Response: 256405
Conc: 0.74 ug/ml

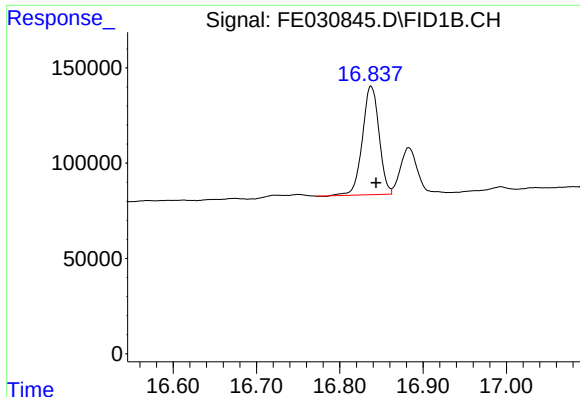

#12 N-OCTACOSANE


R.T.: 16.838 min
Delta R.T.: -0.006 min
Response: 789989
Conc: 2.32 ug/ml

Instrument :
FID_E
ClientSampleId :

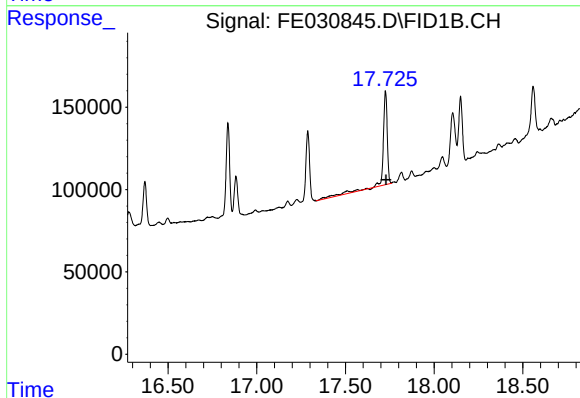


#13 N-TRIACONTANE

R.T.: 17.726 min
Delta R.T.: -0.004 min
Response: 967867
Conc: 2.91 ug/ml

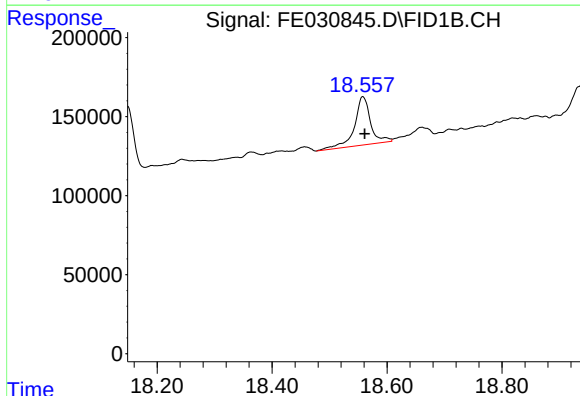


#14 N-DOTRIACONTANE

R.T.: 18.558 min
Delta R.T.: -0.003 min
Response: 593700
Conc: 1.86 ug/ml

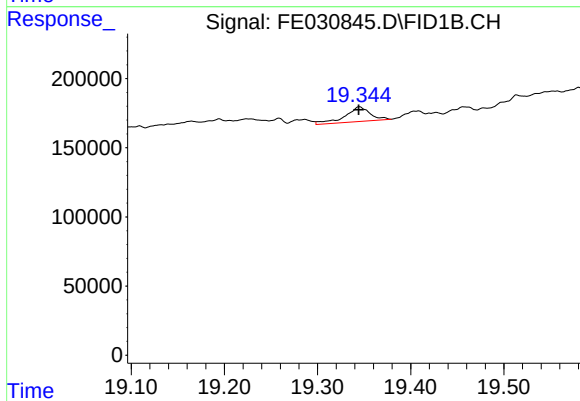

#15 N-TETRATRIACONTANE

R.T.: 19.345 min
Delta R.T.: 0.001 min
Response: 197842
Conc: 0.65 ug/ml

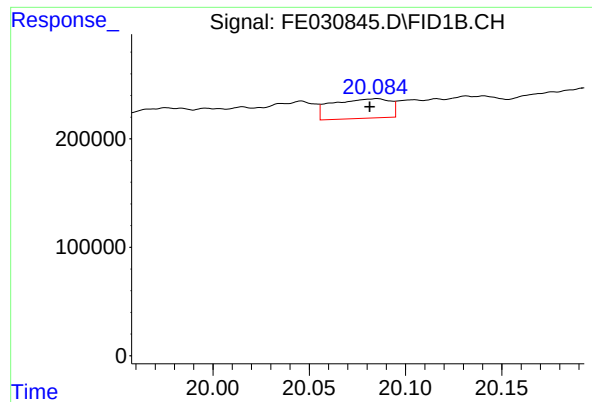

#16 N-HEXATRIACONTANE

R.T.: 20.084 min
Delta R.T.: 0.003 min
Response: 379302
Conc: 1.38 ug/ml

Instrument :
FID_E
ClientSampleId :