

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111319\
 Data File : FE030847.D
 Signal(s) : FID1B.CH
 Acq On : 13 Nov 2019 16:33
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 14 00:50:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
 Quant Title :
 QLast Update : Thu Oct 31 08:47:02 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.662	6139221	19.754 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.724	250531	0.754 ug/ml
14) N-DOTRIACONTANE	18.556	334767	1.049 ug/ml
15) N-TETRATRIACONTANE	19.342	206955	0.680 ug/ml
16) N-HEXATRIACONTANE	20.083	1397192	5.089 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111319\
Data File : FE030847.D
Signal(s) : FID1B.CH
Acq On : 13 Nov 2019 16:33
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 14 00:50:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
Quant Title :
QLast Update : Thu Oct 31 08:47:02 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

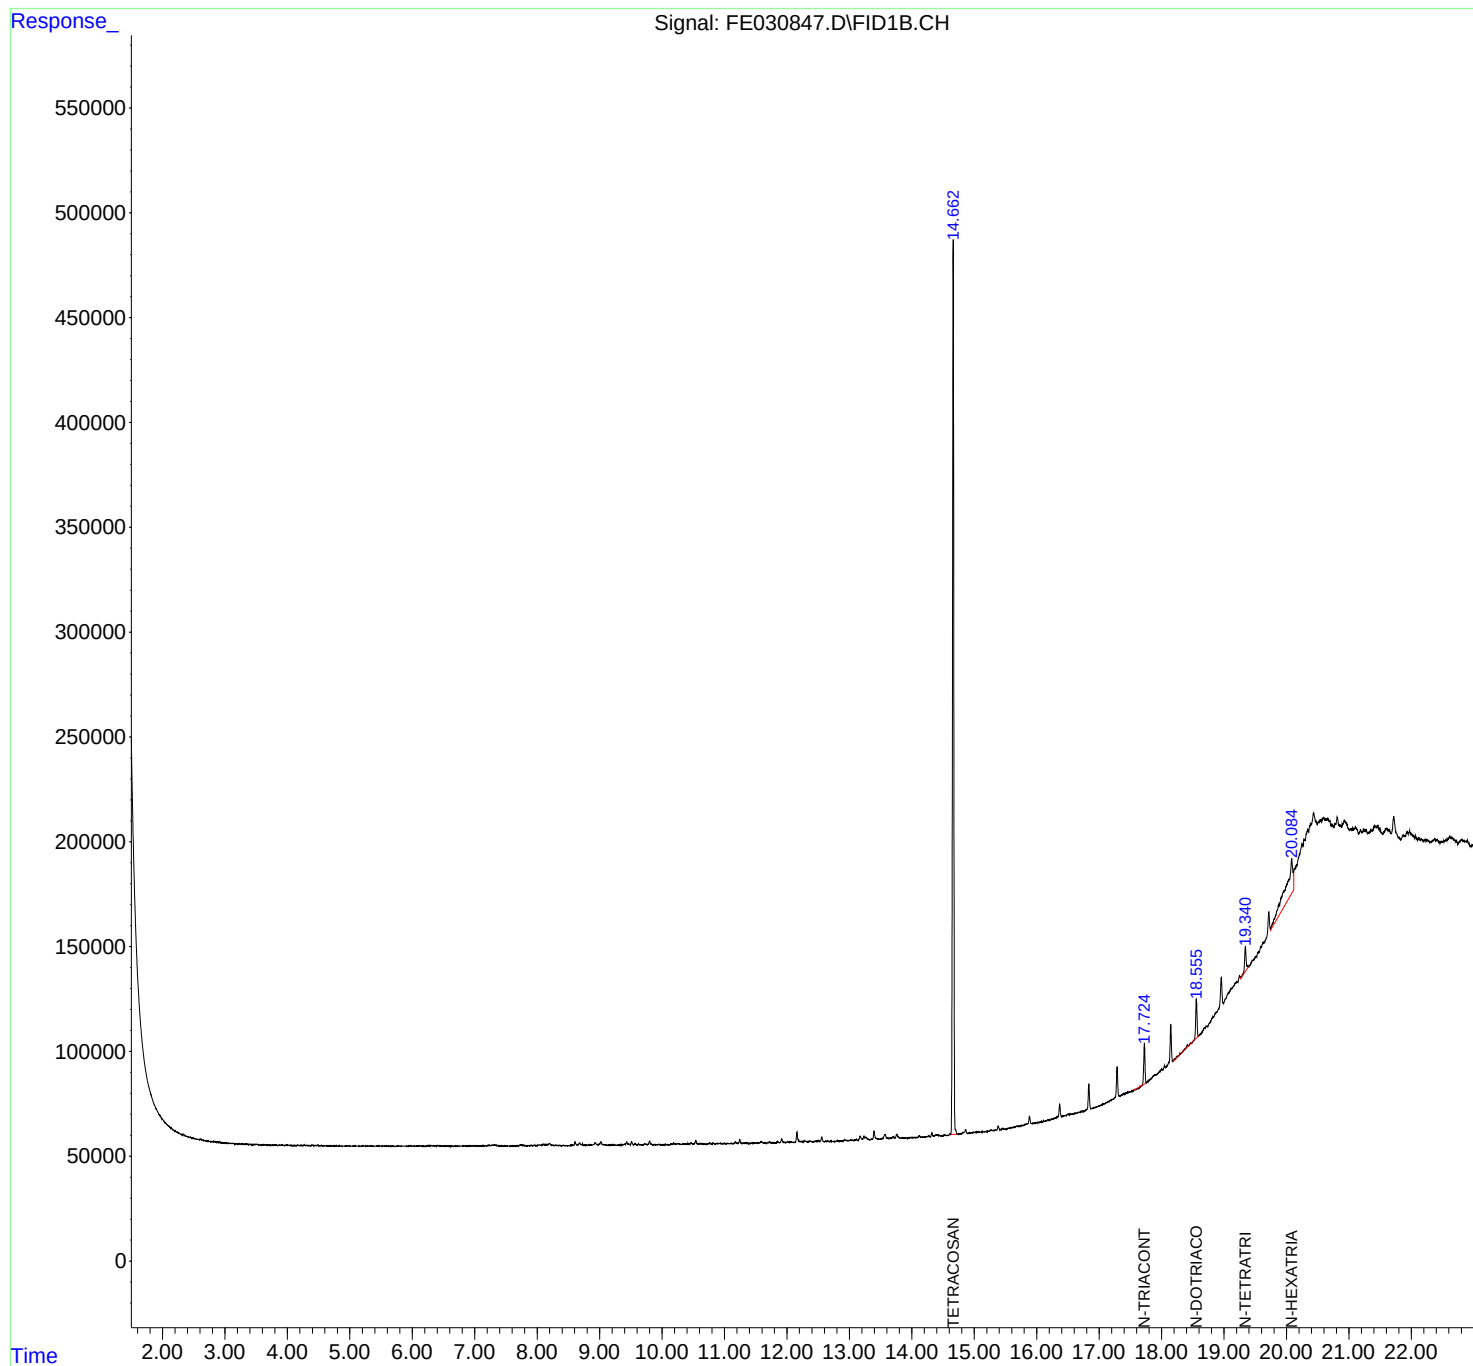


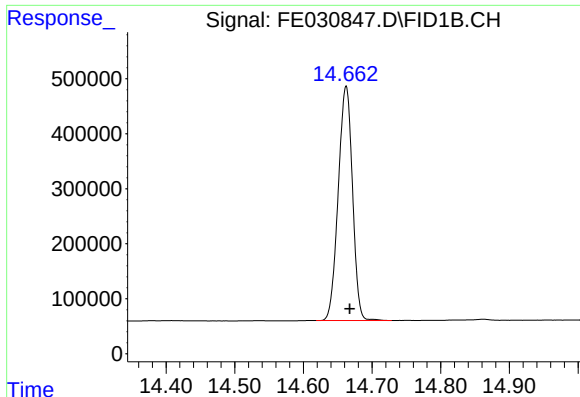

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.662 min
Delta R.T.: -0.005 min
Response: 6139221
Conc: 19.75 ug/ml

Instrument :
FID_E
ClientSampleId :

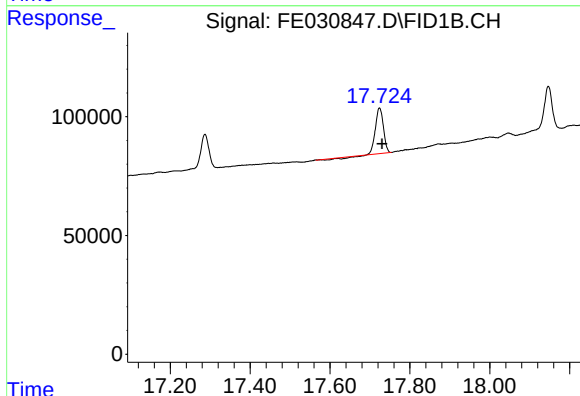


#13 N-TRIACONTANE

R.T.: 17.724 min
Delta R.T.: -0.006 min
Response: 250531
Conc: 0.75 ug/ml

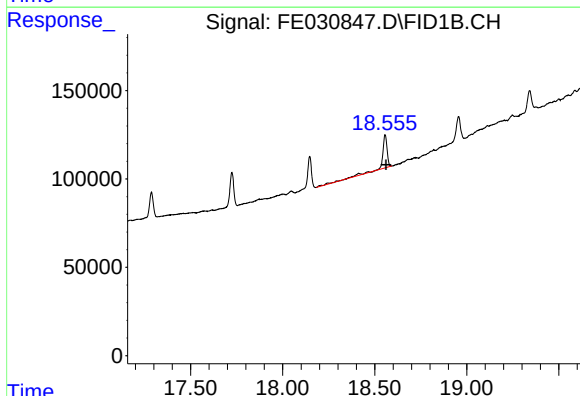


#14 N-DOTRIACONTANE

R.T.: 18.556 min
Delta R.T.: -0.005 min
Response: 334767
Conc: 1.05 ug/ml

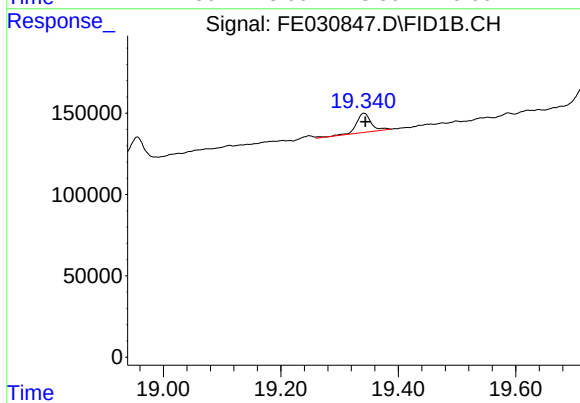

#15 N-TETRATRIACONTANE

R.T.: 19.342 min
Delta R.T.: -0.003 min
Response: 206955
Conc: 0.68 ug/ml

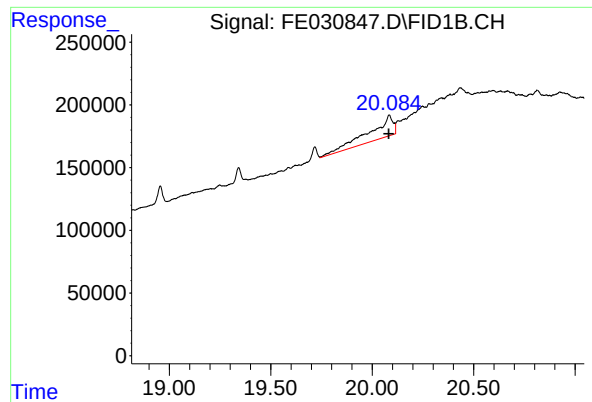

#16 N-HEXATRIACONTANE

R.T.: 20.083 min
Delta R.T.: 0.002 min
Response: 1397192
Conc: 5.09 ug/ml

Instrument :
FID_E
ClientSampleId :