

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111225\
Data File : FB032346.D
Signal(s) : FID2B.CH
Acq On : 12 Nov 2025 15:13
Operator : YP/AJ
Sample : Q3610-01
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 14 01:02:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Quant Title :
QLast Update : Tue Oct 28 04:57:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	97045	4.785 ng/ml
Target Compounds			
6) t Toluene	10.620	5801	0.162 ng/ml
8) t m-Xylene	13.191	7372	0.221 ng/ml
9) t O-Xylene	13.911	4032	0.126 ng/ml
10) t 1,2,4-Trimethylbenzene	16.202	12099	0.437 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111225\
Data File : FB032346.D
Signal(s) : FID2B.CH
Acq On : 12 Nov 2025 15:13
Operator : YP/AJ
Sample : Q3610-01
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 14 01:02:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Quant Title :
QLast Update : Tue Oct 28 04:57:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

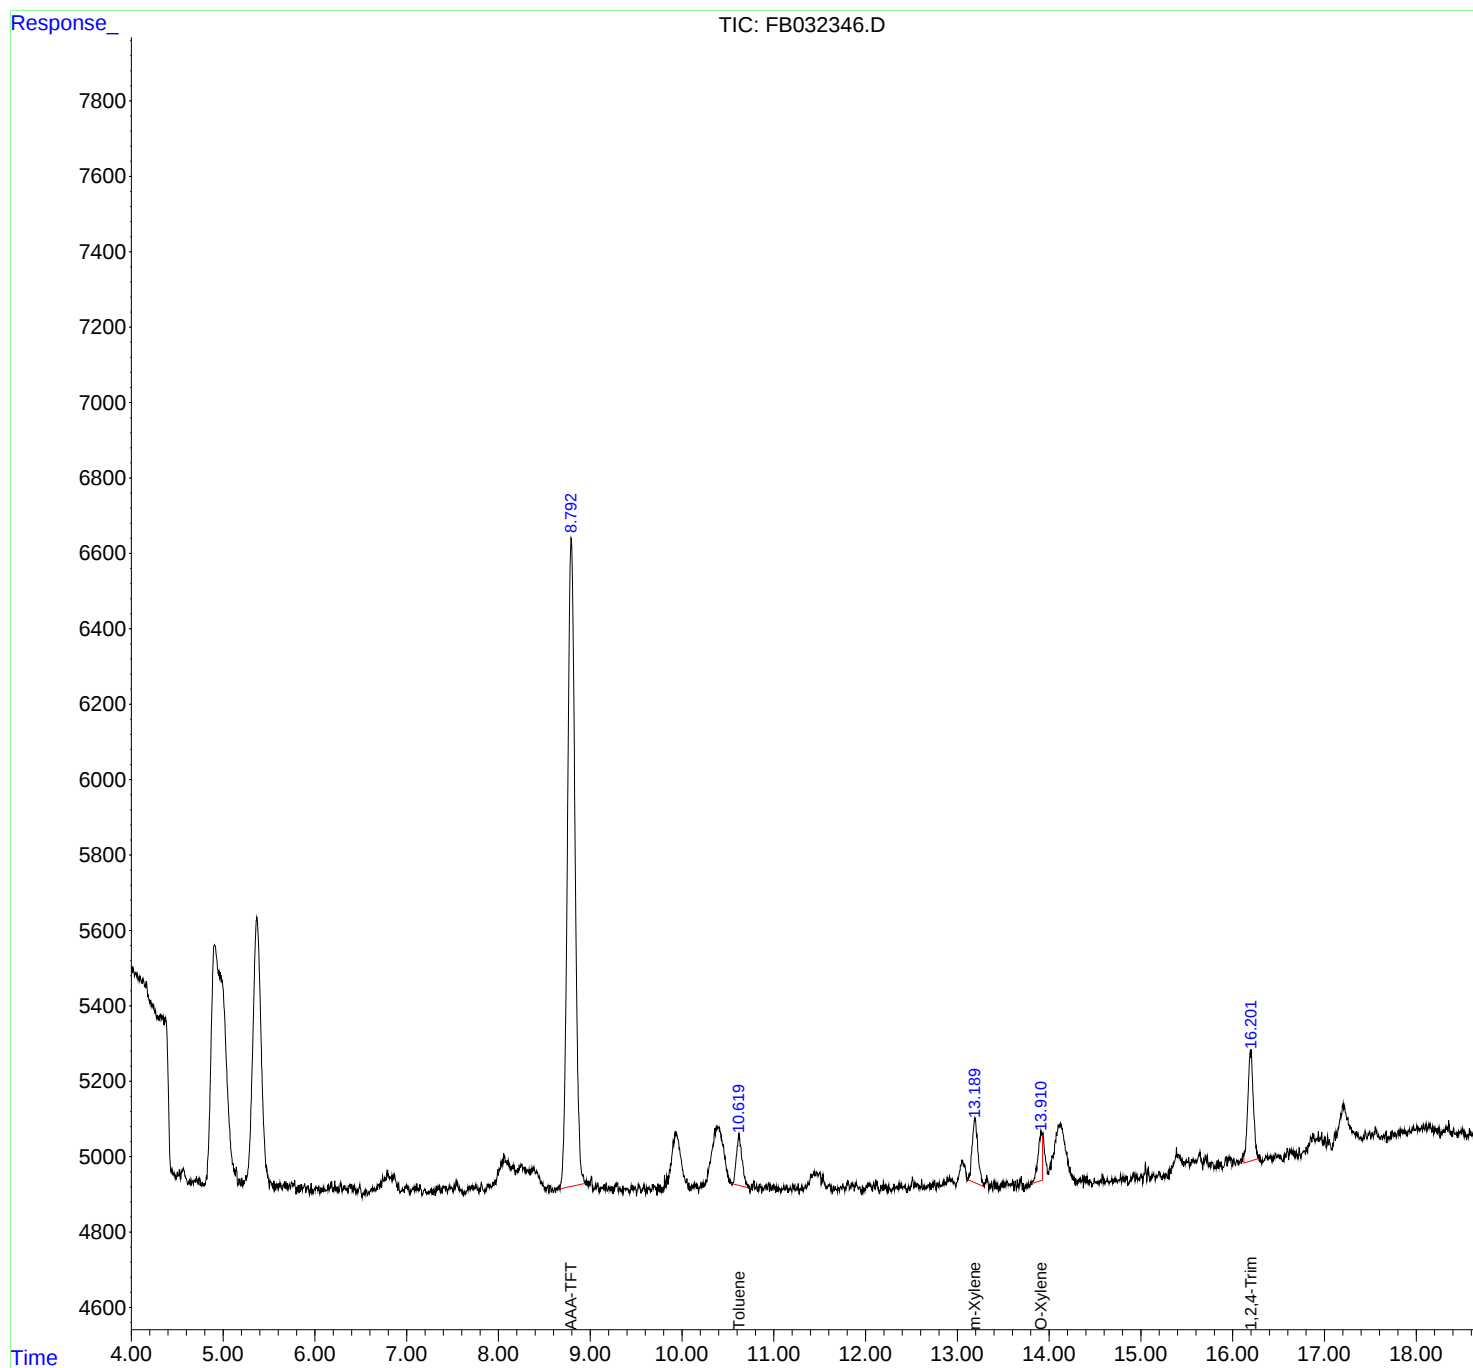


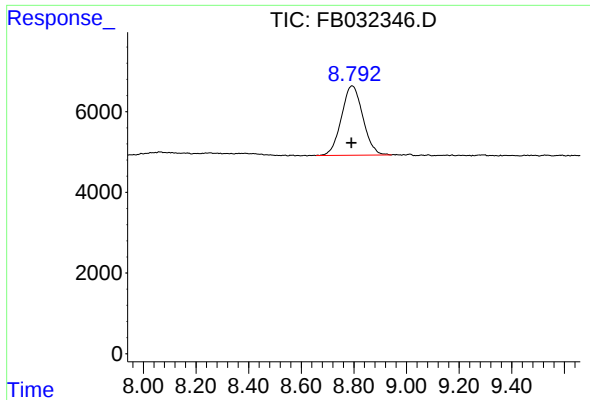

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.003 min
Response: 97045
Conc: 4.78 ng/ml

Instrument :
FID_E
ClientSampleId :

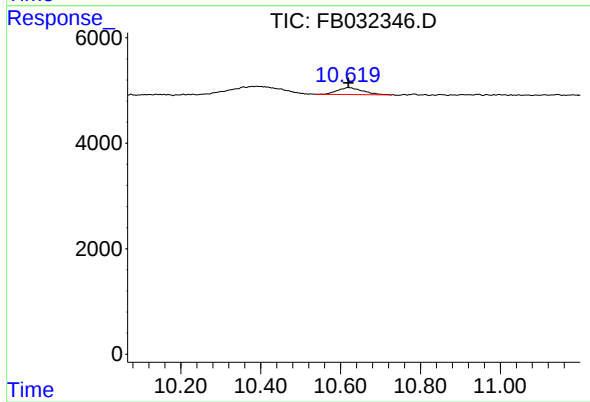


#6 Toluene

R.T.: 10.620 min
Delta R.T.: 0.000 min
Response: 5801
Conc: 0.16 ng/ml

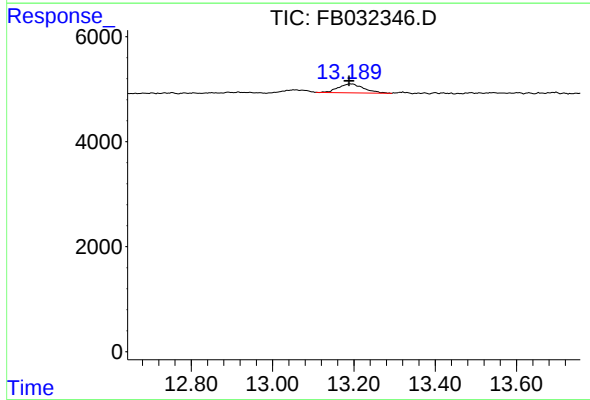


#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: 0.002 min
Response: 7372
Conc: 0.22 ng/ml

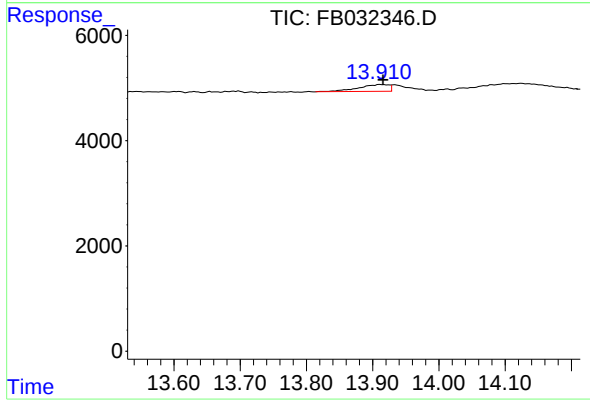

#9 O-Xylene

R.T.: 13.911 min
Delta R.T.: -0.005 min
Response: 4032
Conc: 0.13 ng/ml

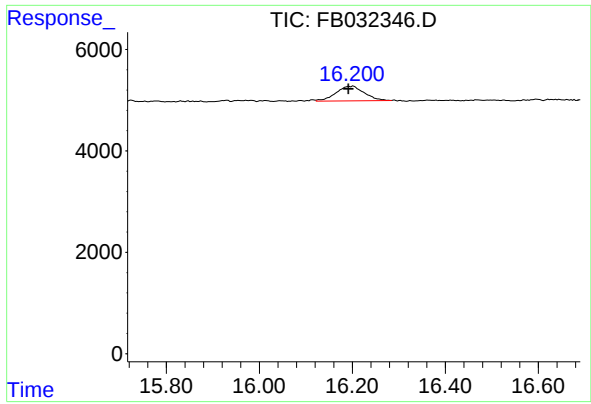

#10 1,2,4-Trimethylbenzene

R.T.: 16.202 min
Delta R.T.: 0.011 min
Response: 12099
Conc: 0.44 ng/ml

Instrument :
FID_E
ClientSampleId :