

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111225\
Data File : FB032360.D
Signal(s) : FID2B.CH
Acq On : 13 Nov 2025 8:48
Operator : YP/AJ
Sample : Q3610-14
Misc : 4.77G/5.00 ML DI WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 14 01:05:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Quant Title :
QLast Update : Tue Oct 28 04:57:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	136323	6.721 ng/ml
Target Compounds			
6) t Toluene	10.613	9504	0.266 ng/ml
7) t Ethylbenzene	13.053	4174	0.131 ng/ml
8) t m-Xylene	13.187	12265	0.368 ng/ml
9) t O-Xylene	13.915	15044	0.468 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	19010	0.687 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB111225\
Data File : FB032360.D
Signal(s) : FID2B.CH
Acq On : 13 Nov 2025 8:48
Operator : YP/AJ
Sample : Q3610-14
Misc : 4.77G/5.00 ML DI WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: Calibration.e
Quant Time: Nov 14 01:05:05 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB102725.M
Quant Title :
QLast Update : Tue Oct 28 04:57:39 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

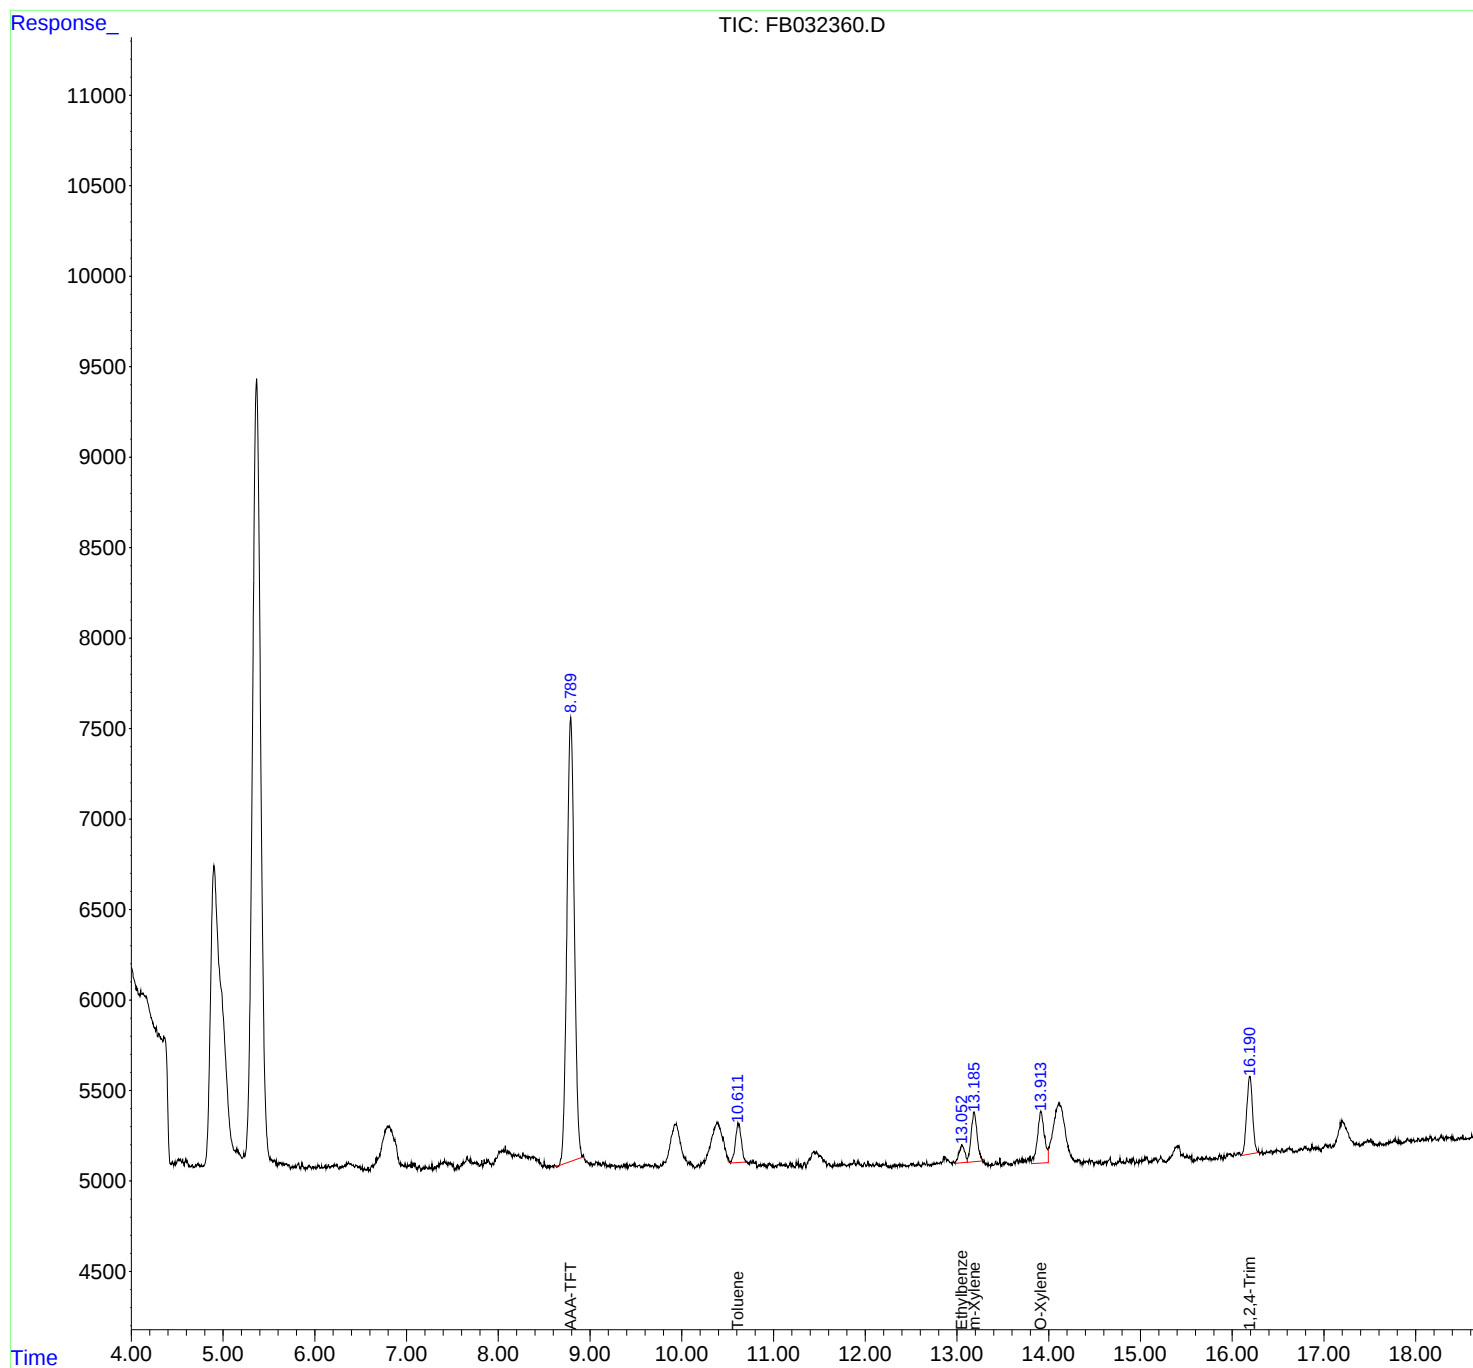


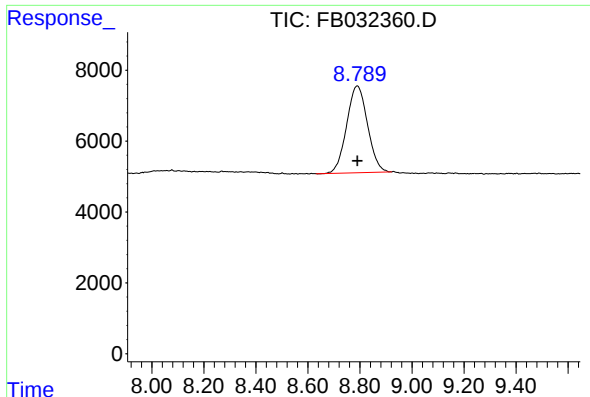

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: 0.000 min
Response: 136323
Conc: 6.72 ng/ml

Instrument :
FID_E
ClientSampleId :

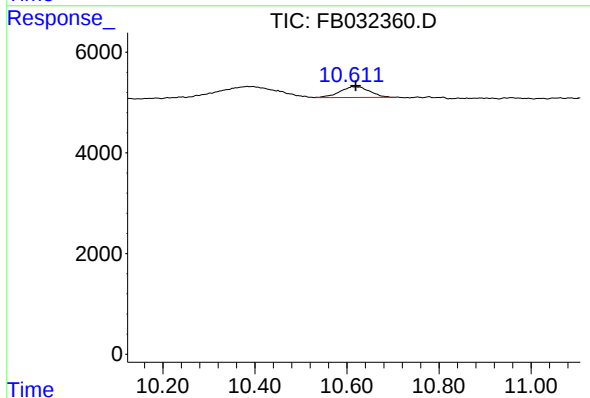


#6 Toluene

R.T.: 10.613 min
Delta R.T.: -0.007 min
Response: 9504
Conc: 0.27 ng/ml

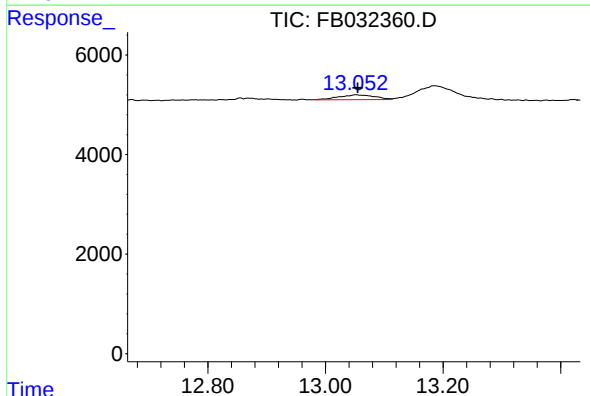


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.002 min
Response: 4174
Conc: 0.13 ng/ml

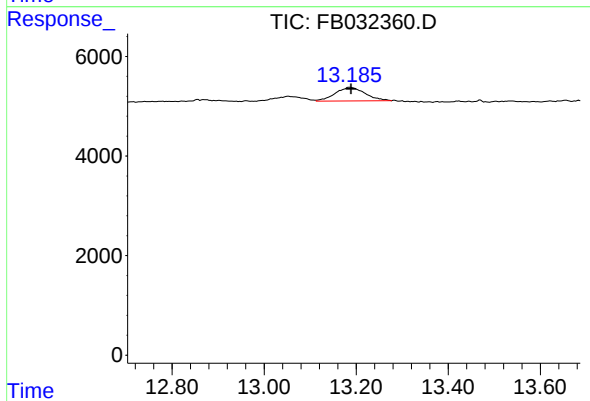

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: -0.002 min
Response: 12265
Conc: 0.37 ng/ml

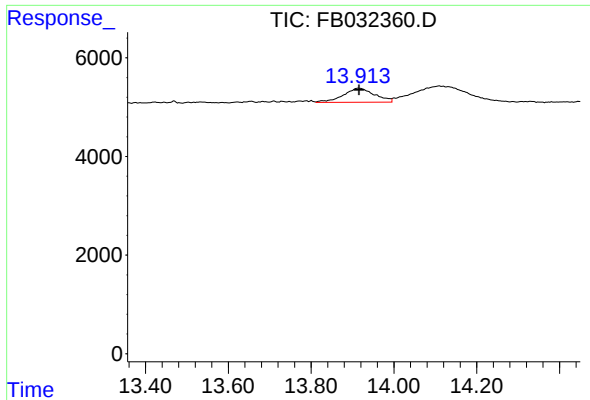

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: -0.001 min
Response: 15044
Conc: 0.47 ng/ml

Instrument :
FID_E
ClientSampleId :

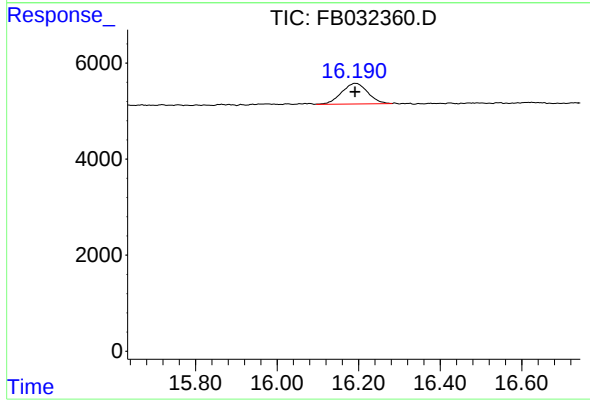

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.000 min
Response: 19010
Conc: 0.69 ng/ml