

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111225\
Data File : FF016665.D
Signal(s) : FID2B.ch
Acq On : 12 Nov 2025 20:51
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 14 04:52:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102925.M
Quant Title :
QLast Update : Wed Oct 29 12:48:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
14)	N-DOTRIACONTANE	18.967	68688	0.641 ug/ml
15)	N-TETRATRIACONTANE	19.755	54038	0.550 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111225\
Data File : FF016665.D
Signal(s) : FID2B.ch
Acq On : 12 Nov 2025 20:51
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 14 04:52:57 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102925.M
Quant Title :
QLast Update : Wed Oct 29 12:48:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

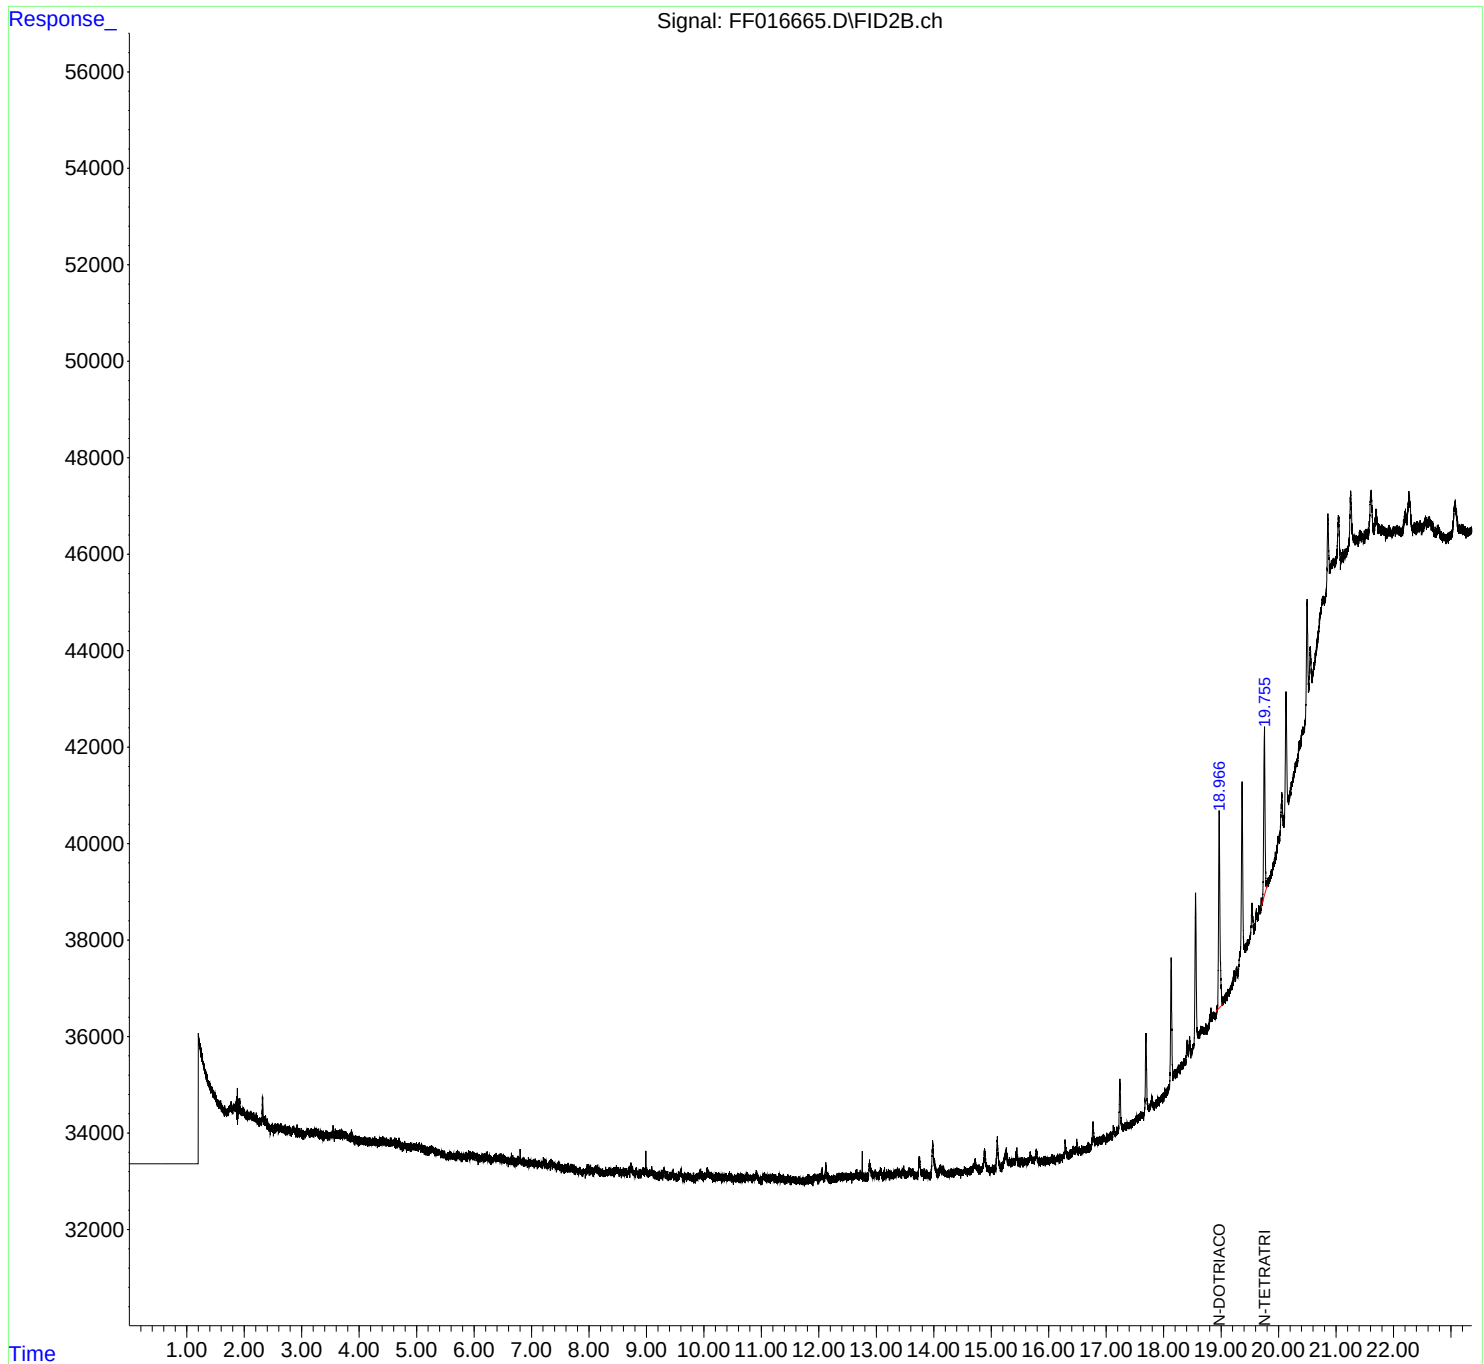


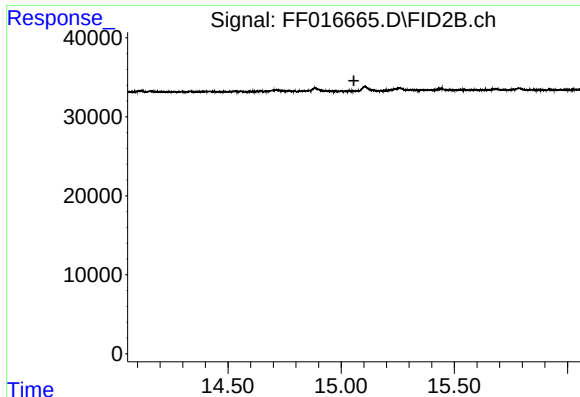

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.056 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

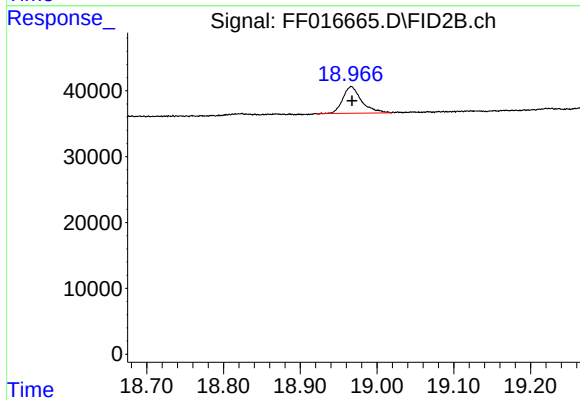

#14 N-DOTRIACONTANE

R.T.: 18.967 min
Delta R.T.: 0.000 min
Response: 68688
Conc: 0.64 ug/ml

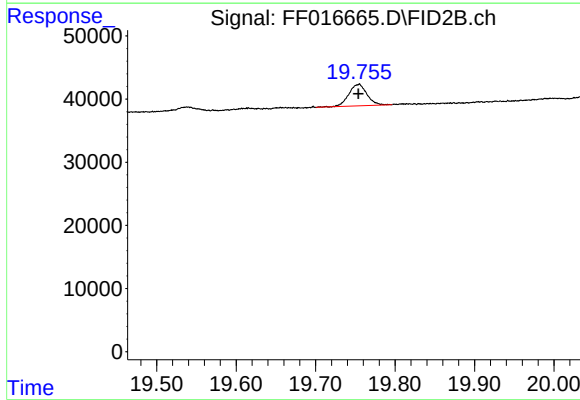

#15 N-TETRATRIACONTANE

R.T.: 19.755 min
Delta R.T.: 0.000 min
Response: 54038
Conc: 0.55 ug/ml