

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111325\
Data File : FF016676.D
Signal(s) : FID2B.ch
Acq On : 13 Nov 2025 08:08
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 14 05:45:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102925.M
Quant Title :
QLast Update : Wed Oct 29 12:48:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
13)	N-TRIACONTANE	18.127	62967	0.560 ug/ml
14)	N-DOTRIACONTANE	18.964	101687	0.949 ug/ml
15)	N-TETRATRIACONTANE	19.751	86000	0.875 ug/ml
16)	N-HEXATRIACONTANE	20.495	55091	0.644 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111325\
Data File : FF016676.D
Signal(s) : FID2B.ch
Acq On : 13 Nov 2025 08:08
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 14 05:45:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102925.M
Quant Title :
QLast Update : Wed Oct 29 12:48:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

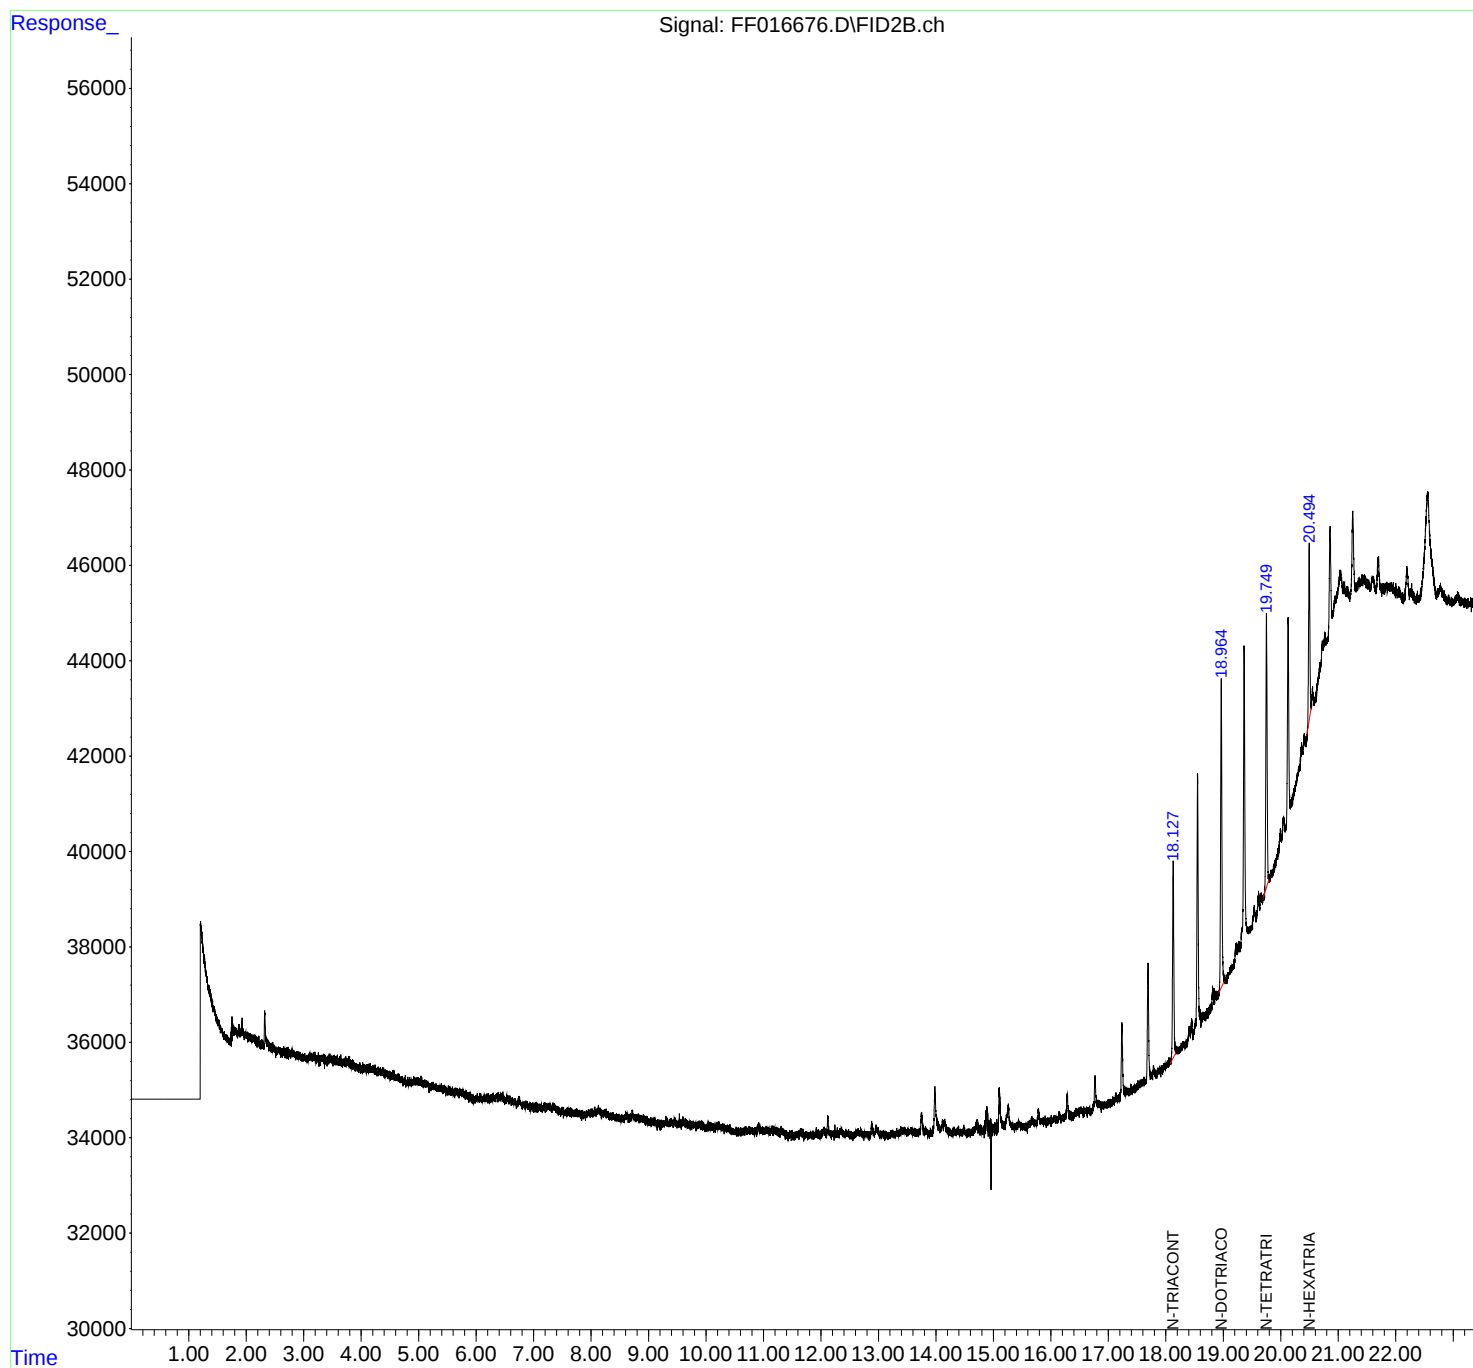


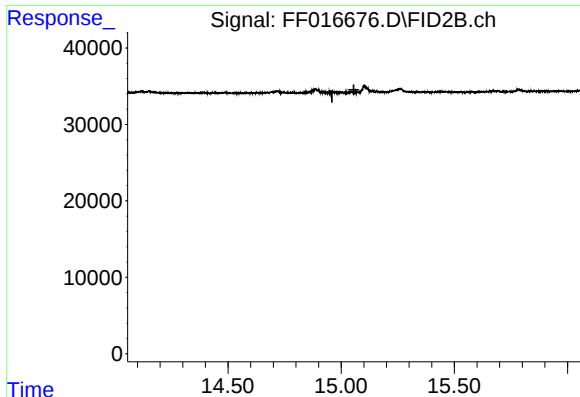

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 15.056 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

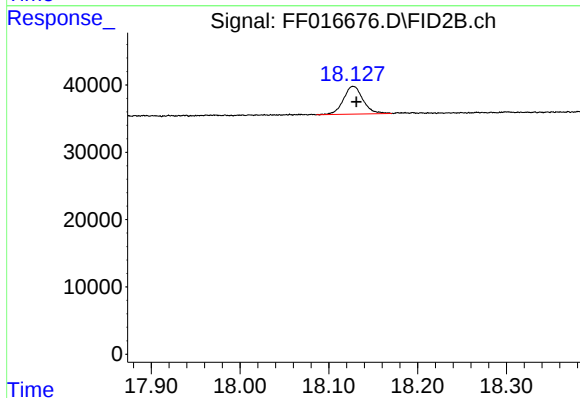


#13 N-TRIACONTANE

R.T.: 18.127 min
Delta R.T.: -0.003 min
Response: 62967
Conc: 0.56 ug/ml

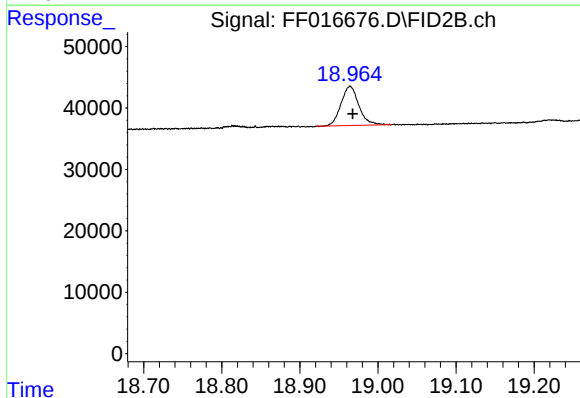


#14 N-DOTRIACONTANE

R.T.: 18.964 min
Delta R.T.: -0.003 min
Response: 101687
Conc: 0.95 ug/ml

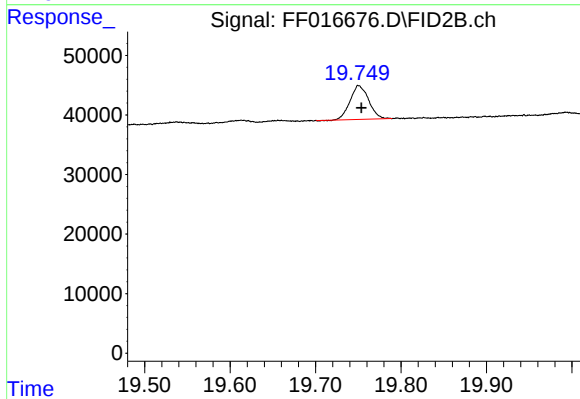

#15 N-TETRATRIACONTANE

R.T.: 19.751 min
Delta R.T.: -0.003 min
Response: 86000
Conc: 0.88 ug/ml

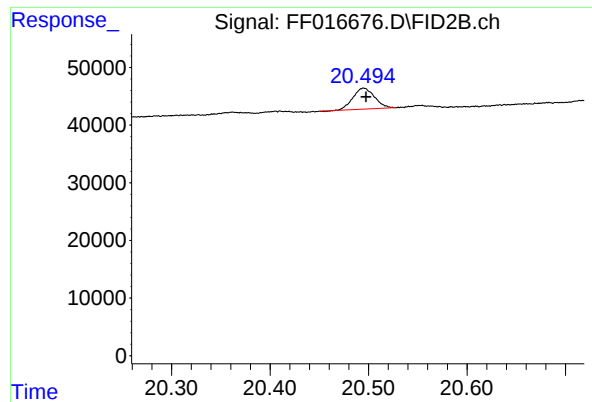

#16 N-HEXATRIACONTANE

R.T.: 20.495 min
Delta R.T.: -0.003 min
Response: 55091
Conc: 0.64 ug/ml

Instrument :

FID_E

ClientSampleId :