

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111325\
 Data File : FF016682.D
 Signal(s) : FID2B.ch
 Acq On : 13 Nov 2025 16:04
 Operator : YP\AJ
 Sample : Q3610-01
 Misc :
 ALS Vial : 73 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 14 05:47:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102925.M
 Quant Title :
 QLast Update : Wed Oct 29 12:48:52 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units


System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.052	1356662	12.986 ug/ml
Target Compounds			
7) N-EICOSANE	13.008f	269971	2.211 ug/ml
10) N-TETRACOSANE	15.233	163948	1.384 ug/ml
11) N-HEXACOSANE	16.282	20056	0.175 ug/ml
12) N-OCTACOSANE	17.238	58695	0.515 ug/ml
13) N-TRIACONTANE	18.126	306582	2.729 ug/ml
14) N-DOTRIACONTANE	18.957	143676	1.340 ug/ml
16) N-HEXATRIACONTANE	20.509	52892	0.619 ug/ml
17) N-OCTATRIACONTANE	21.256	80640	1.051 ug/ml
18) N-TETRACONTANE	22.203	27246	0.399 ug/ml


(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111325\
Data File : FF016682.D
Signal(s) : FID2B.ch
Acq On : 13 Nov 2025 16:04
Operator : YP\AJ
Sample : Q3610-01
Misc :
ALS Vial : 73 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 14 05:47:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102925.M
Quant Title :
QLast Update : Wed Oct 29 12:48:52 2025
Response via : Initial Calibration
Integrator: ChemStation

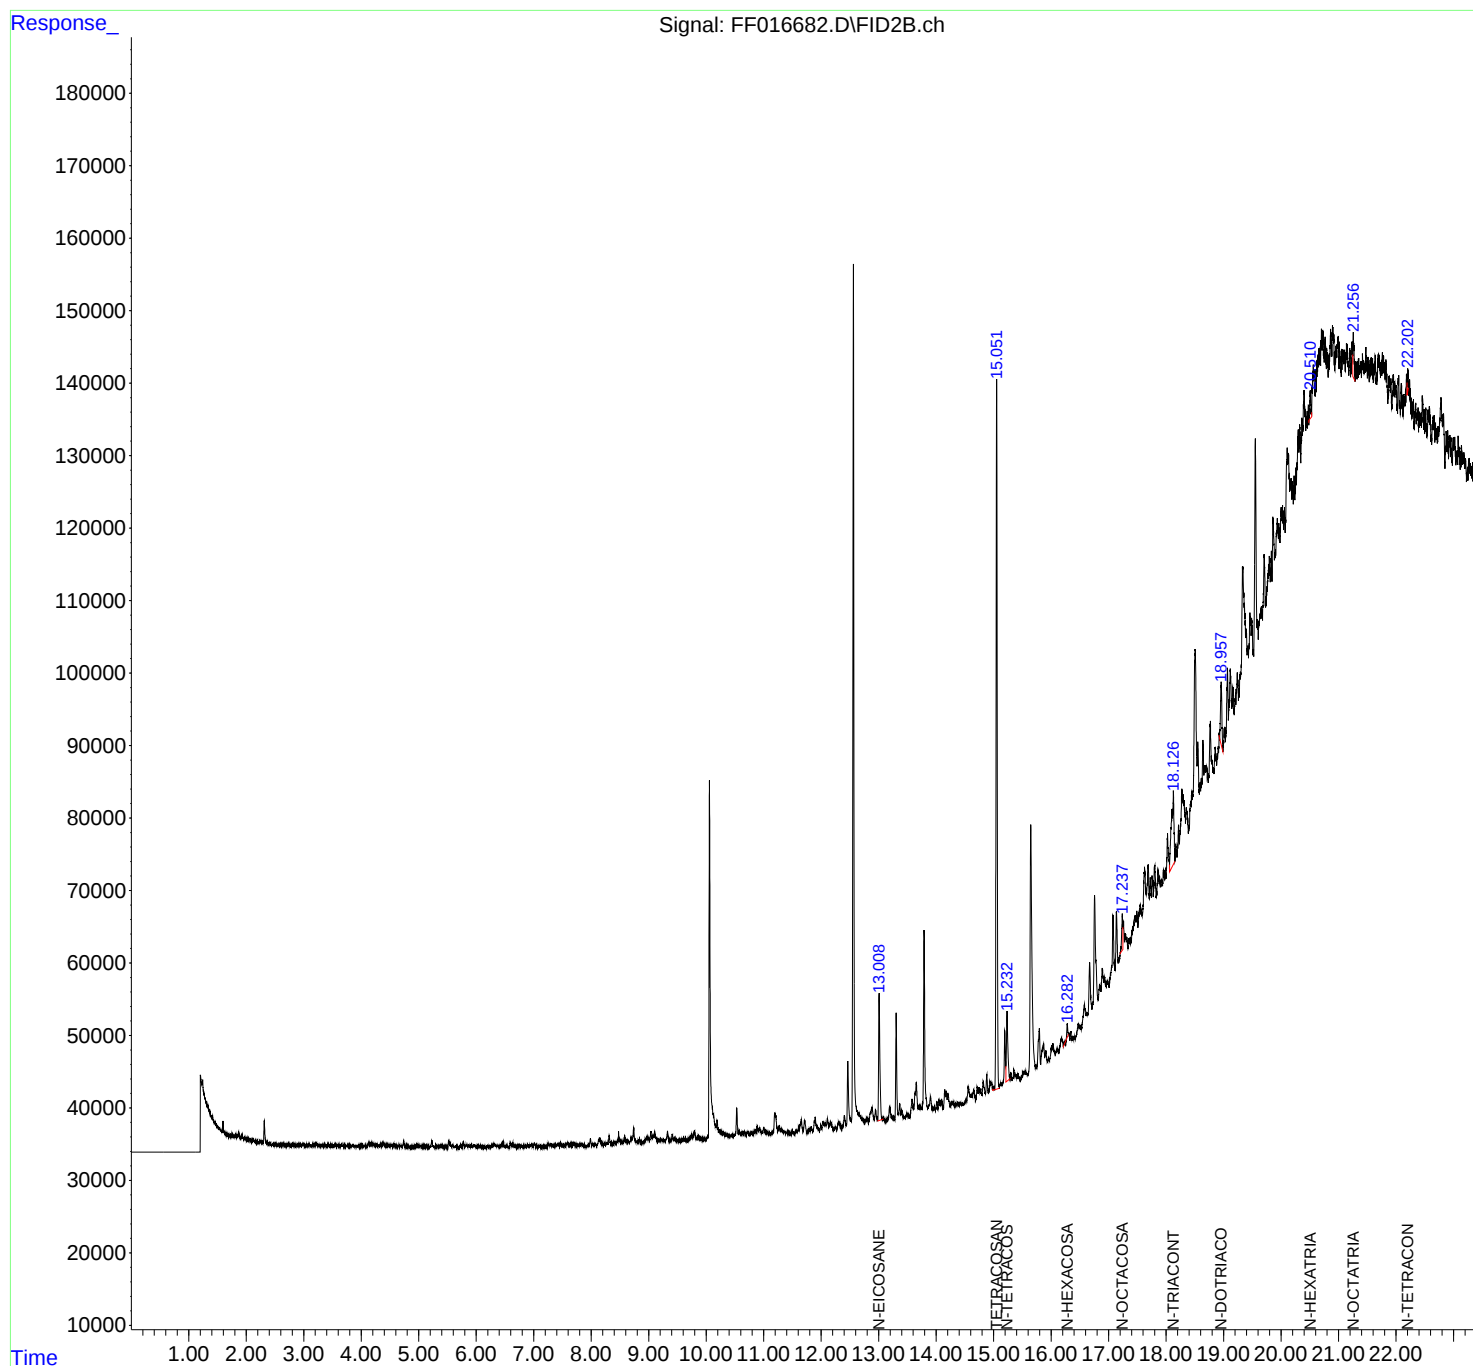


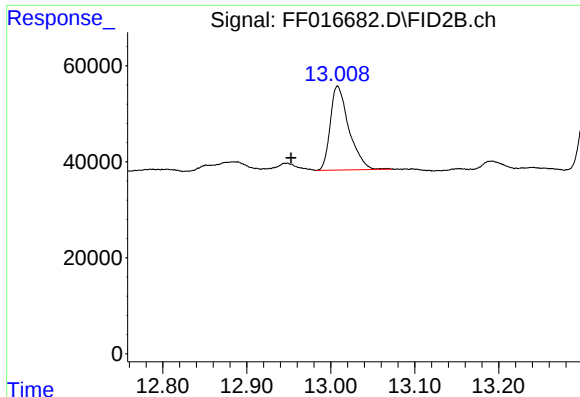

#7 N-EICOSANE


R.T.: 13.008 min
Delta R.T.: 0.055 min
Response: 269971
Conc: 2.21 ug/ml

Instrument :
FID_E
ClientSampleId :

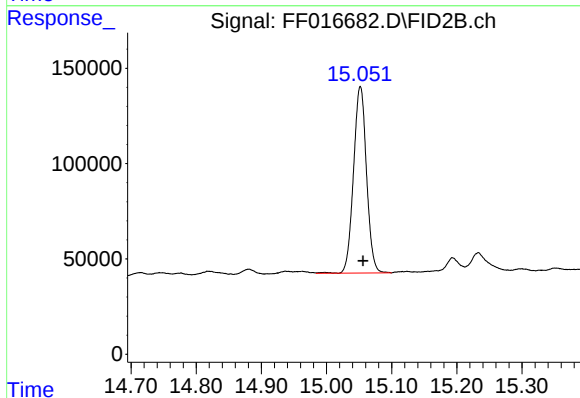


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.052 min
Delta R.T.: -0.004 min
Response: 1356662
Conc: 12.99 ug/ml

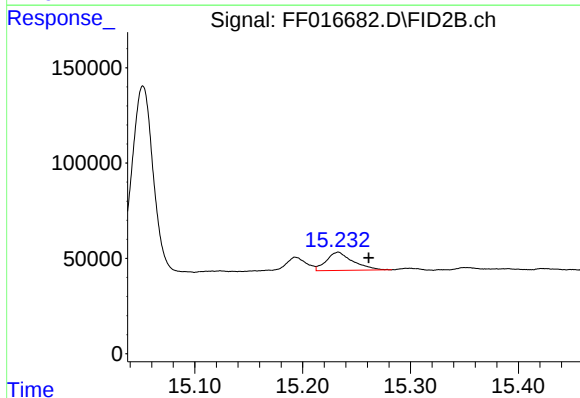


#10 N-TETRACOSANE

R.T.: 15.233 min
Delta R.T.: -0.028 min
Response: 163948
Conc: 1.38 ug/ml

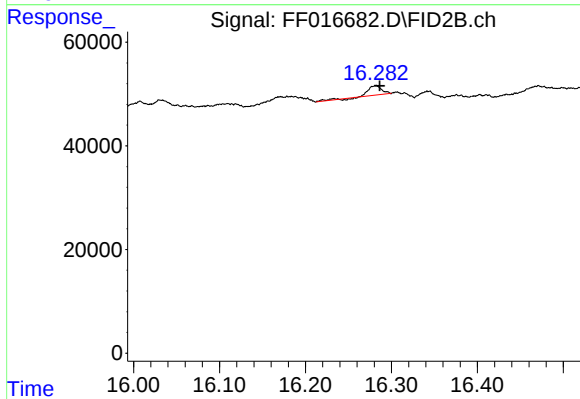

#11 N-HEXACOSANE


R.T.: 16.282 min
Delta R.T.: -0.005 min
Response: 20056
Conc: 0.17 ug/ml

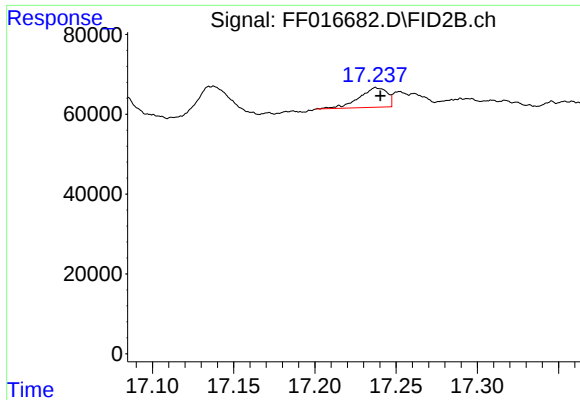

#12 N-OCTACOSANE


R.T.: 17.238 min
Delta R.T.: -0.002 min
Response: 58695
Conc: 0.52 ug/ml

Instrument :
FID_E
ClientSampleId :

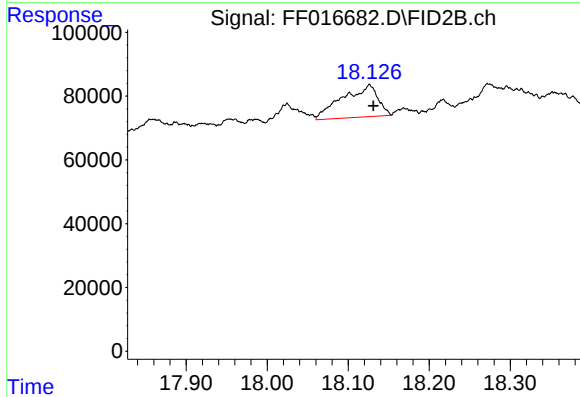


#13 N-TRIACONTANE

R.T.: 18.126 min
Delta R.T.: -0.005 min
Response: 306582
Conc: 2.73 ug/ml

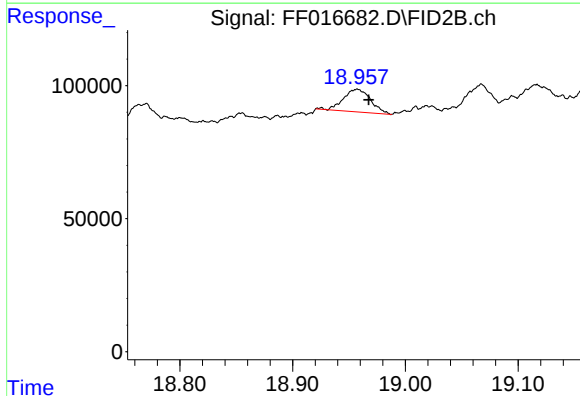


#14 N-DOTRIACONTANE

R.T.: 18.957 min
Delta R.T.: -0.010 min
Response: 143676
Conc: 1.34 ug/ml

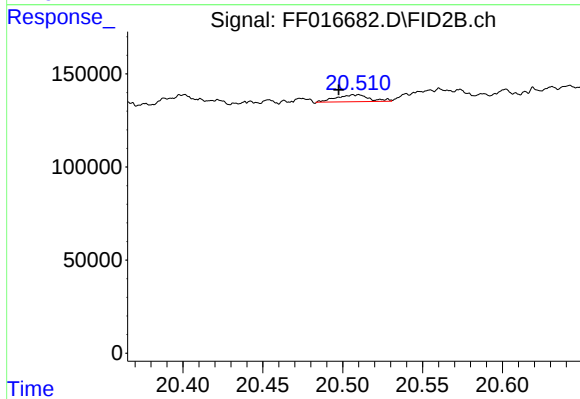

#16 N-HEXATRIACONTANE


R.T.: 20.509 min
Delta R.T.: 0.011 min
Response: 52892
Conc: 0.62 ug/ml

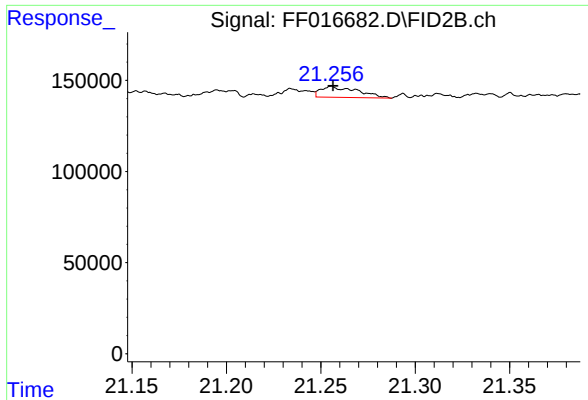

#17 N-OCTATRIACONTANE

R.T.: 21.256 min
Delta R.T.: 0.000 min
Response: 80640
Conc: 1.05 ug/ml

Instrument :
FID_E
ClientSampleId :

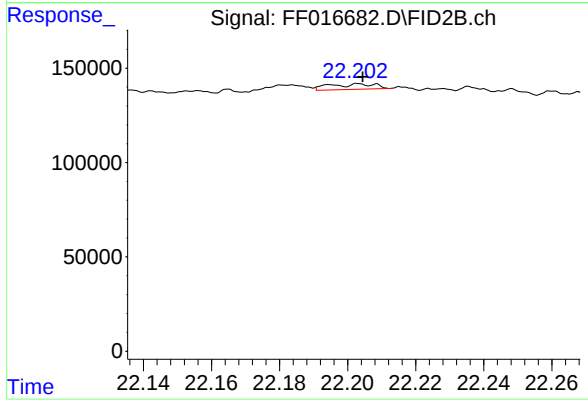

#18 N-TETRACONTANE

R.T.: 22.203 min
Delta R.T.: 0.000 min
Response: 27246
Conc: 0.40 ug/ml