

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111325\
 Data File : FF016687.D
 Signal(s) : FID2B.ch
 Acq On : 13 Nov 2025 19:01
 Operator : YP\AJ
 Sample : Q3610-04
 Misc :
 ALS Vial : 76 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 14 05:49:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102925.M
 Quant Title :
 QLast Update : Wed Oct 29 12:48:52 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.054	1359908	13.017 ug/ml
Target Compounds			
7) N-EICOSANE	13.022f	63824	0.523 ug/ml
11) N-HEXACOSANE	16.282	46690	0.406 ug/ml
12) N-OCTACOSANE	17.235	48824	0.428 ug/ml
13) N-TRIACONTANE	18.127	53585	0.477 ug/ml
14) N-DOTRIACONTANE	18.960	84203	0.785 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF111325\
Data File : FF016687.D
Signal(s) : FID2B.ch
Acq On : 13 Nov 2025 19:01
Operator : YP\AJ
Sample : Q3610-04
Misc :
ALS Vial : 76 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 14 05:49:13 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF102925.M
Quant Title :
QLast Update : Wed Oct 29 12:48:52 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

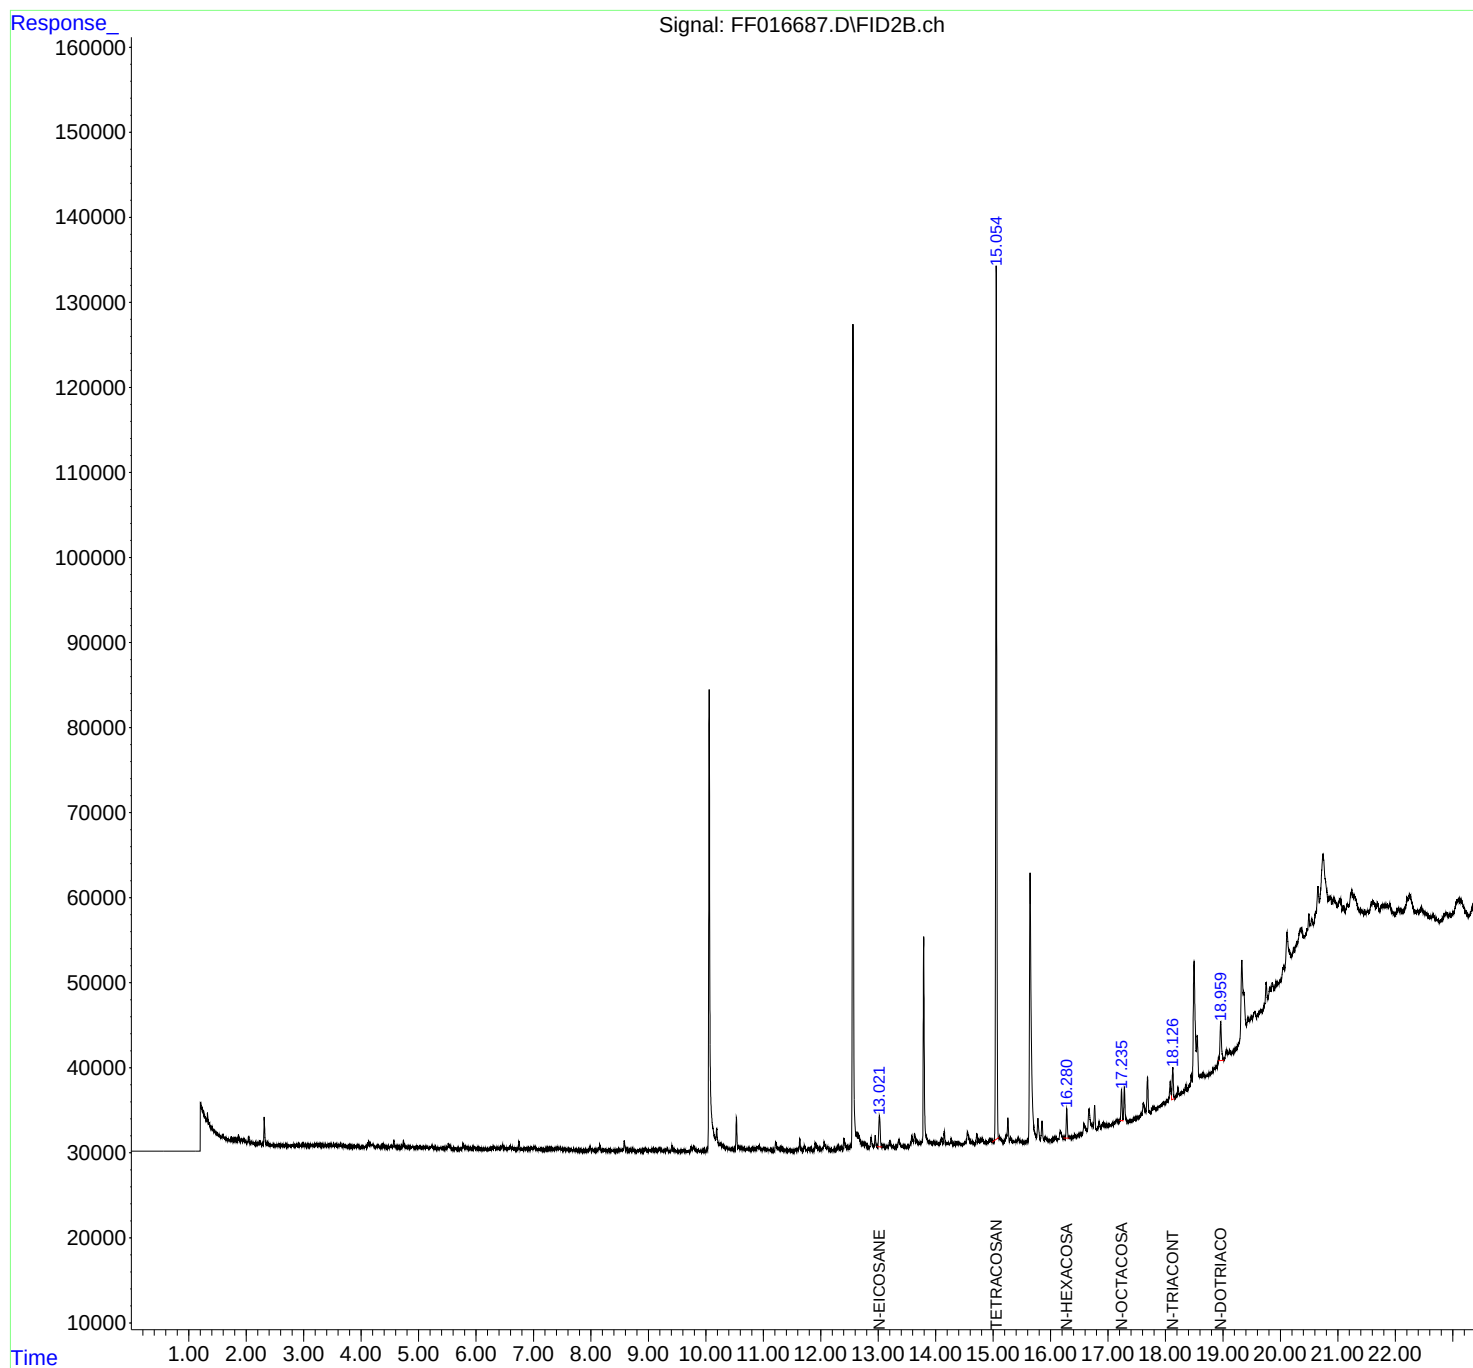


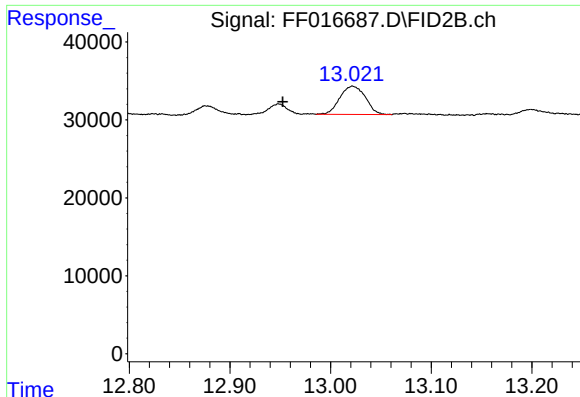

#7 N-EICOSANE


R.T.: 13.022 min
Delta R.T.: 0.069 min
Response: 63824
Conc: 0.52 ug/ml

Instrument :
FID_E
ClientSampleId :

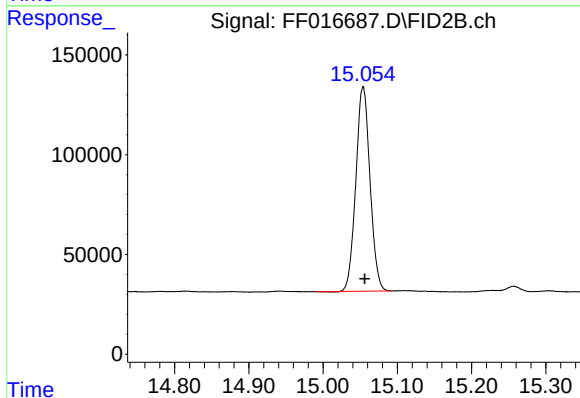


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.054 min
Delta R.T.: -0.002 min
Response: 1359908
Conc: 13.02 ug/ml

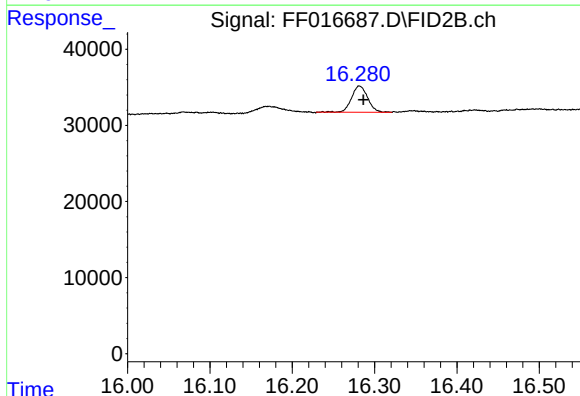


#11 N-HEXACOSANE

R.T.: 16.282 min
Delta R.T.: -0.005 min
Response: 46690
Conc: 0.41 ug/ml

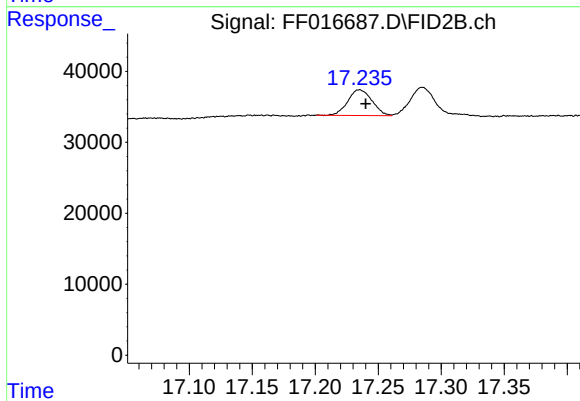

#12 N-OCTACOSANE


R.T.: 17.235 min
Delta R.T.: -0.005 min
Response: 48824
Conc: 0.43 ug/ml

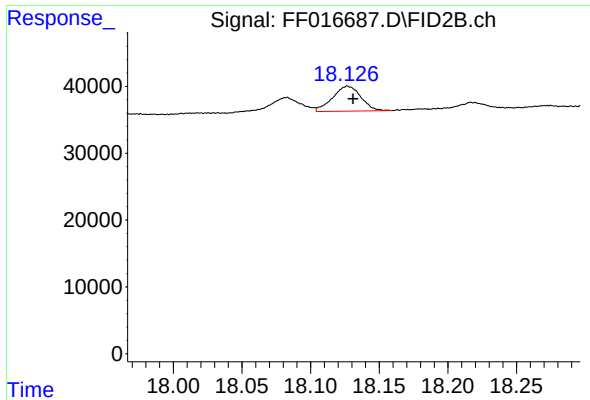

#13 N-TRIACONTANE

R.T.: 18.127 min
Delta R.T.: -0.004 min
Response: 53585
Conc: 0.48 ug/ml

Instrument :
FID_E
ClientSampleId :

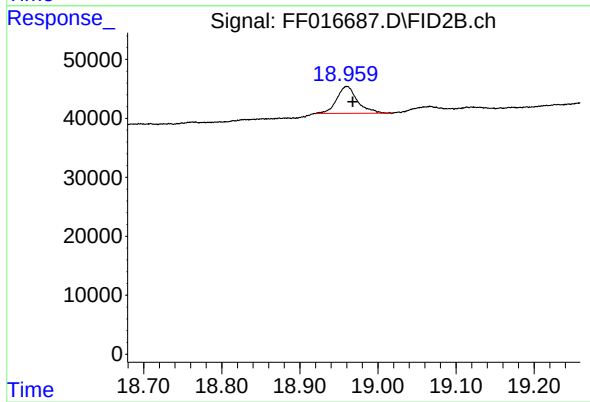

#14 N-DOTRIACONTANE

R.T.: 18.960 min
Delta R.T.: -0.007 min
Response: 84203
Conc: 0.79 ug/ml