

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111418\
Data File : FE029231.D
Signal(s) : FID1B.CH
Acq On : 14 Nov 2018 16:08
Operator : AJ\SJ
Sample : J5838-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 15 04:13:10 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE102318.M
Quant Title :
QLast Update : Wed Oct 24 08:22:18 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
6)	N-TETRADECANE	8.456	469915	3.546 ug/ml
9)	N-EICOSANE	12.843	231118	1.560 ug/ml
10)	N-TETRACOSANE	15.081	225670	1.579 ug/ml
11)	N-OCTACOSANE	17.080	113170	0.832 ug/ml
12)	N-DOTRIACONTANE	18.856	75894	0.637 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111418\
Data File : FE029231.D
Signal(s) : FID1B.CH
Acq On : 14 Nov 2018 16:08
Operator : AJ\SJ
Sample : J5838-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 15 04:13:10 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE102318.M
Quant Title :
QLast Update : Wed Oct 24 08:22:18 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

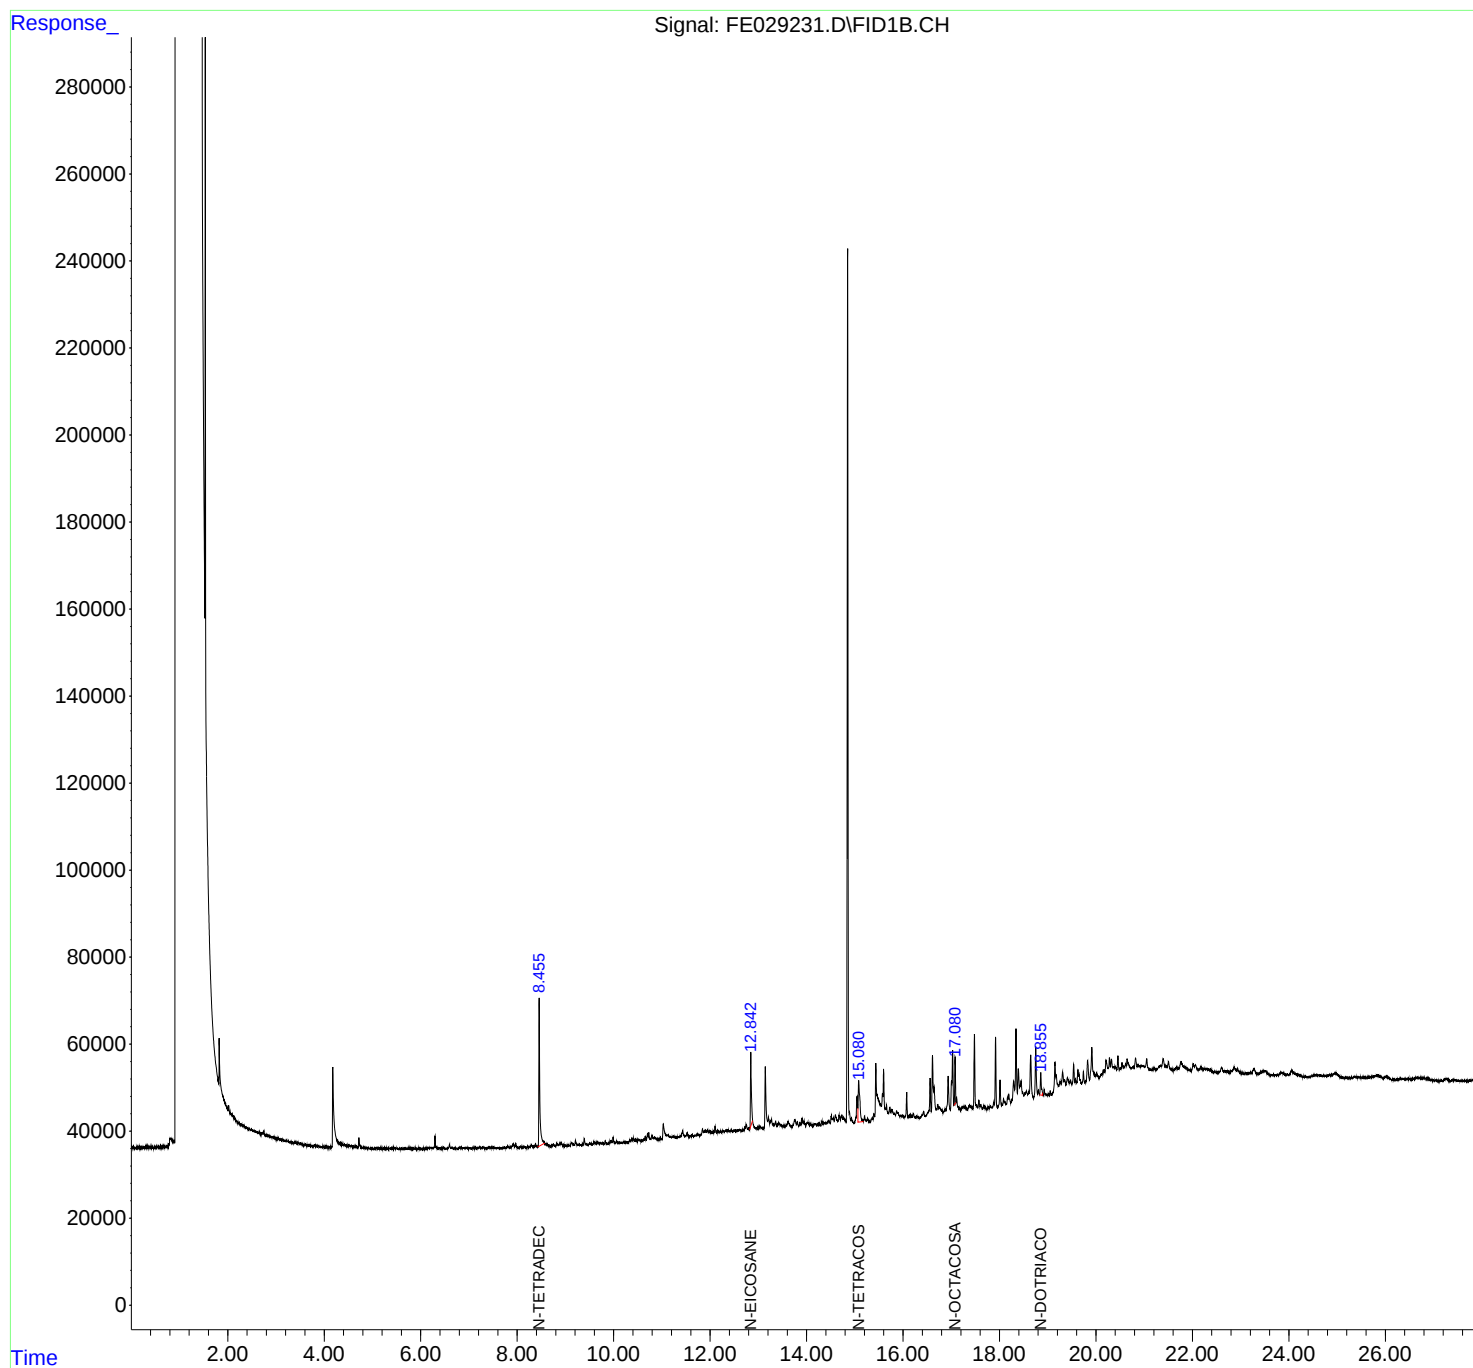

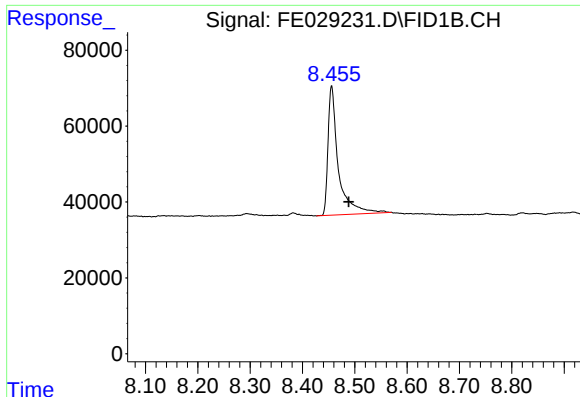


#6 N-TETRADECANE

R.T.: 8.456 min
Delta R.T.: -0.033 min
Response: 469915
Conc: 3.55 ug/ml

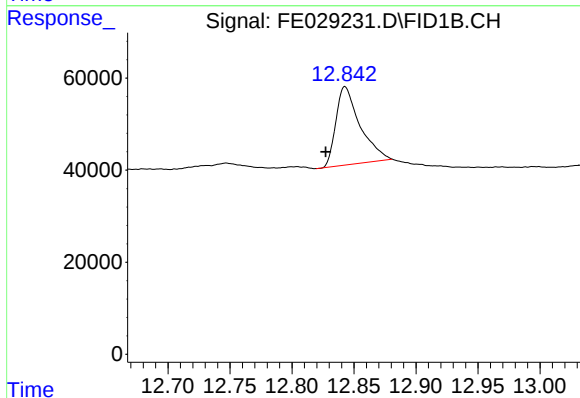


#9 N-EICOSANE

R.T.: 12.843 min
Delta R.T.: 0.016 min
Response: 231118
Conc: 1.56 ug/ml

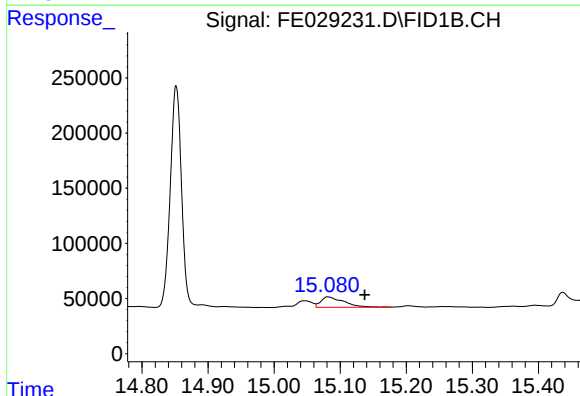


#10 N-TETRACOSANE

R.T.: 15.081 min
Delta R.T.: -0.056 min
Response: 225670
Conc: 1.58 ug/ml

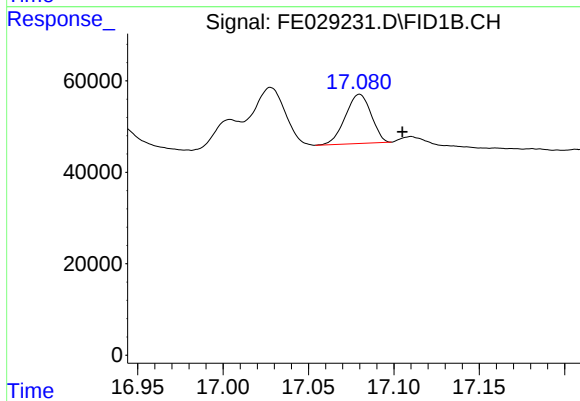


#11 N-OCTACOSANE

R.T.: 17.080 min
Delta R.T.: -0.025 min
Response: 113170
Conc: 0.83 ug/ml

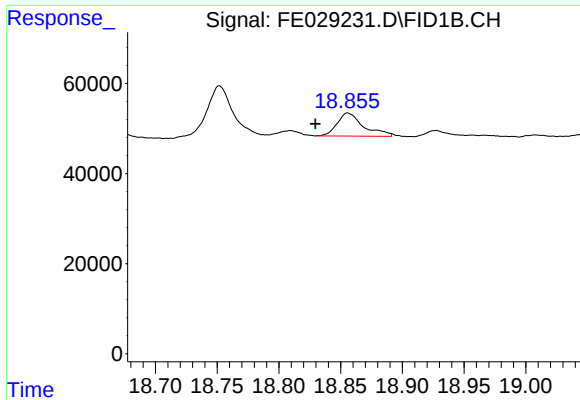

#12 N-DOTRIACONTANE

R.T.: 18.856 min
Delta R.T.: 0.026 min
Response: 75894
Conc: 0.64 ug/ml

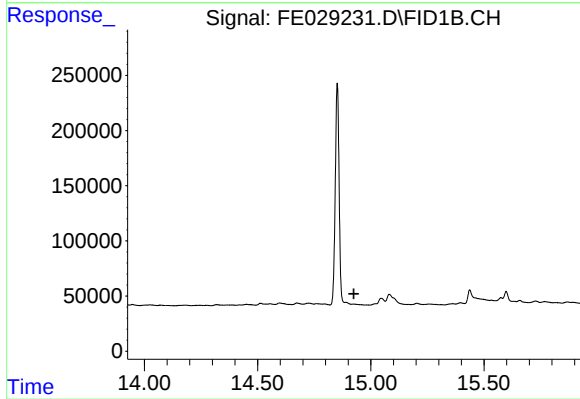

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.925 min
Response: 0
Conc: N.D.