

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111418\
Data File : FE029238.D
Signal(s) : FID1B.CH
Acq On : 14 Nov 2018 20:30
Operator : AJ\SJ
Sample : J5929-01MS
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 15 04:14:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE102318.M
Quant Title :
QLast Update : Wed Oct 24 08:22:18 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
1)	N-OCTANE	2.485	1694077	14.625 ug/ml
3)	N-DECANE	4.715	39590	0.220 ug/ml
6)	N-TETRADECANE	8.453	724851	5.470 ug/ml
9)	N-EICOSANE	12.837	338353	2.284 ug/ml
11)	N-OCTACOSANE	17.080	174090	1.279 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111418\
Data File : FE029238.D
Signal(s) : FID1B.CH
Acq On : 14 Nov 2018 20:30
Operator : AJ\SJ
Sample : J5929-01MS
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 15 04:14:22 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE102318.M
Quant Title :
QLast Update : Wed Oct 24 08:22:18 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

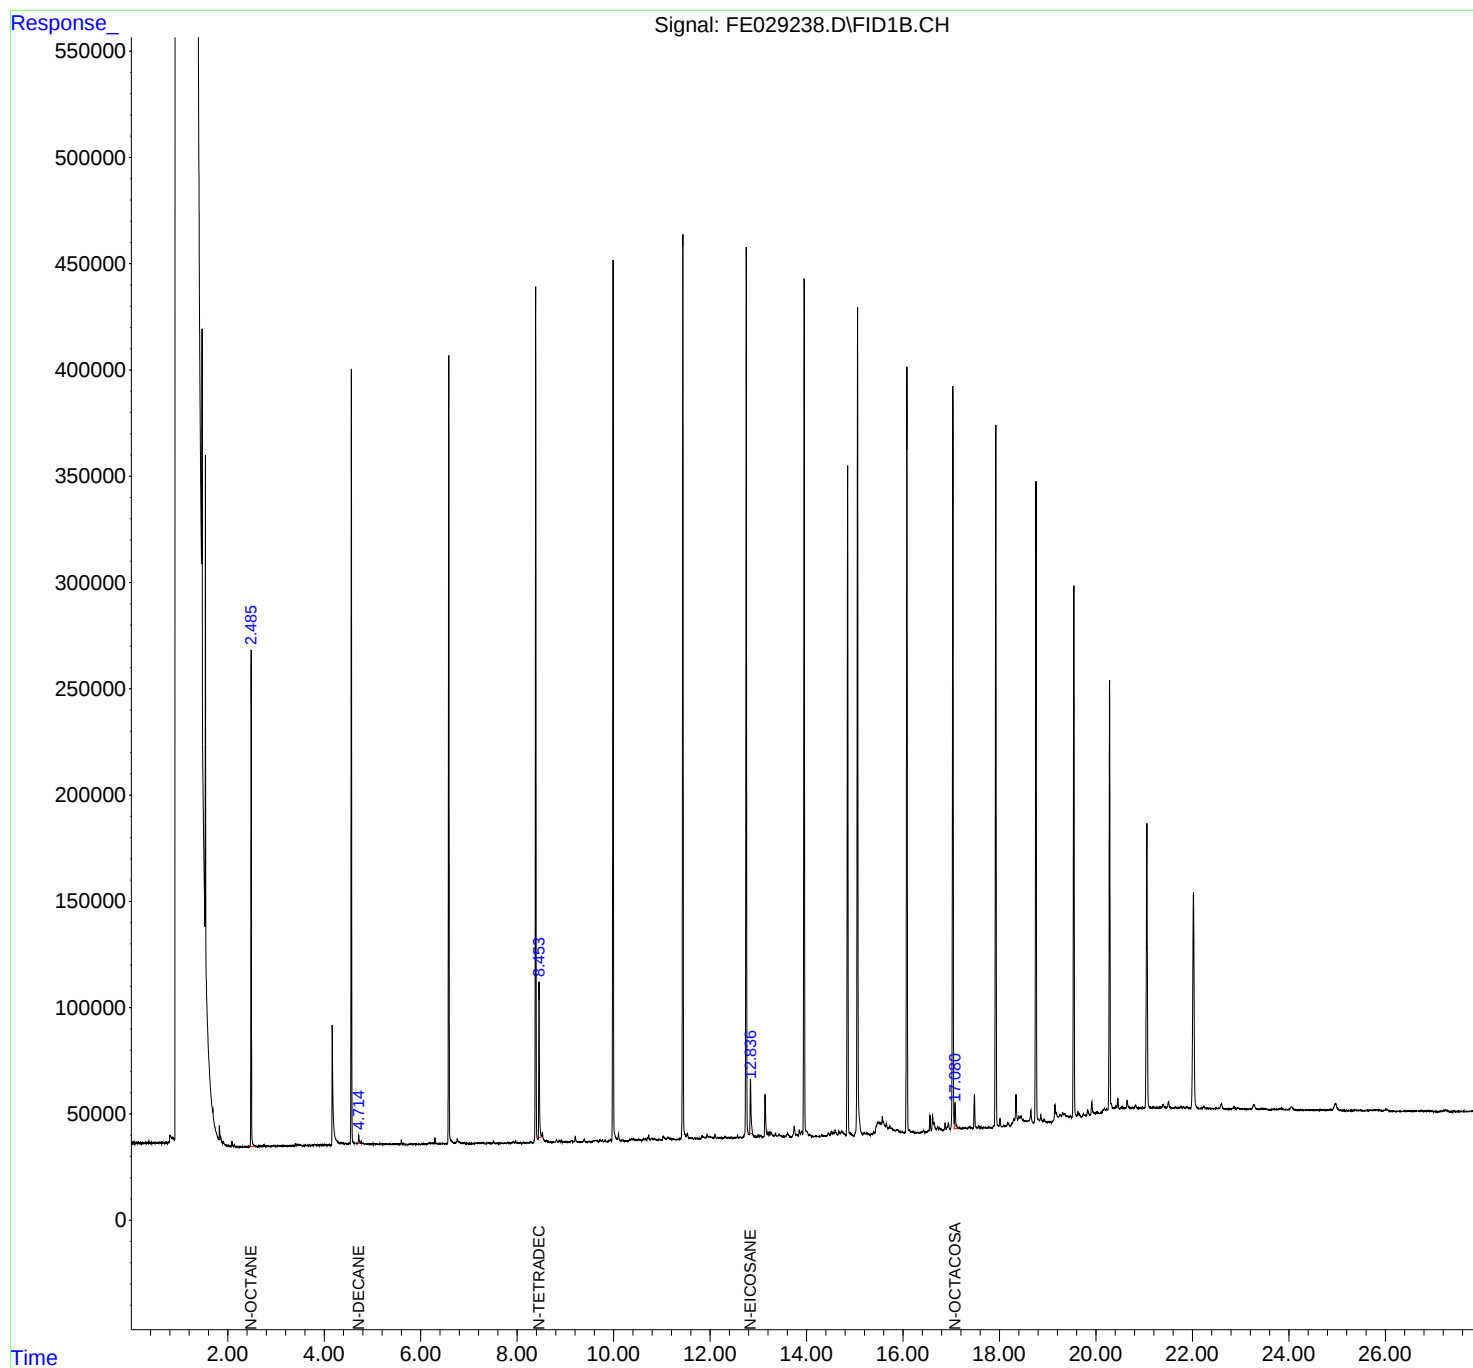

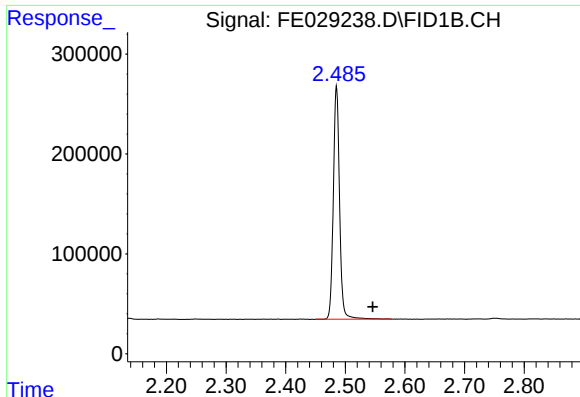


#1 N-OCTANE

R.T.: 2.485 min
Delta R.T.: -0.061 min
Response: 1694077
Conc: 14.63 ug/ml

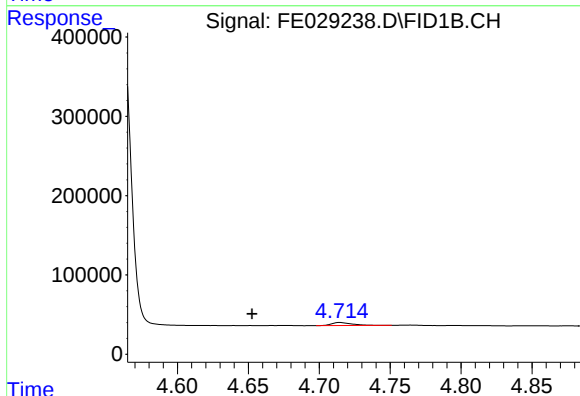


#3 N-DECANE

R.T.: 4.715 min
Delta R.T.: 0.062 min
Response: 39590
Conc: 0.22 ug/ml

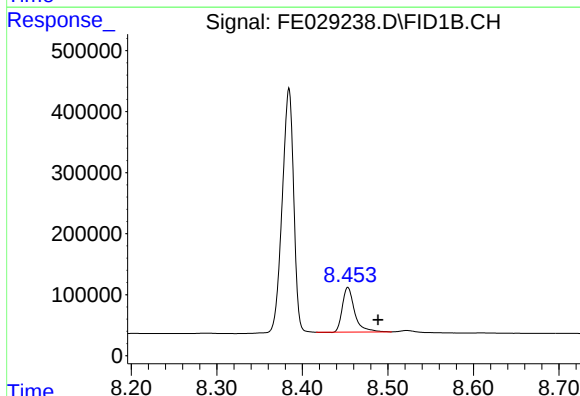


#6 N-TETRADECANE

R.T.: 8.453 min
Delta R.T.: -0.035 min
Response: 724851
Conc: 5.47 ug/ml

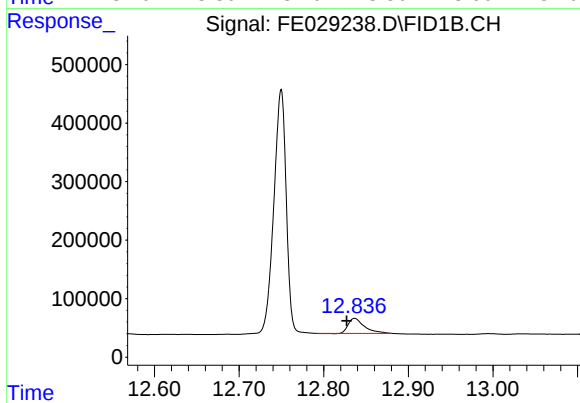


#9 N-EICOSANE

R.T.: 12.837 min
Delta R.T.: 0.009 min
Response: 338353
Conc: 2.28 ug/ml

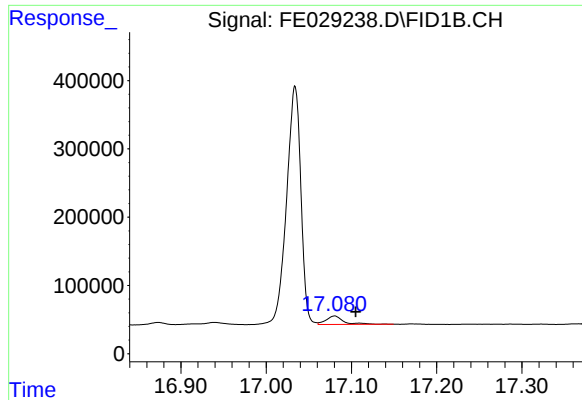

#11 N-OCTACOSANE

R.T.: 17.080 min
Delta R.T.: -0.025 min
Response: 174090
Conc: 1.28 ug/ml

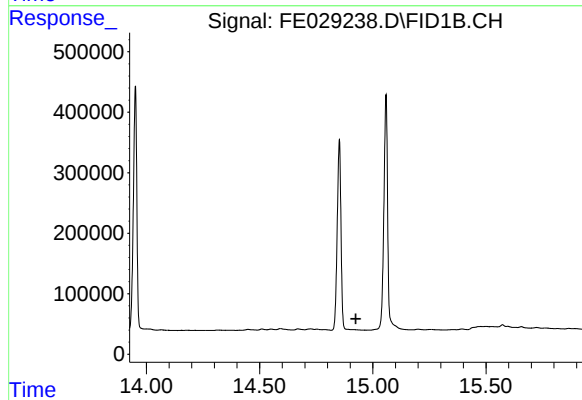

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.925 min
Response: 0
Conc: N.D.