

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111418\
 Data File : FE029241.D
 Signal(s) : FID1B.CH
 Acq On : 14 Nov 2018 22:22
 Operator : AJ\SJ
 Sample : 4400 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 15 04:14:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE102318.M
 Quant Title :
 QLast Update : Wed Oct 24 08:22:18 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.859	8433829	50.198 ug/ml
Target Compounds			
1) N-OCTANE	2.498	42423034	366.251 ug/ml
2) N-NONANE	3.555	220882	1.874 ug/ml
3) N-DECANE	4.626	366225	2.040 ug/ml
4) N-UNDECANE	5.641	77018012	603.875 ug/ml
5) N-DODECANE	6.627	78490589	608.190 ug/ml
7) N-HEXADECANE	10.037	71924259	509.668 ug/ml
8) N-OCTADECANE	11.531	151273	1.030 ug/ml
9) N-EICOSANE	12.764	14666054	98.992 ug/ml
10) N-TETRACOSANE	15.072	14620855	102.309 ug/ml
11) N-OCTACOSANE	17.038	6926374	50.901 ug/ml
12) N-DOTRIACONTANE	18.762	5826750	48.891 ug/ml
14) N-HEXATRIACONTANE	20.287	4925288	51.037 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111418\
Data File : FE029241.D
Signal(s) : FID1B.CH
Acq On : 14 Nov 2018 22:22
Operator : AJ\SJ
Sample : 4400 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 15 04:14:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE102318.M
Quant Title :
QLast Update : Wed Oct 24 08:22:18 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

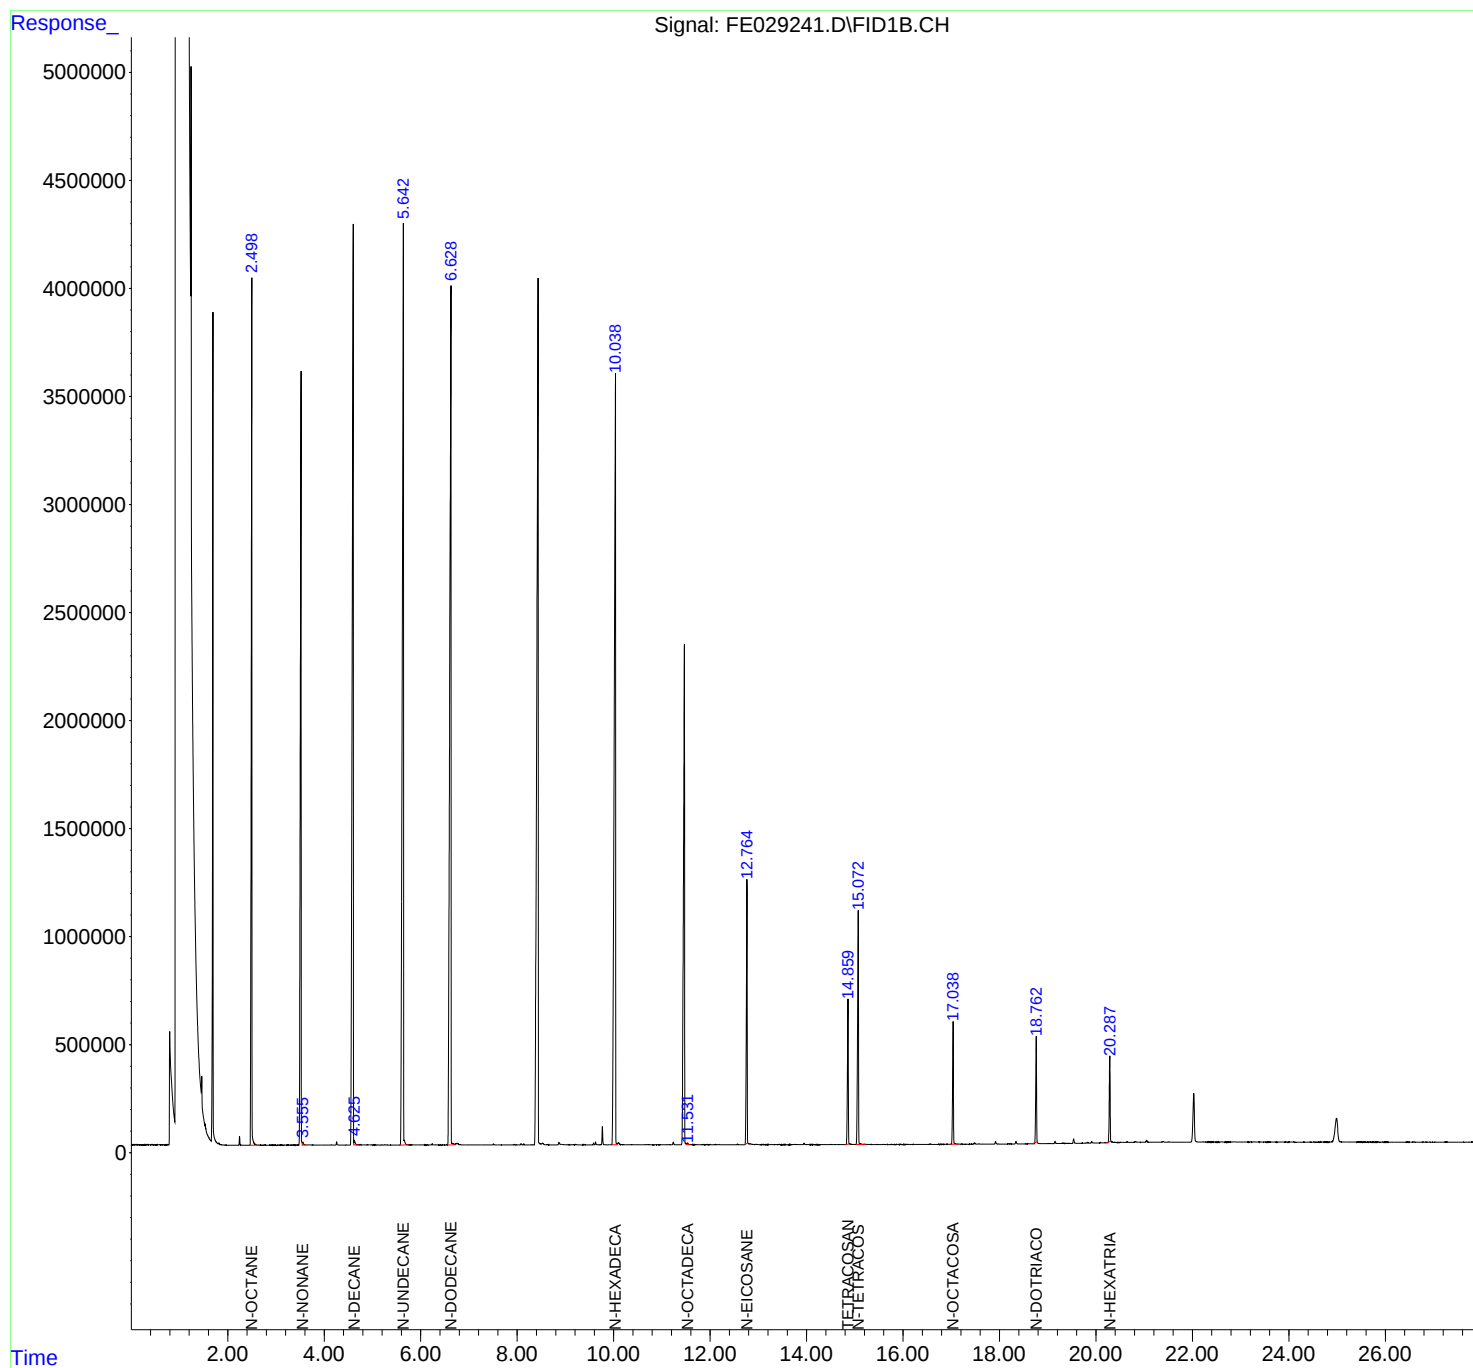

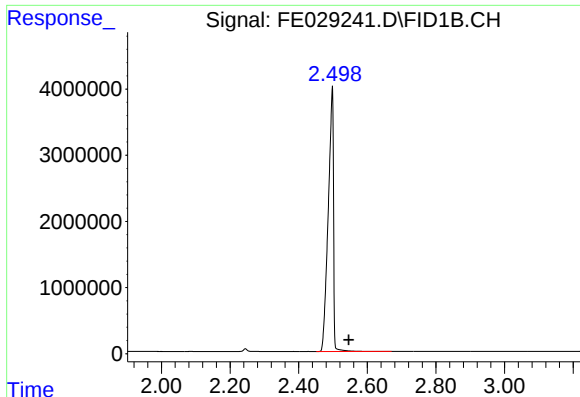


#1 N-OCTANE

R.T.: 2.498 min
Delta R.T.: -0.049 min
Response: 42423034
Conc: 366.25 ug/ml

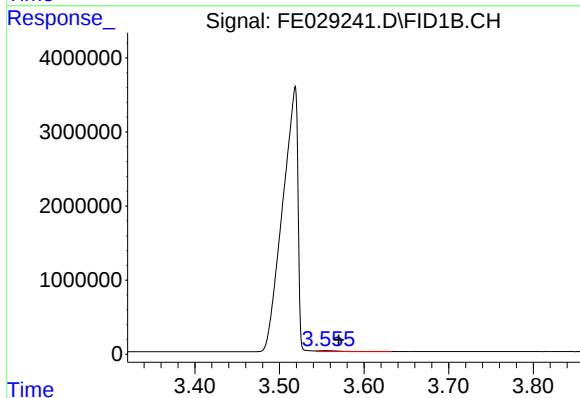


#2 N-NONANE

R.T.: 3.555 min
Delta R.T.: -0.015 min
Response: 220882
Conc: 1.87 ug/ml

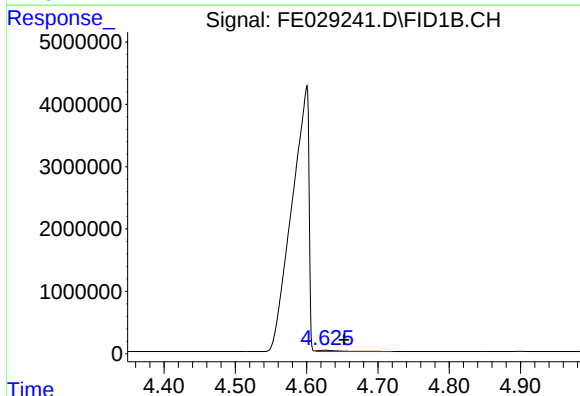


#3 N-DECANE

R.T.: 4.626 min
Delta R.T.: -0.027 min
Response: 366225
Conc: 2.04 ug/ml

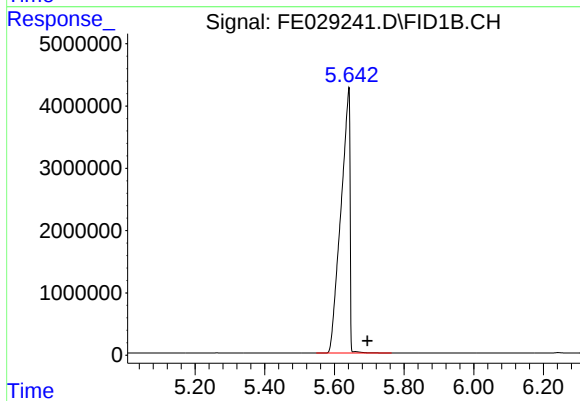


#4 N-UNDECANE

R.T.: 5.641 min
Delta R.T.: -0.054 min
Response: 77018012
Conc: 603.87 ug/ml

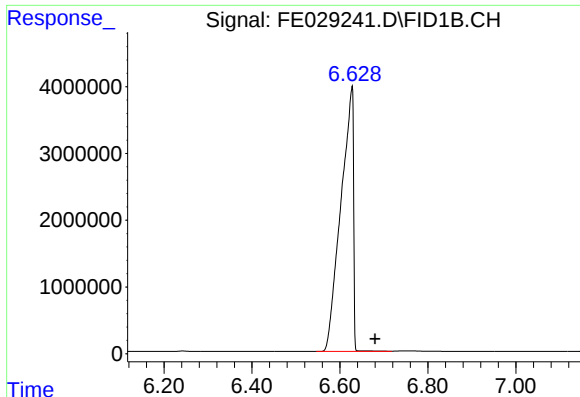


#5 N-DODECANE

R.T.: 6.627 min
Delta R.T.: -0.053 min
Response: 78490589
Conc: 608.19 ug/ml

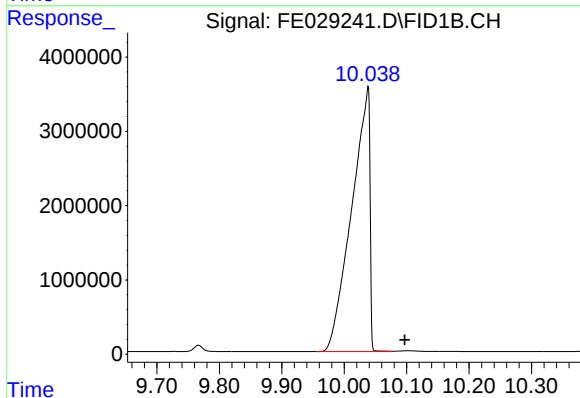


#7 N-HEXADECANE

R.T.: 10.037 min
Delta R.T.: -0.059 min
Response: 71924259
Conc: 509.67 ug/ml

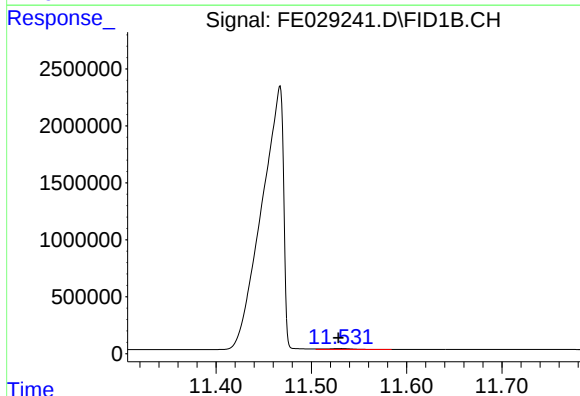


#8 N-OCTADECANE

R.T.: 11.531 min
Delta R.T.: 0.003 min
Response: 151273
Conc: 1.03 ug/ml

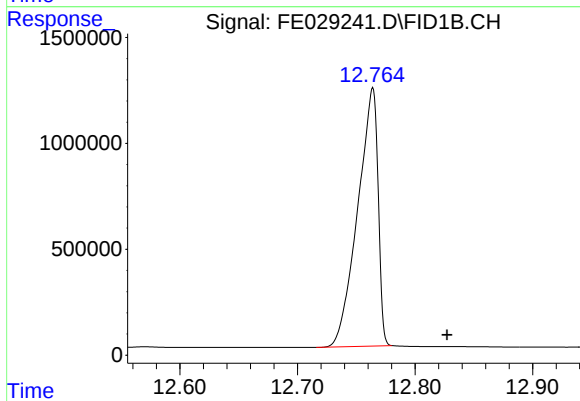


#9 N-EICOSANE

R.T.: 12.764 min
Delta R.T.: -0.063 min
Response: 14666054
Conc: 98.99 ug/ml

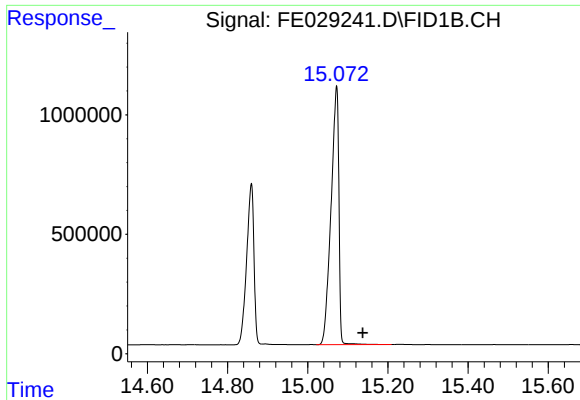


#10 N-TETRACOSANE

R.T.: 15.072 min
Delta R.T.: -0.065 min
Response: 14620855
Conc: 102.31 ug/ml

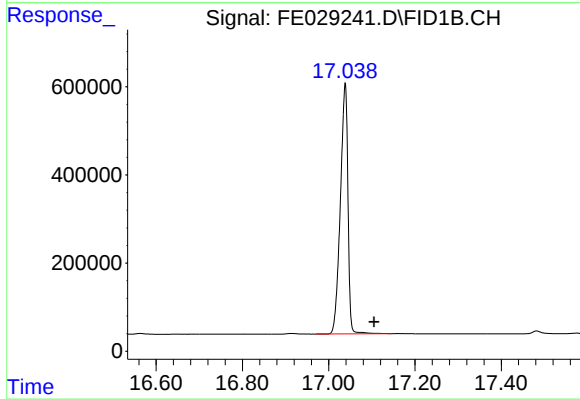


#11 N-OCTACOSANE

R.T.: 17.038 min
Delta R.T.: -0.067 min
Response: 6926374
Conc: 50.90 ug/ml

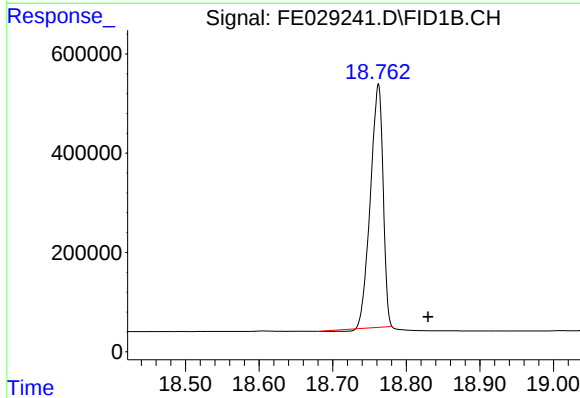


#12 N-DOTRIACONTANE

R.T.: 18.762 min
Delta R.T.: -0.067 min
Response: 5826750
Conc: 48.89 ug/ml

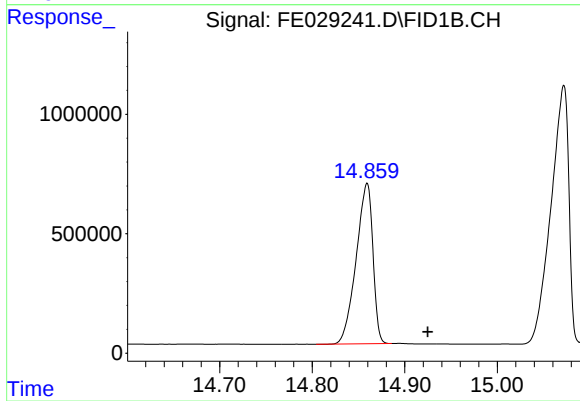

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.859 min
Delta R.T.: -0.066 min
Response: 8433829
Conc: 50.20 ug/ml

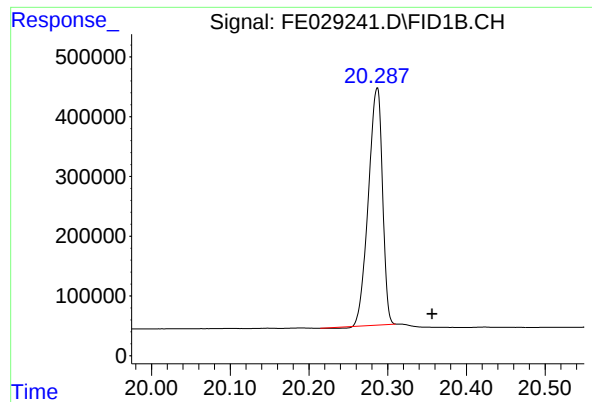

#14 N-HEXATRIACONTANE

R.T.: 20.287 min
Delta R.T.: -0.070 min
Response: 4925288
Conc: 51.04 ug/ml