

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111519\
 Data File : FE030876.D
 Signal(s) : FID1B.CH
 Acq On : 15 Nov 2019 21:31
 Operator : DD\AJ
 Sample : K5671-06 10X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 15 22:42:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
 Quant Title :
 QLast Update : Thu Oct 31 08:47:02 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.651	512050	1.648 ug/ml
Target Compounds			
4) N-TETRADECANE	8.251	180643	0.482 ug/ml
7) N-EICOSANE	12.607	1994678	5.458 ug/ml
8) N-DOCOSANE	13.771	396157	1.102 ug/ml
10) N-TETRACOSANE	14.826	971709	2.732 ug/ml
12) N-OCTACOSANE	16.829	531494	1.559 ug/ml
13) N-TRIACONTANE	17.716	530202	1.596 ug/ml
14) N-DOTRIACONTANE	18.548	243638	0.763 ug/ml
18) N-TETRACONTANE	21.712	505407	1.924 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111519\
Data File : FE030876.D
Signal(s) : FID1B.CH
Acq On : 15 Nov 2019 21:31
Operator : DD\AJ
Sample : K5671-06 10X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 15 22:42:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
Quant Title :
QLast Update : Thu Oct 31 08:47:02 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

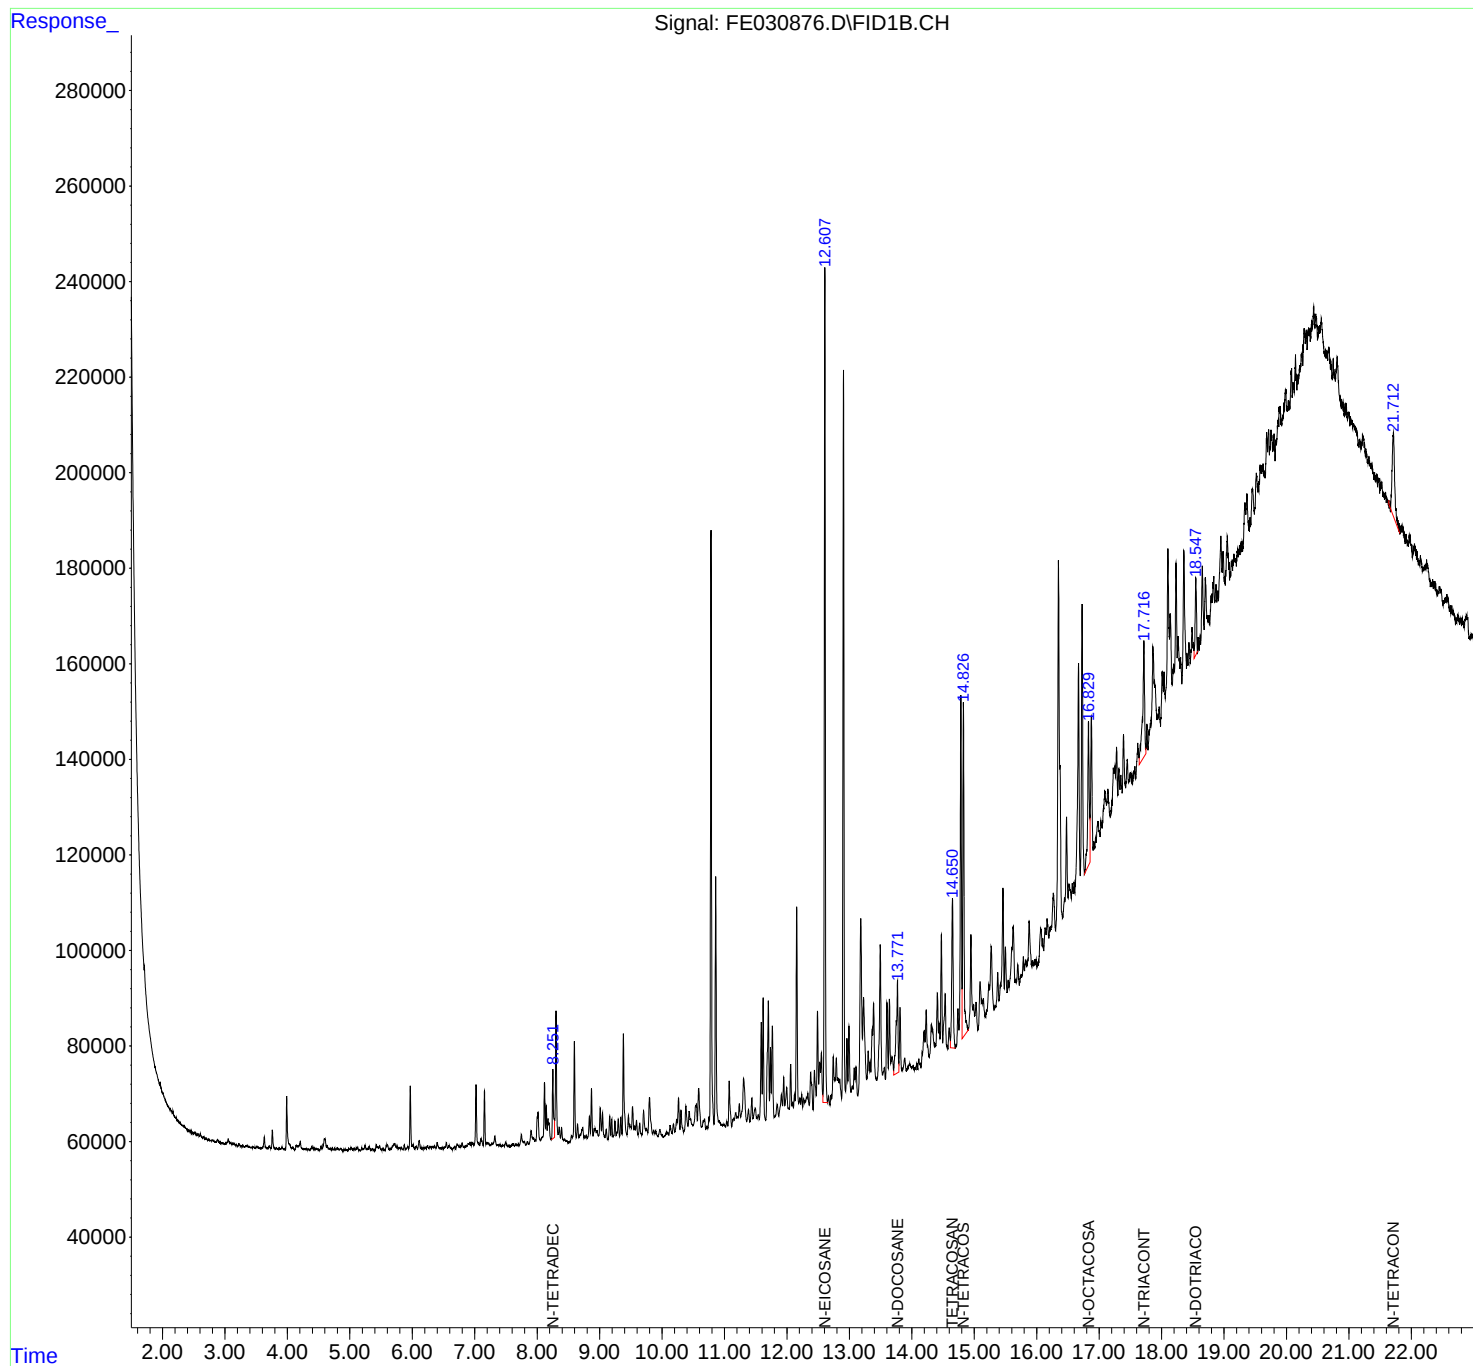


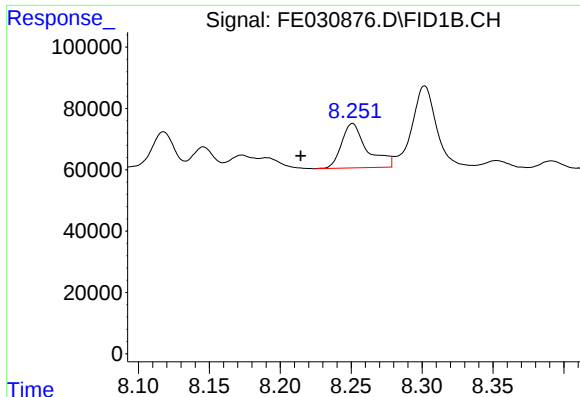

#4 N-TETRADECANE


R.T.: 8.251 min
Delta R.T.: 0.037 min
Response: 180643
Conc: 0.48 ug/ml

Instrument :
FID_E
ClientSampleId :

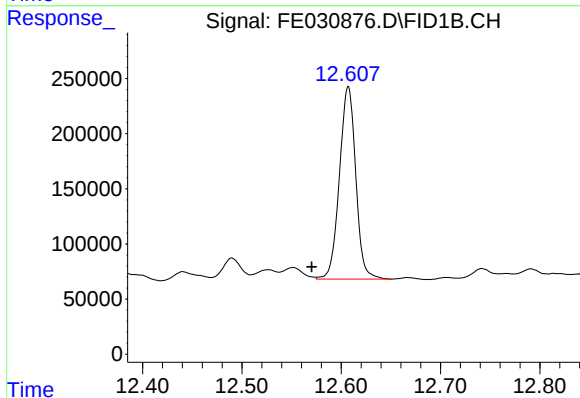


#7 N-EICOSANE

R.T.: 12.607 min
Delta R.T.: 0.037 min
Response: 1994678
Conc: 5.46 ug/ml

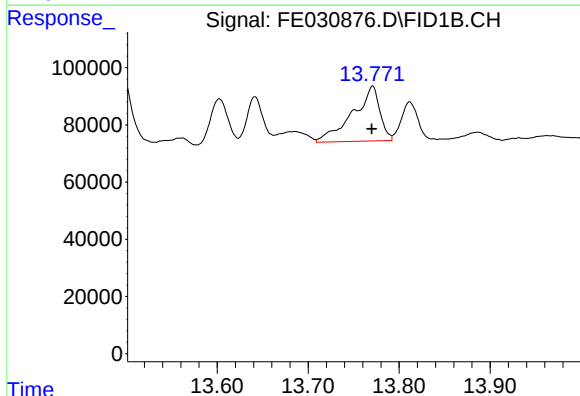


#8 N-DOCOSANE

R.T.: 13.771 min
Delta R.T.: 0.000 min
Response: 396157
Conc: 1.10 ug/ml

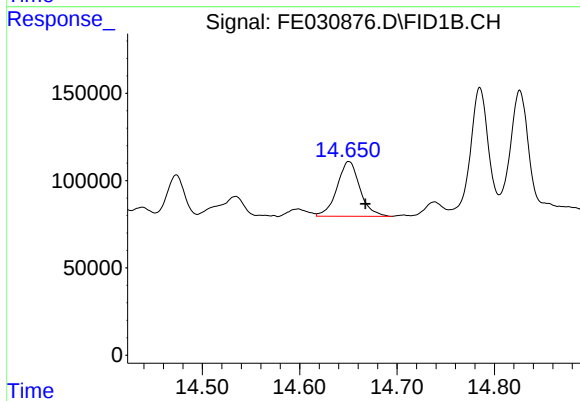

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.651 min
Delta R.T.: -0.017 min
Response: 512050
Conc: 1.65 ug/ml

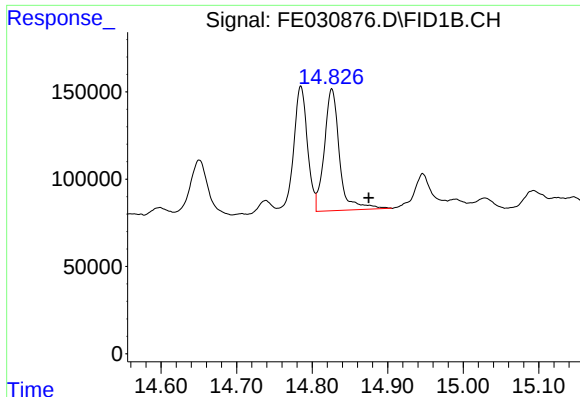

#10 N-TETRACOSANE


R.T.: 14.826 min
Delta R.T.: -0.049 min
Response: 971709
Conc: 2.73 ug/ml

Instrument :
FID_E
ClientSampleId :

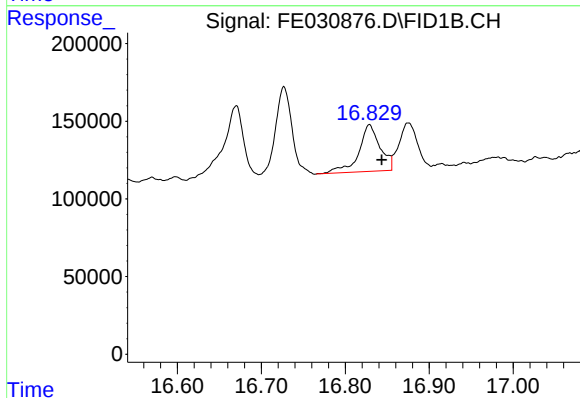


#12 N-OCTACOSANE

R.T.: 16.829 min
Delta R.T.: -0.014 min
Response: 531494
Conc: 1.56 ug/ml

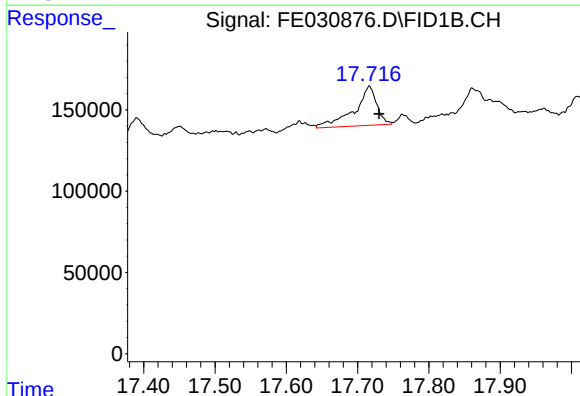


#13 N-TRIACONTANE

R.T.: 17.716 min
Delta R.T.: -0.014 min
Response: 530202
Conc: 1.60 ug/ml

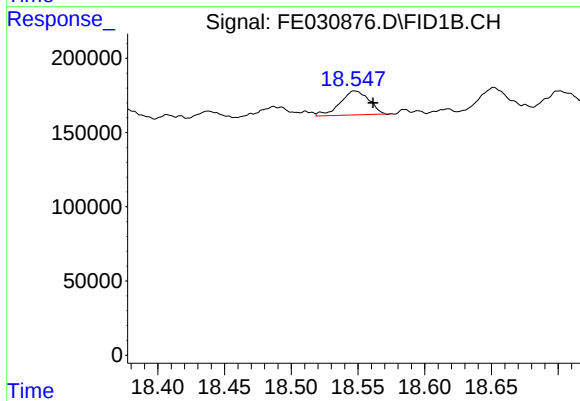

#14 N-DOTRIACONTANE

R.T.: 18.548 min
Delta R.T.: -0.013 min
Response: 243638
Conc: 0.76 ug/ml

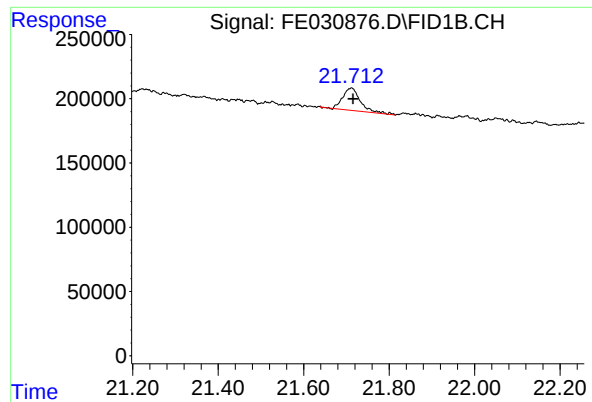

#18 N-TETRACONTANE

R.T.: 21.712 min
Delta R.T.: -0.004 min
Response: 505407
Conc: 1.92 ug/ml

Instrument :
FID_E
ClientSampleId :