

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111519\
 Data File : FE030880.D
 Signal(s) : FID1B.CH
 Acq On : 15 Nov 2019 23:45
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 16 00:42:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
 Quant Title :
 QLast Update : Thu Oct 31 08:47:02 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.658	6278086	20.200 ug/ml
Target Compounds			
12) N-OCTACOSANE	16.829	272424	0.799 ug/ml
13) N-TRIACONTANE	17.718	515004	1.551 ug/ml
14) N-DOTRIACONTANE	18.551	661252	2.071 ug/ml
15) N-TETRATRIACONTANE	19.336	561077	1.843 ug/ml
16) N-HEXATRIACONTANE	20.079	1537910	5.602 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111519\
Data File : FE030880.D
Signal(s) : FID1B.CH
Acq On : 15 Nov 2019 23:45
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 16 00:42:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
Quant Title :
QLast Update : Thu Oct 31 08:47:02 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

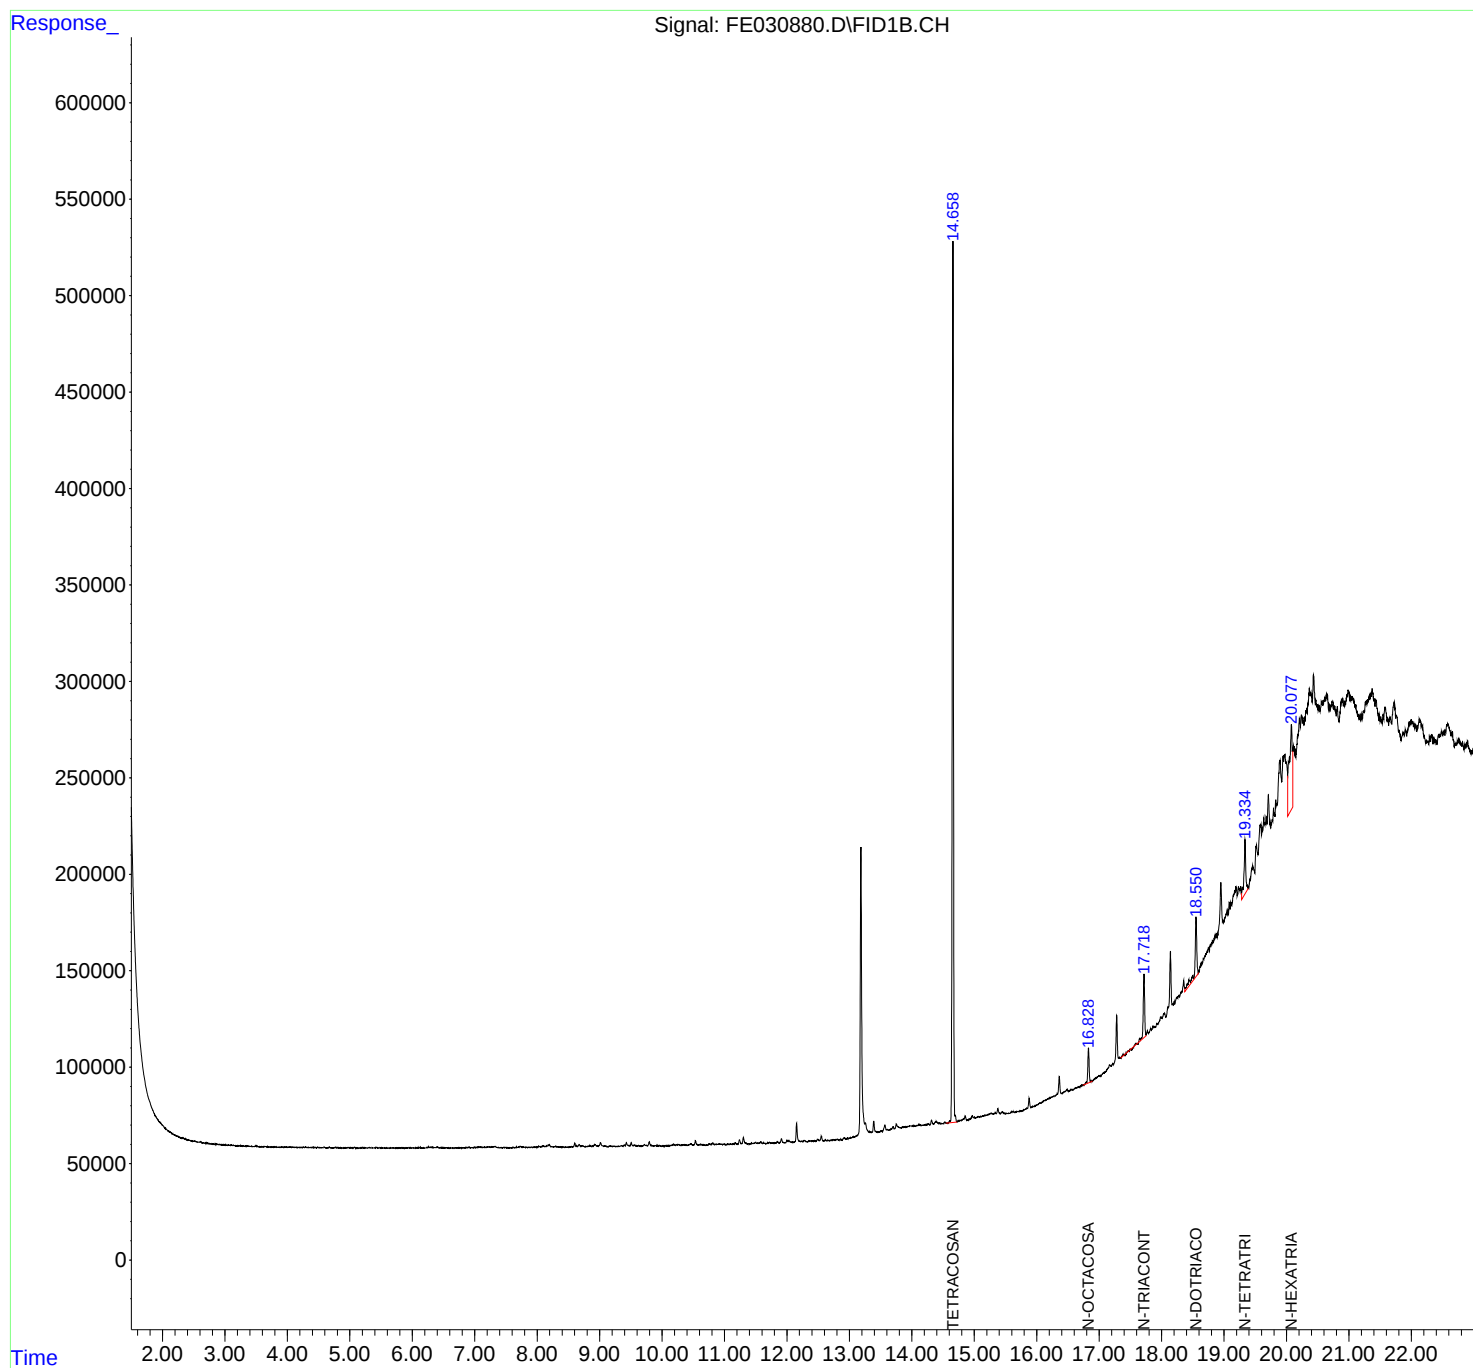


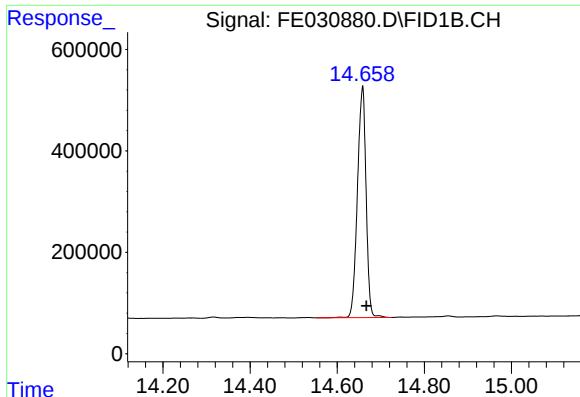

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.658 min
Delta R.T.: -0.010 min
Response: 6278086
Conc: 20.20 ug/ml

Instrument :
FID_E
ClientSampleId :

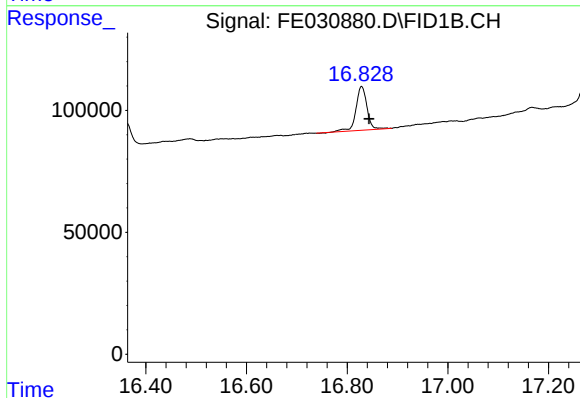


#12 N-OCTACOSANE

R.T.: 16.829 min
Delta R.T.: -0.015 min
Response: 272424
Conc: 0.80 ug/ml

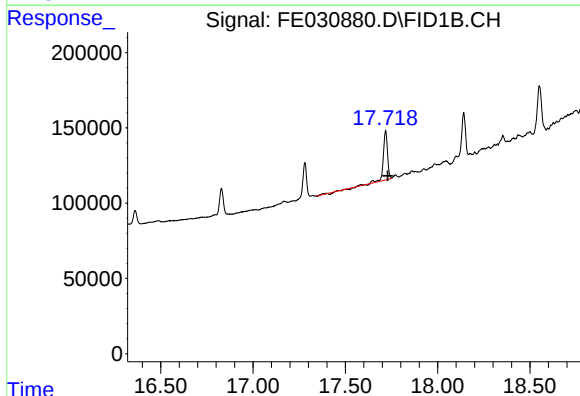


#13 N-TRIACONTANE

R.T.: 17.718 min
Delta R.T.: -0.012 min
Response: 515004
Conc: 1.55 ug/ml

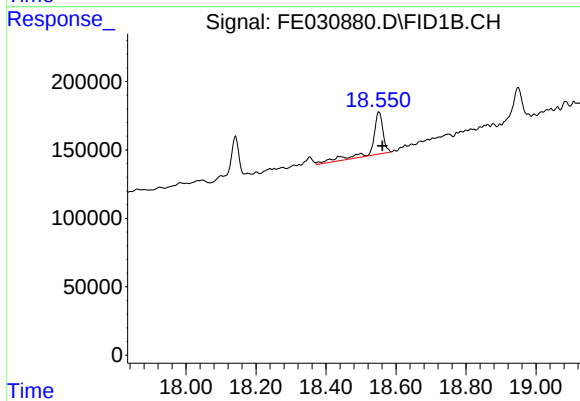

#14 N-DOTRIACONTANE

R.T.: 18.551 min
Delta R.T.: -0.010 min
Response: 661252
Conc: 2.07 ug/ml

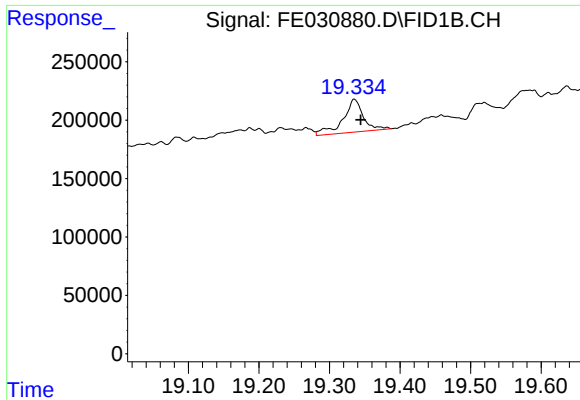

#15 N-TETRATRIACONTANE


R.T.: 19.336 min

Delta R.T.: -0.008 min

Response: 561077

Conc: 1.84 ug/ml

Instrument :
FID_E
ClientSampleId :

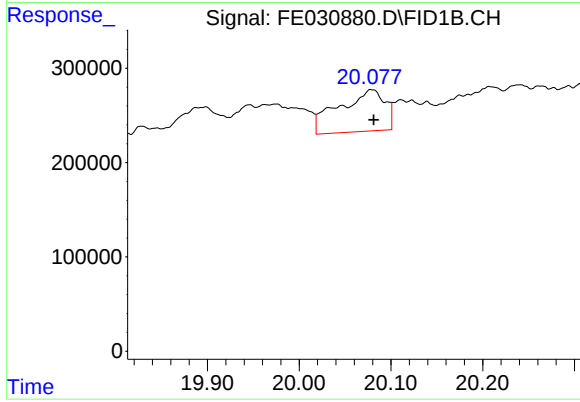

#16 N-HEXATRIACONTANE

R.T.: 20.079 min

Delta R.T.: -0.002 min

Response: 1537910

Conc: 5.60 ug/ml