

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111519\
 Data File : FE030867.D
 Signal(s) : FID1B.CH
 Acq On : 15 Nov 2019 16:29
 Operator : DD\AJ
 Sample : PB124840BS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 PB124840BS

Integration File: autoint1.e
 Quant Time: Nov 15 22:40:20 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
 Quant Title :
 QLast Update : Thu Oct 31 08:47:02 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.660	5672596	18.252 ug/ml
Target Compounds			
2) N-DECANE	4.393	6966355	18.308 ug/ml
3) N-DODECANE	6.404	7004752	18.409 ug/ml
4) N-TETRADECANE	8.200	6912733	18.460 ug/ml
5) N-HEXADECANE	9.803	6893041	18.482 ug/ml
6) N-OCTADECANE	11.247	6789523	18.569 ug/ml
7) N-EICOSANE	12.559	6697998	18.327 ug/ml
8) N-DOCOSANE	13.759	6581279	18.307 ug/ml
10) N-TETRACOSANE	14.864	6478022	18.212 ug/ml
11) N-HEXACOSANE	15.886	6365345	18.252 ug/ml
12) N-OCTACOSANE	16.838	6319569	18.536 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111519\
Data File : FE030867.D
Signal(s) : FID1B.CH
Acq On : 15 Nov 2019 16:29
Operator : DD\AJ
Sample : PB124840BS
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB124840BS

Integration File: autoint1.e
Quant Time: Nov 15 22:40:20 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
Quant Title :
QLast Update : Thu Oct 31 08:47:02 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

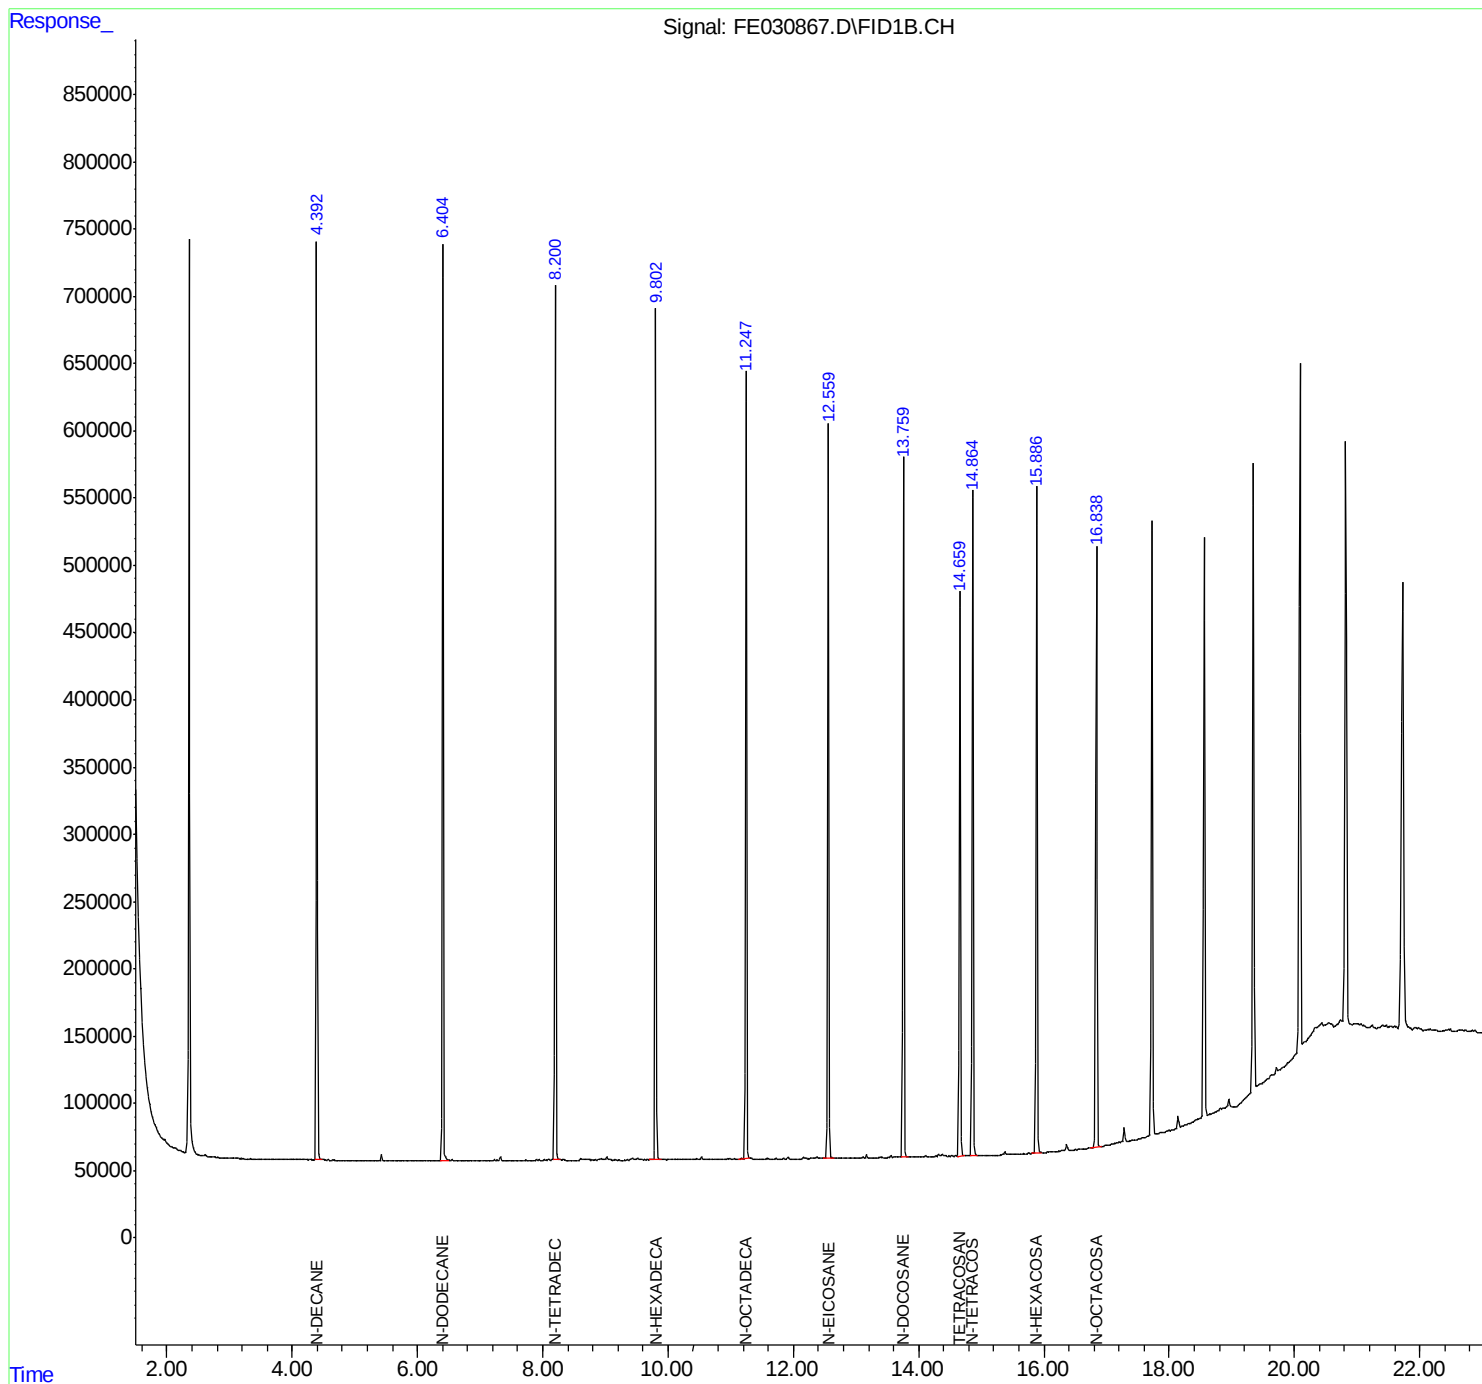


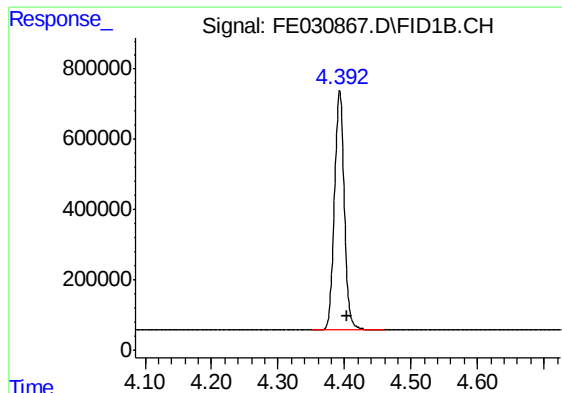

#2 N-DECANE


R.T.: 4.393 min
Delta R.T.: -0.012 min
Response: 6966355
Conc: 18.31 ug/ml

Instrument :
FID_E
ClientSampleId :
PB124840BS

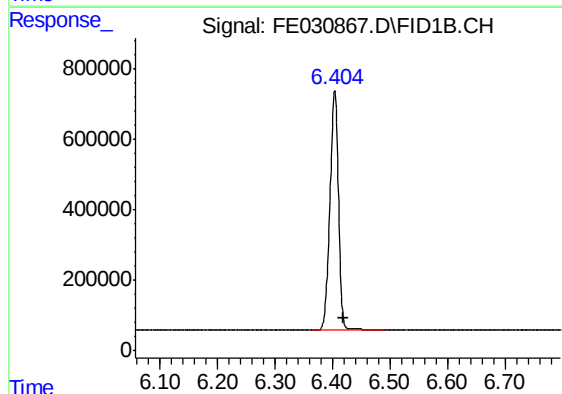


#3 N-DODECANE

R.T.: 6.404 min
Delta R.T.: -0.015 min
Response: 7004752
Conc: 18.41 ug/ml

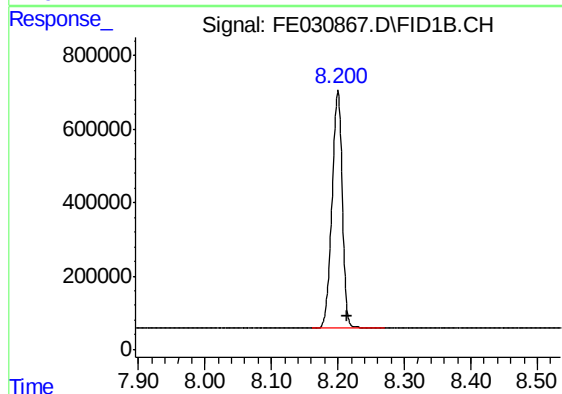


#4 N-TETRADECANE

R.T.: 8.200 min
Delta R.T.: -0.015 min
Response: 6912733
Conc: 18.46 ug/ml

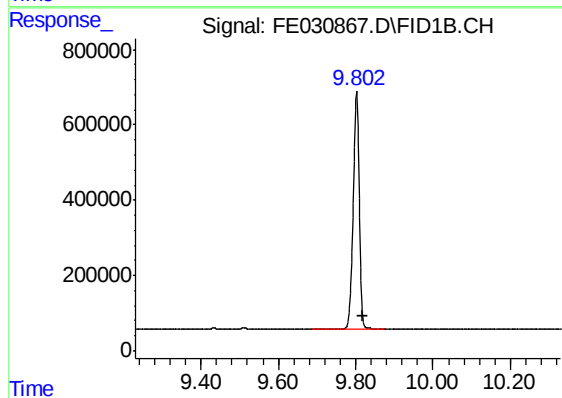

#5 N-HEXADECANE


R.T.: 9.803 min
Delta R.T.: -0.014 min
Response: 6893041
Conc: 18.48 ug/ml

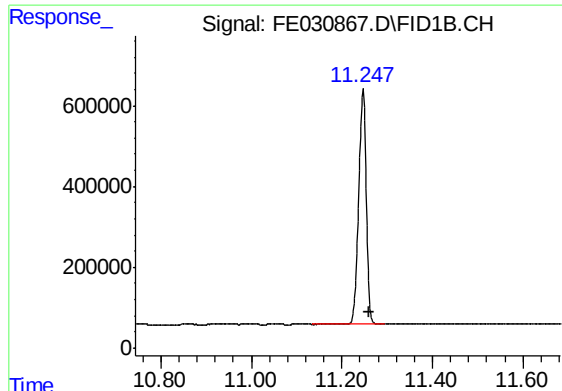

#6 N-OCTADECANE


R.T.: 11.247 min
Delta R.T.: -0.013 min
Response: 6789523
Conc: 18.57 ug/ml

Instrument :
FID_E
ClientSampleId :
PB124840BS

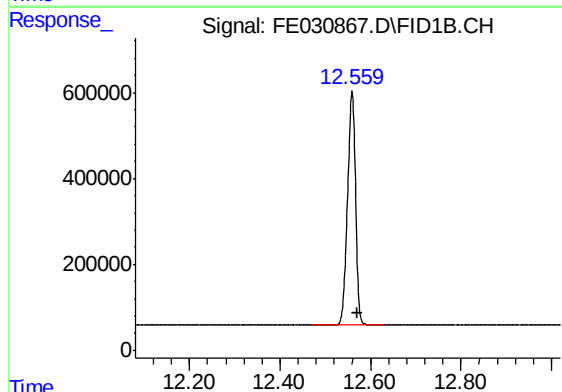


#7 N-EICOSANE

R.T.: 12.559 min
Delta R.T.: -0.011 min
Response: 6697998
Conc: 18.33 ug/ml

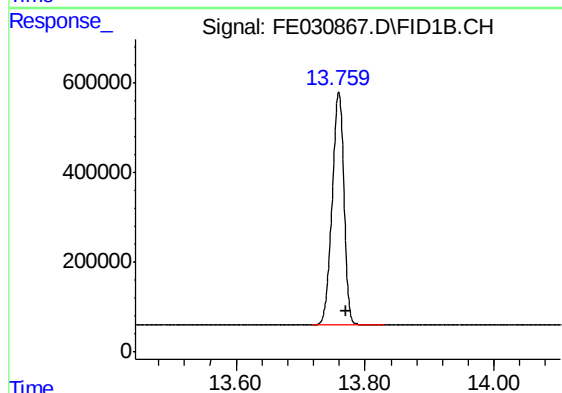


#8 N-DOCOSANE

R.T.: 13.759 min
Delta R.T.: -0.010 min
Response: 6581279
Conc: 18.31 ug/ml

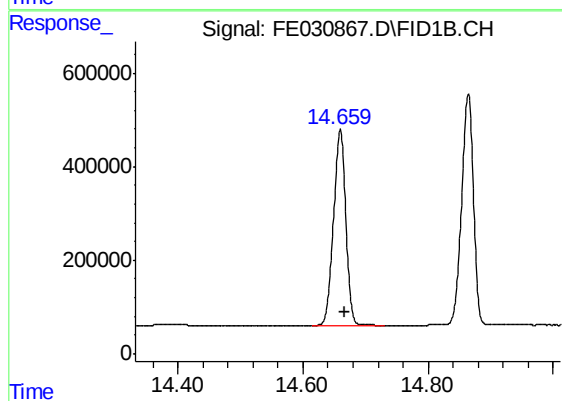

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.660 min
Delta R.T.: -0.008 min
Response: 5672596
Conc: 18.25 ug/ml

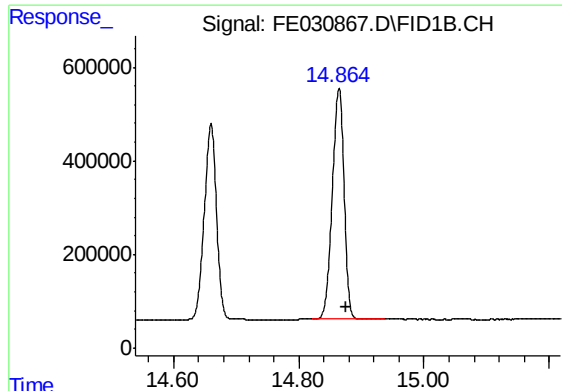

#10 N-TETRACOSANE


R.T.: 14.864 min
Delta R.T.: -0.011 min
Response: 6478022
Conc: 18.21 ug/ml

Instrument :
FID_E
ClientSampleId :
PB124840BS

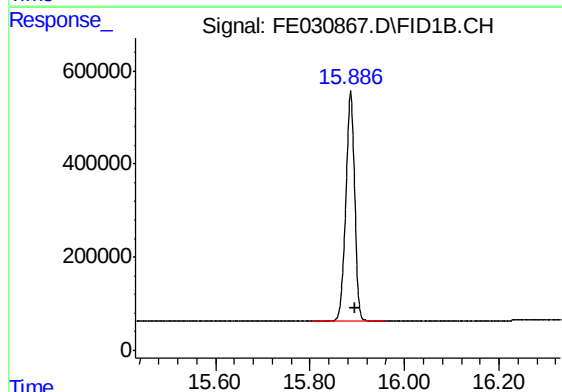

#11 N-HEXACOSANE

R.T.: 15.886 min
Delta R.T.: -0.008 min
Response: 6365345
Conc: 18.25 ug/ml

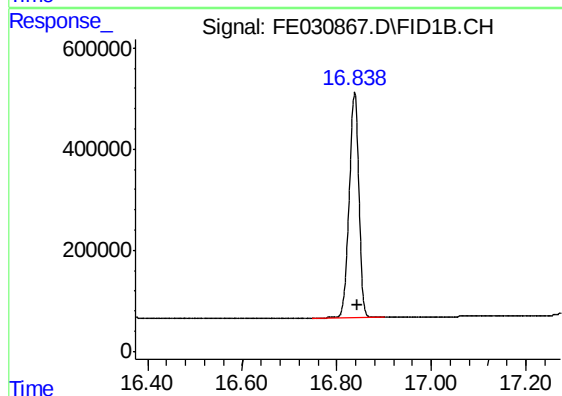

#12 N-OCTACOSANE

R.T.: 16.838 min
Delta R.T.: -0.006 min
Response: 6319569
Conc: 18.54 ug/ml