

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111522AL\
 Data File : FE038770.D
 Signal(s) : FID1B.ch
 Acq On : 15 Nov 2022 08:07
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 16 04:00:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 102522.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 26 04:49:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.491f	134879	0.985 ug/ml
Spiked Amount 50.000		Recovery =	1.97%
Target Compounds			
10) T n-Eicosane (C20)	12.938	171396	1.064 ug/ml
11) T n-Heneicosane (C21)	13.551	448284	2.775 ug/ml
13) T n-Docosane (C22)	14.143	452684	2.804 ug/ml
14) T n-Tetracosane (C24)	15.248	427854	2.667 ug/ml
15) T n-Hexacosane (C26)	16.273	278389	1.753 ug/ml
16) T n-Octacosane (C28)	17.222	211079	1.345 ug/ml
17) T n-Tricontane (C30)	18.109	122859	0.770 ug/ml
18) T n-Dotriacontane (C32)	18.942	189013	1.199 ug/ml
20) T n-Hexatriacontane (C36)	20.465	95092	0.666 ug/ml
22) T n-Tetracontane (C40)	22.123	158019	1.252 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111522AL\
Data File : FE038770.D
Signal(s) : FID1B.ch
Acq On : 15 Nov 2022 08:07
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 16 04:00:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 102522.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 04:49:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

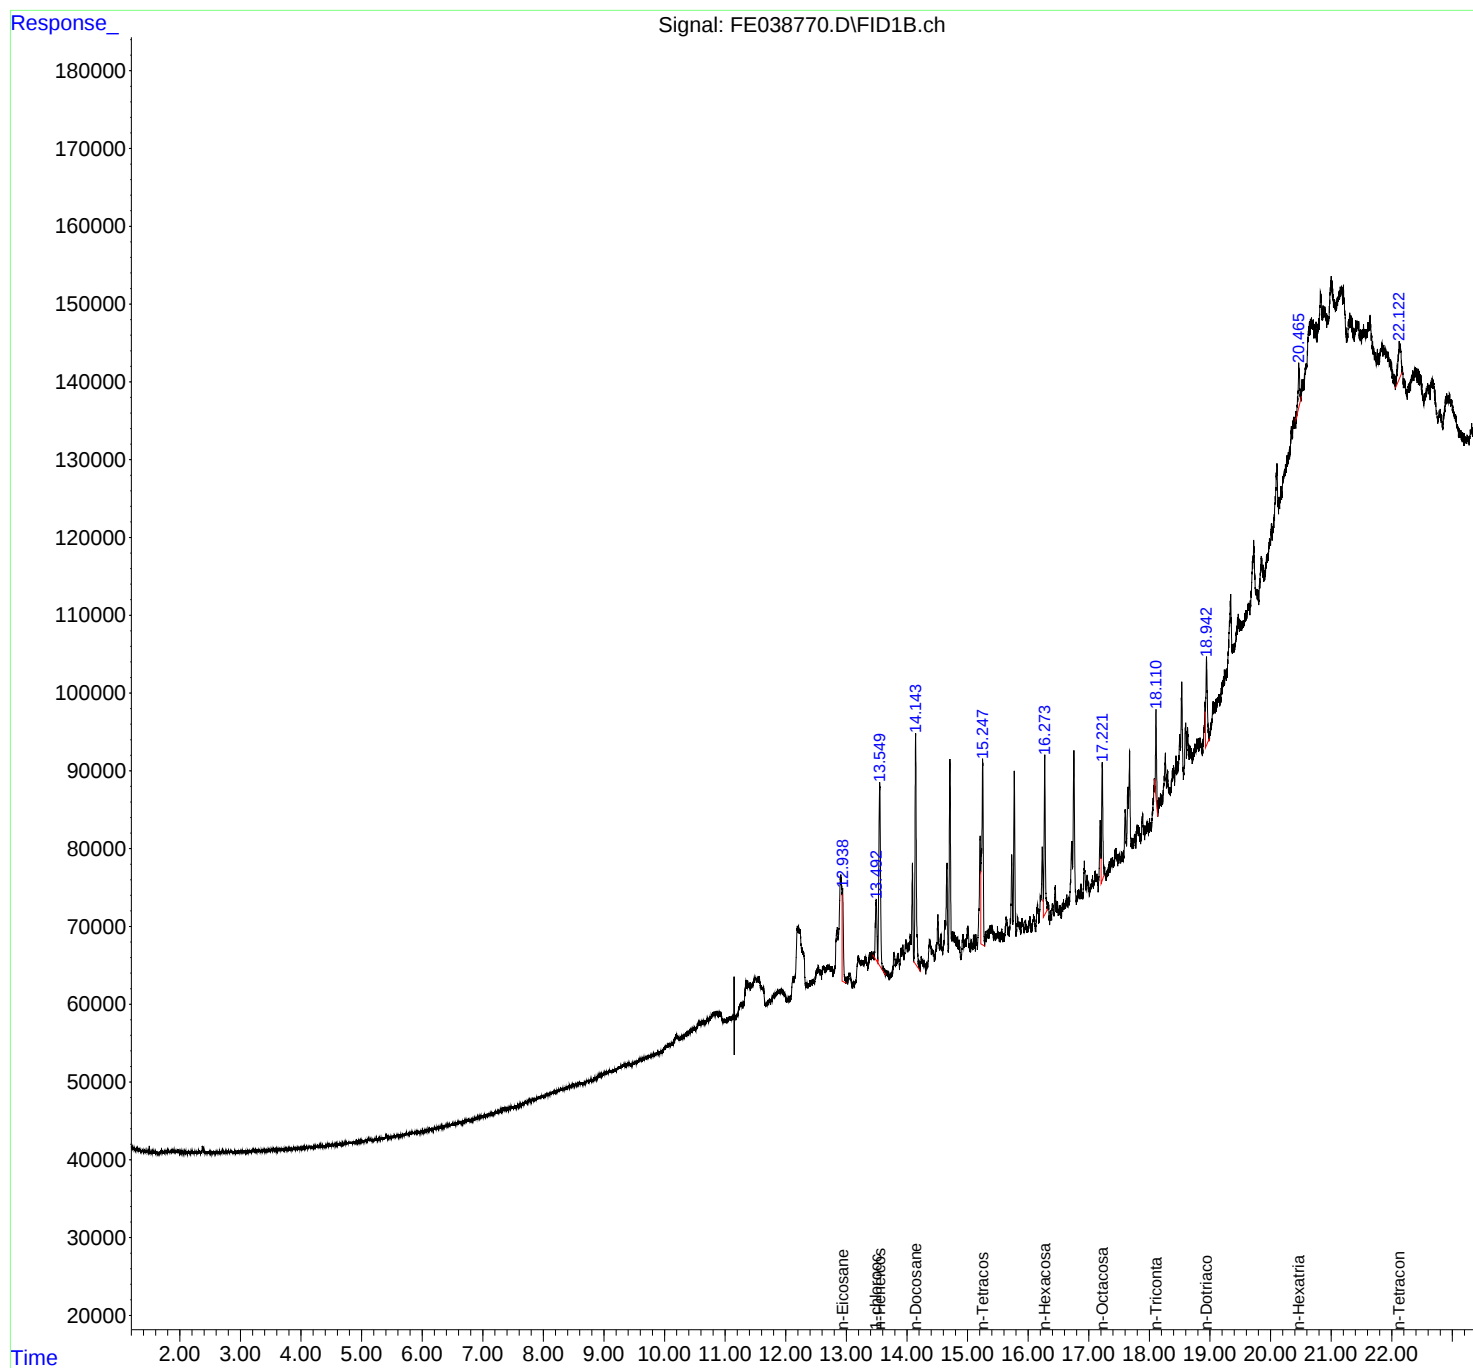


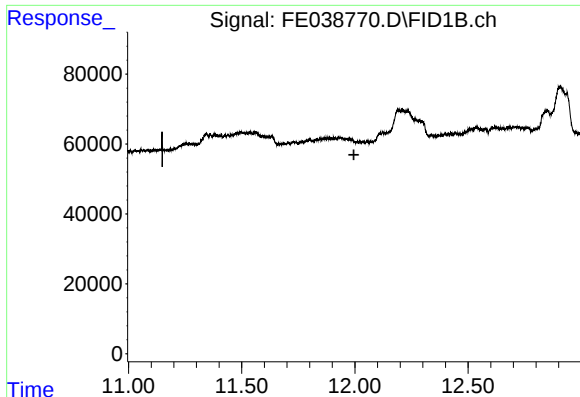

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.996 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

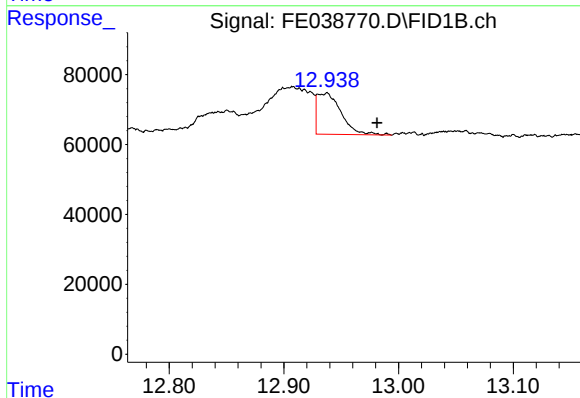


#10 n-Eicosane (C20)

R.T.: 12.938 min
Delta R.T.: -0.043 min
Response: 171396
Conc: 1.06 ug/ml

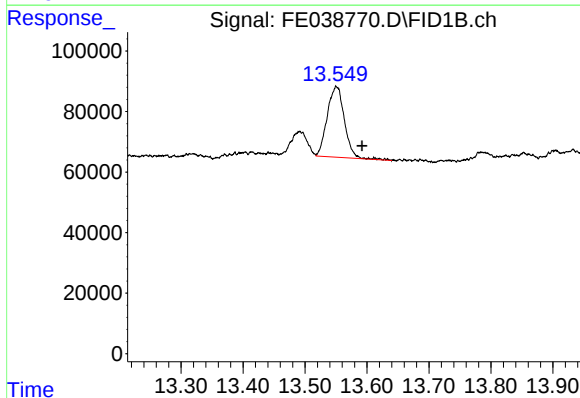


#11 n-Heneicosane (C21)

R.T.: 13.551 min
Delta R.T.: -0.041 min
Response: 448284
Conc: 2.78 ug/ml

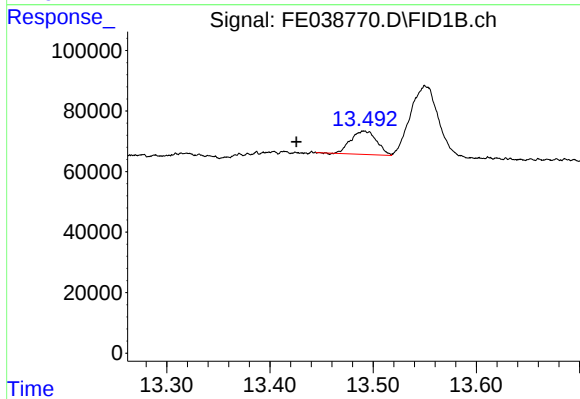

#12 1-chlorooctadecane (SURR)


R.T.: 13.491 min
Delta R.T.: 0.065 min
Response: 134879
Conc: 0.99 ug/ml

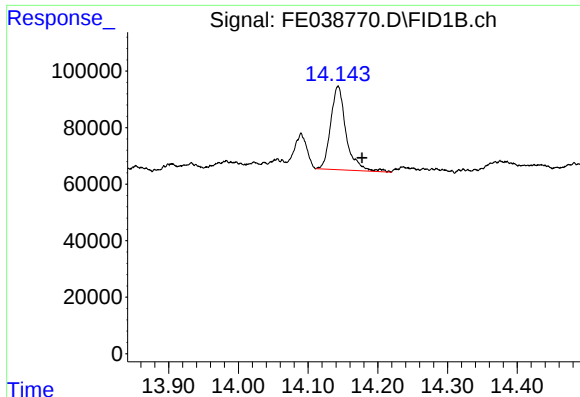

#13 n-Docosane (C22)


R.T.: 14.143 min
Delta R.T.: -0.034 min
Response: 452684
Conc: 2.80 ug/ml

Instrument :
FID_E
ClientSampleId :

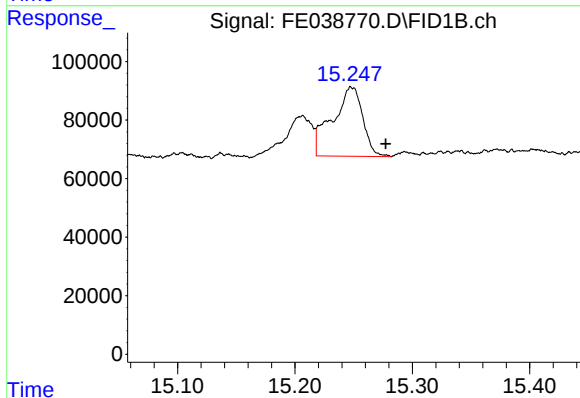


#14 n-Tetracosane (C24)

R.T.: 15.248 min
Delta R.T.: -0.029 min
Response: 427854
Conc: 2.67 ug/ml

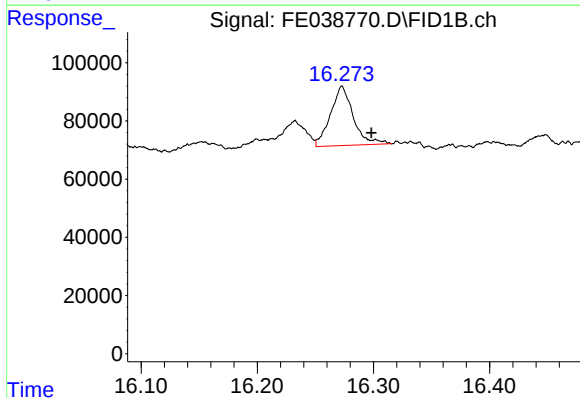


#15 n-Hexacosane (C26)

R.T.: 16.273 min
Delta R.T.: -0.025 min
Response: 278389
Conc: 1.75 ug/ml

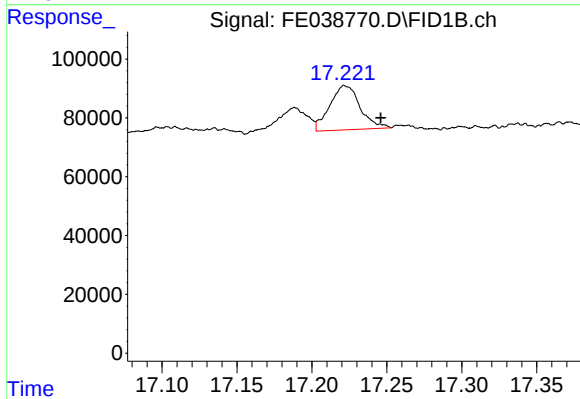

#16 n-Octacosane (C28)


R.T.: 17.222 min
Delta R.T.: -0.024 min
Response: 211079
Conc: 1.35 ug/ml

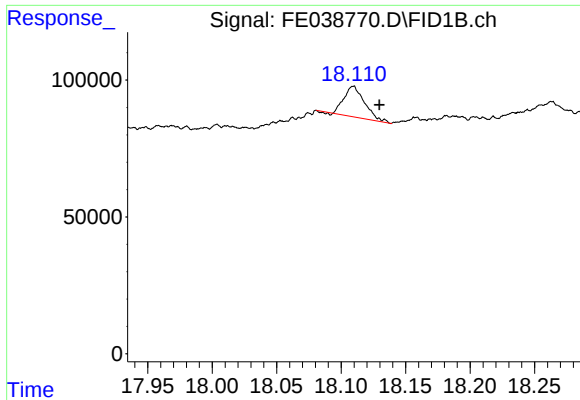

#17 n-Tricontane (C30)


R.T.: 18.109 min
Delta R.T.: -0.020 min
Response: 122859
Conc: 0.77 ug/ml

Instrument :
FID_E
ClientSampleId :

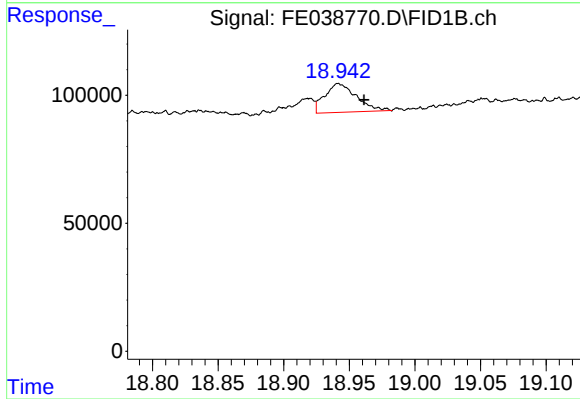


#18 n-Dotriacontane (C32)

R.T.: 18.942 min
Delta R.T.: -0.019 min
Response: 189013
Conc: 1.20 ug/ml

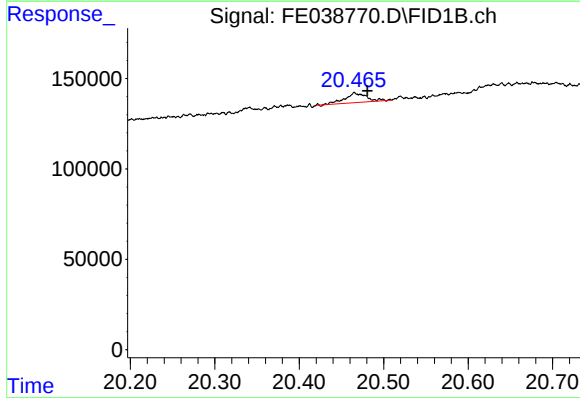

#20 n-Hexatriacontane (C36)

R.T.: 20.465 min
Delta R.T.: -0.015 min
Response: 95092
Conc: 0.67 ug/ml

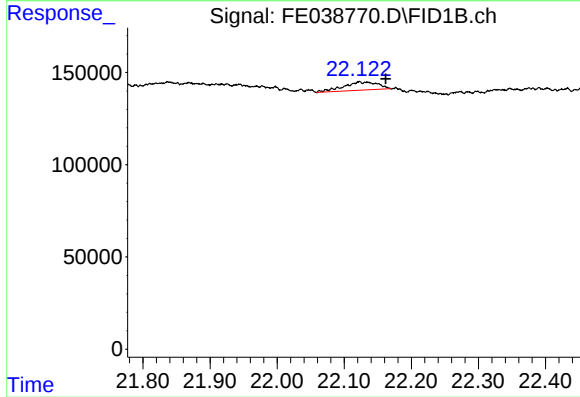

#22 n-Tetracontane (C40)

R.T.: 22.123 min
Delta R.T.: -0.040 min
Response: 158019
Conc: 1.25 ug/ml