

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111523AL\
Data File : FE045364.D
Signal(s) : FID1B.ch
Acq On : 15 Nov 2023 14:23
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 15 15:53:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 110423.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 05:16:05 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
20) T	n-Hexatriacontane (C36)	20.463	74250	0.457 ug/ml
21) T	n-Octatriacontane (C38)	21.163	236739	1.425 ug/ml
22) T	n-Tetracontane (C40)	22.135f	733334	4.293 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111523AL\
Data File : FE045364.D
Signal(s) : FID1B.ch
Acq On : 15 Nov 2023 14:23
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 15 15:53:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 110423.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 05:16:05 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

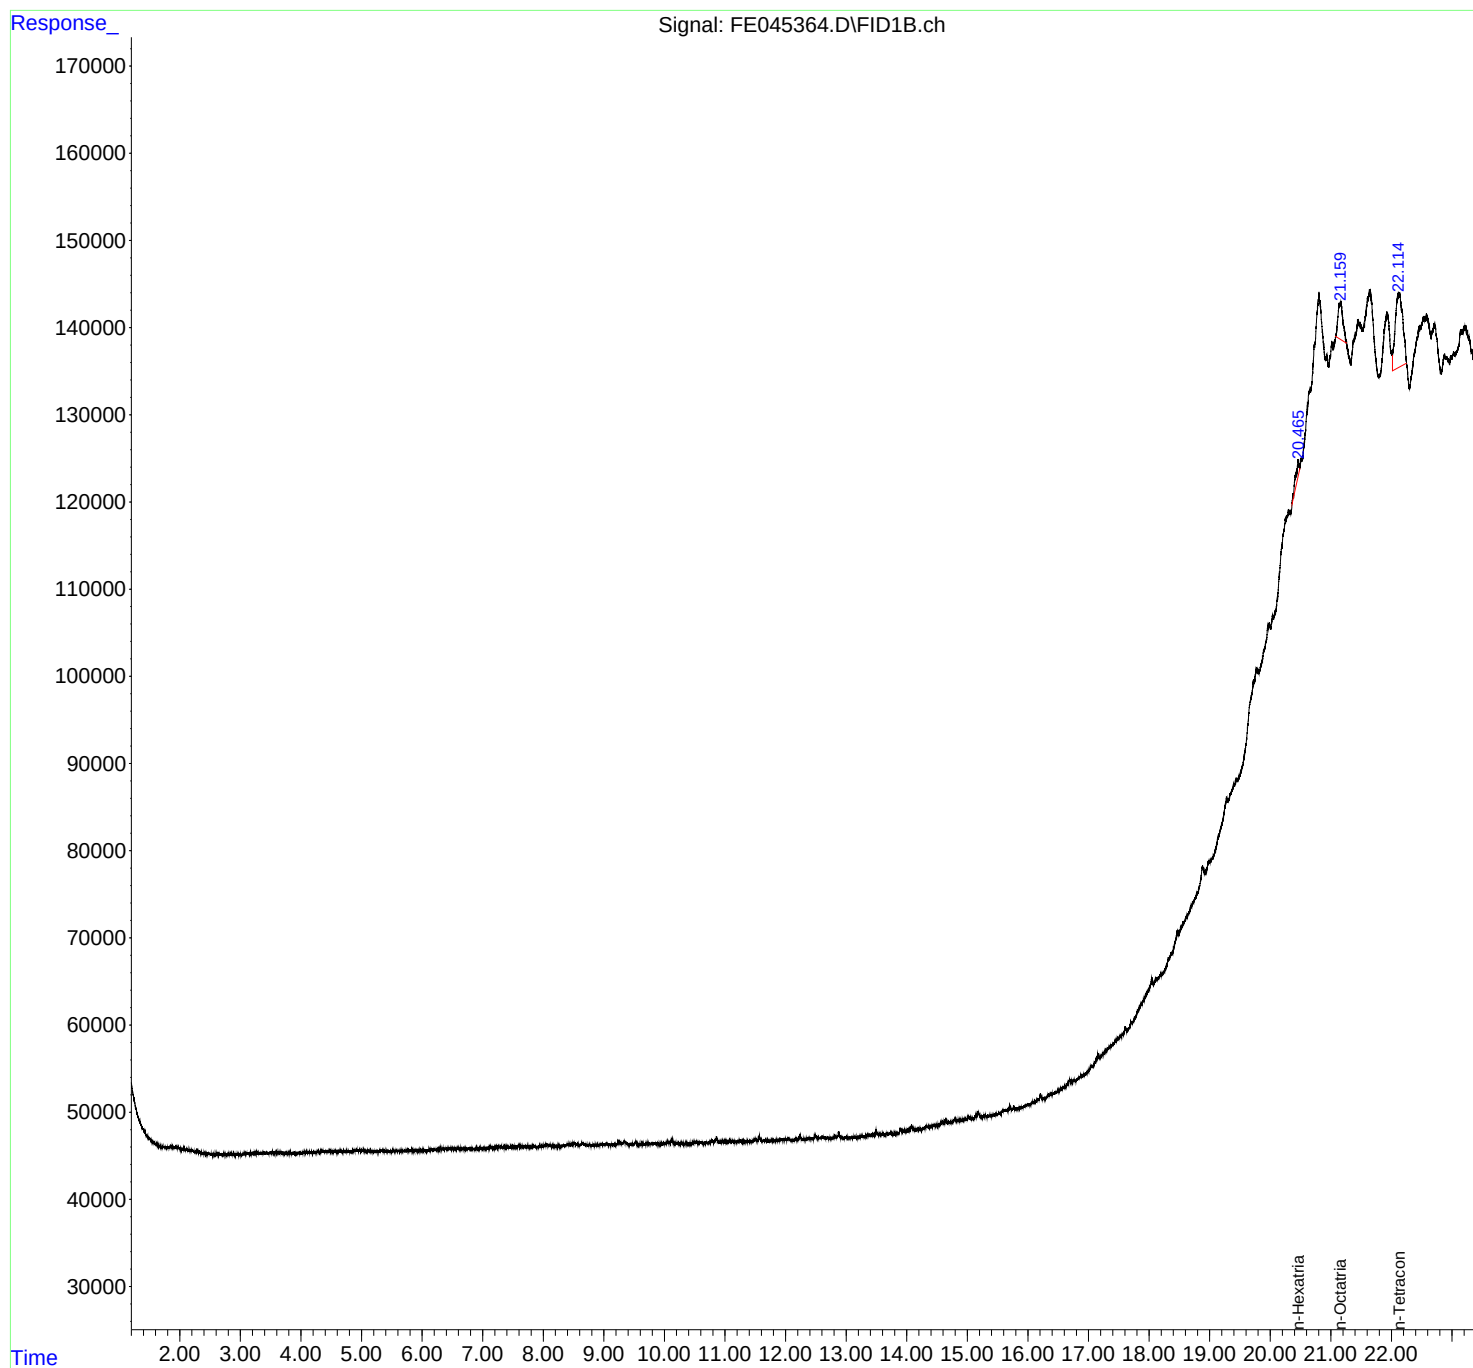


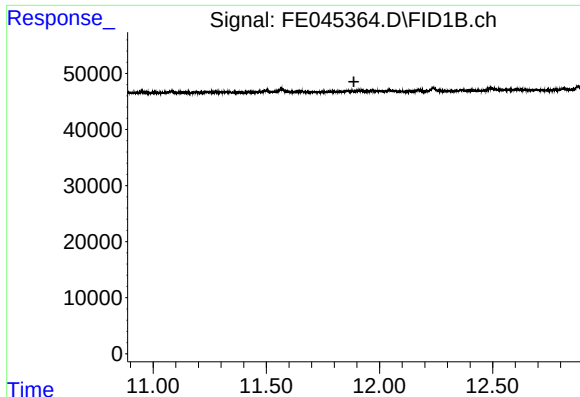

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.887 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

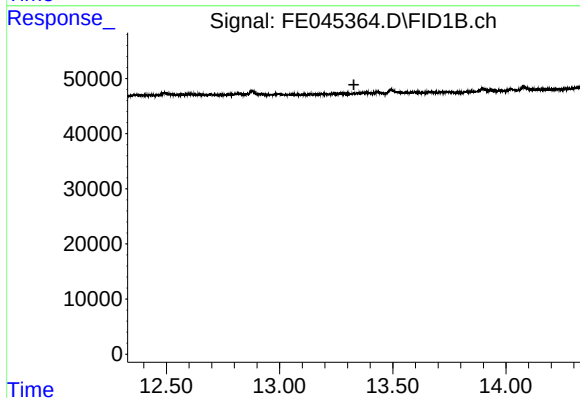


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.328 min
Response: 0
Conc: N.D.

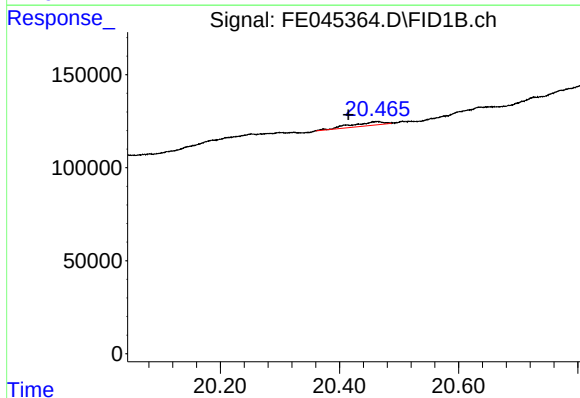


#20 n-Hexatriacontane (C36)

R.T.: 20.463 min
Delta R.T.: 0.048 min
Response: 74250
Conc: 0.46 ug/ml

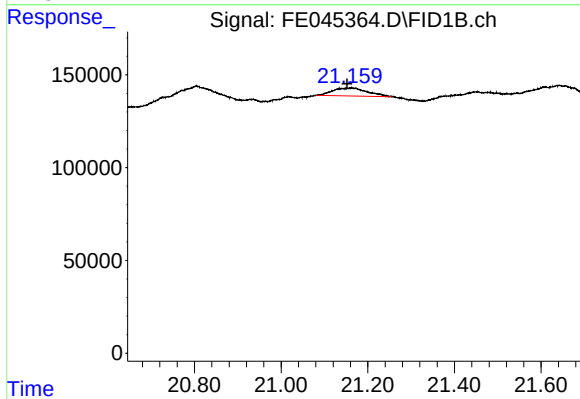

#21 n-Octatriacontane (C38)

R.T.: 21.163 min
Delta R.T.: 0.011 min
Response: 236739
Conc: 1.42 ug/ml

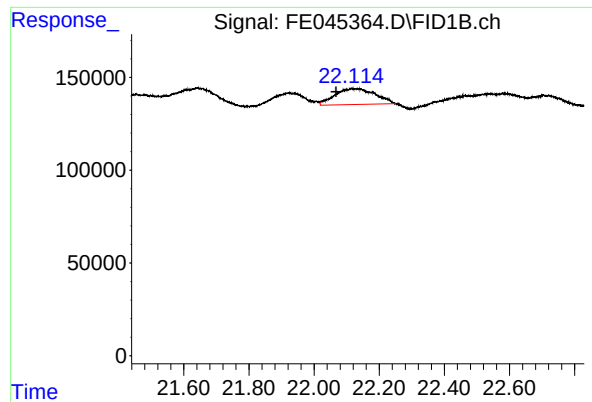

#22 n-Tetracontane (C40)

R.T.: 22.135 min
Delta R.T.: 0.067 min
Response: 733334
Conc: 4.29 ug/ml

Instrument :

FID_E

ClientSampleId :