

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111618\
 Data File : FE029253.D
 Signal(s) : FID1B.CH
 Acq On : 16 Nov 2018 11:30
 Operator : AJ\SJ
 Sample : 4400 TRPH STD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 16 14:42:21 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE111618.M
 Quant Title :
 QLast Update : Fri Nov 16 14:42:03 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.863	8947843	50.000 ug/ml
Target Compounds			
1) N-OCTANE	2.504	52790788	400.000 ug/ml
2) N-NONANE	3.522	55241601	400.000 ug/ml
3) N-DECANE	4.602	85742333	400.000 ug/ml
4) N-UNDECANE	5.643	92481395	600.000 ug/ml
5) N-DODECANE	6.628	93878232	600.000 ug/ml
6) N-TETRADECANE	8.435	97568548	600.000 ug/ml
7) N-HEXADECANE	10.042	86579314	500.000 ug/ml
8) N-OCTADECANE	11.472	44659330	250.000 ug/ml
9) N-EICOSANE	12.769	18023351	100.000 ug/ml
10) N-TETRACOSANE	15.079	17427830	100.000 ug/ml
11) N-OCTACOSANE	17.044	7897386	50.000 ug/ml
12) N-DOTRIACONTANE	18.768	7192303	50.000 ug/ml
14) N-HEXATRIACONTANE	20.297	7277260	50.000 ug/ml
15) N-TETRACONTANE	22.047	7072466	50.000 ug/ml
16) N-TETRTETRACOOCTANE	25.014	6061208	50.000 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111618\
Data File : FE029253.D
Signal(s) : FID1B.CH
Acq On : 16 Nov 2018 11:30
Operator : AJ\SJ
Sample : 4400 TRPH STD
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 16 14:42:21 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE111618.M
Quant Title :
QLast Update : Fri Nov 16 14:42:03 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

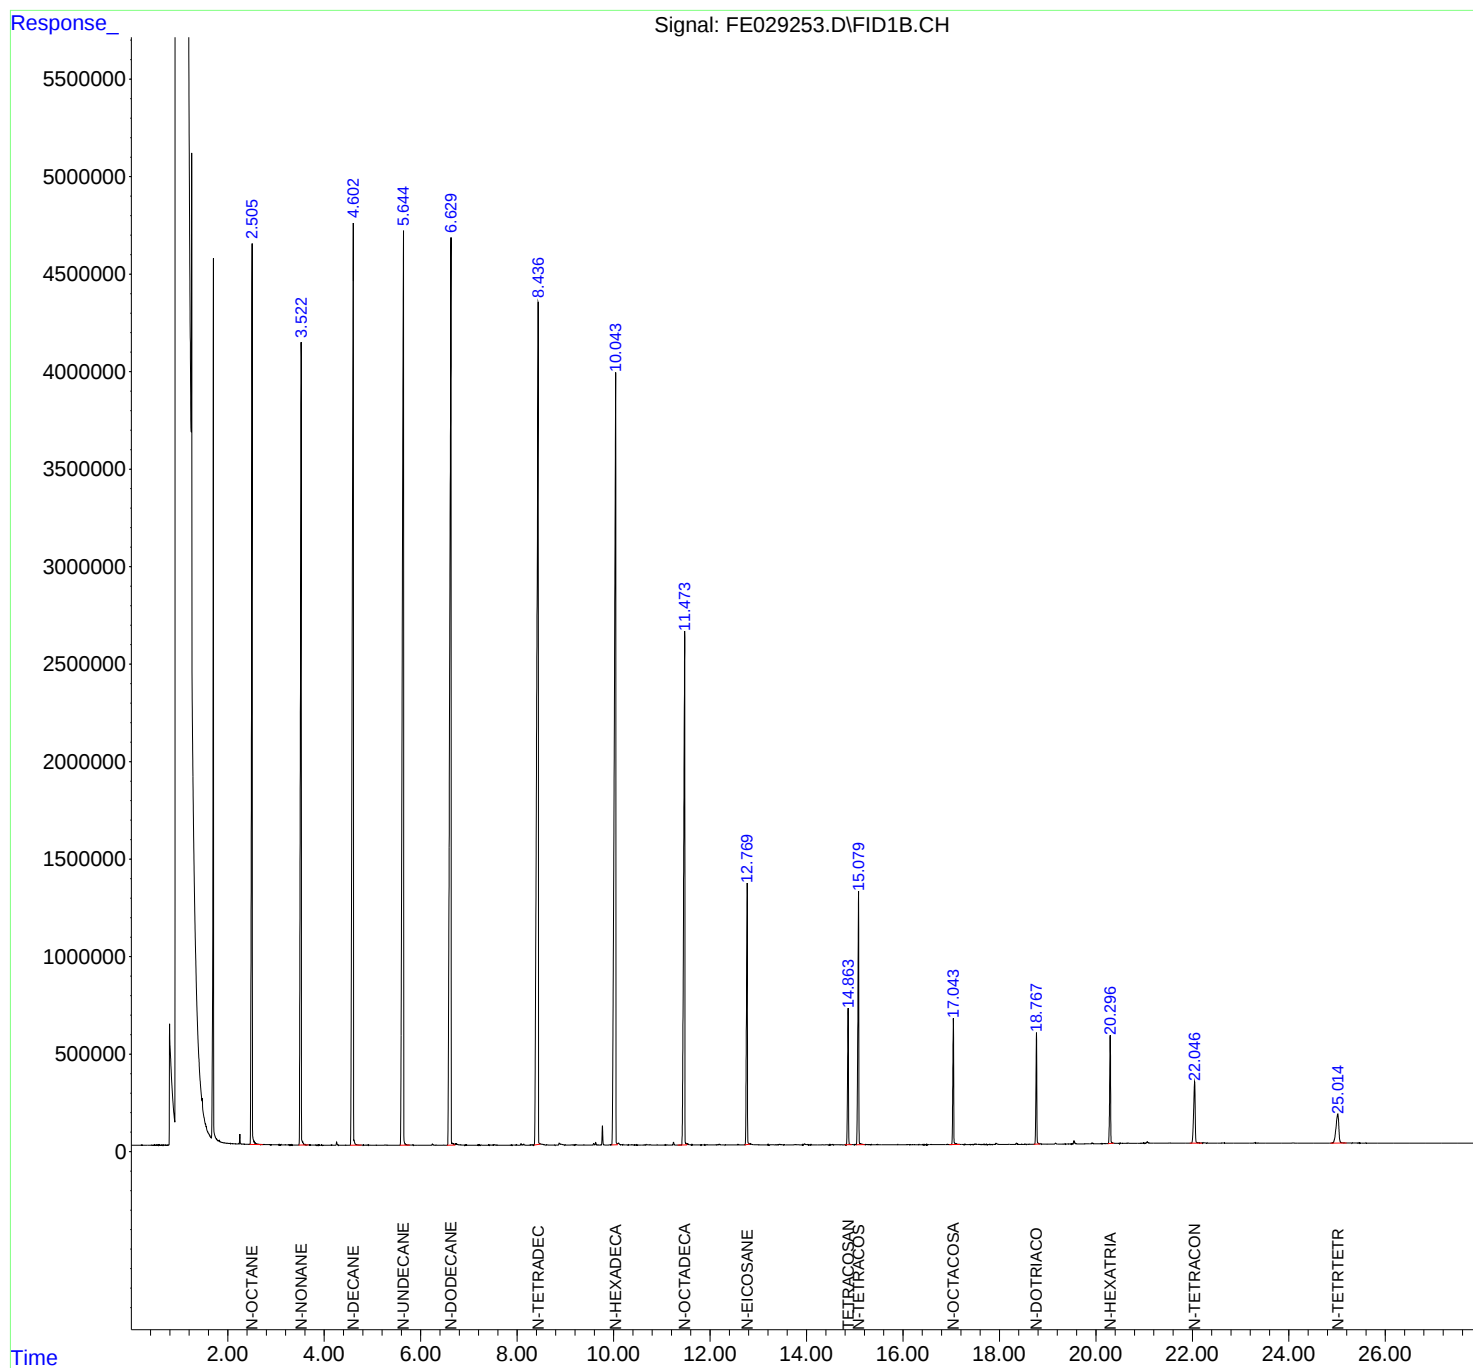

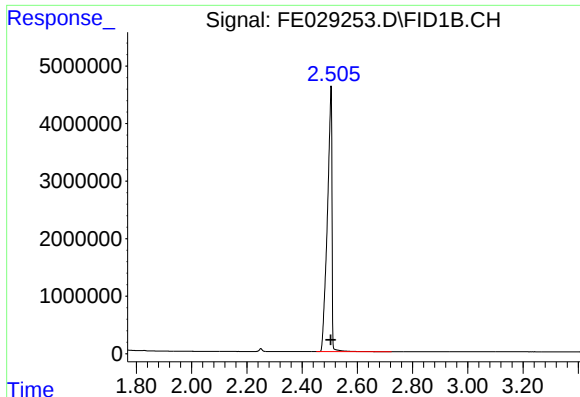


#1 N-OCTANE

R.T.: 2.504 min
Delta R.T.: 0.000 min
Response: 52790788
Conc: 400.00 ug/ml

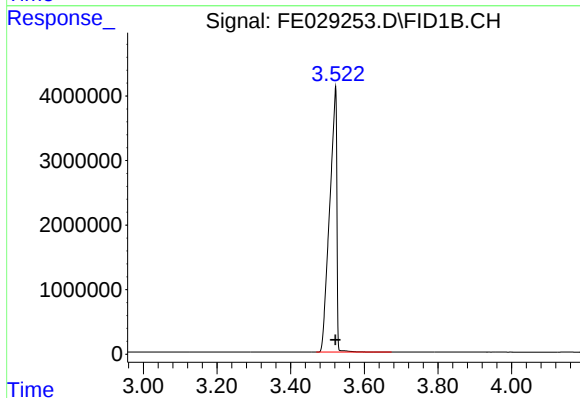


#2 N-NONANE

R.T.: 3.522 min
Delta R.T.: 0.000 min
Response: 55241601
Conc: 400.00 ug/ml

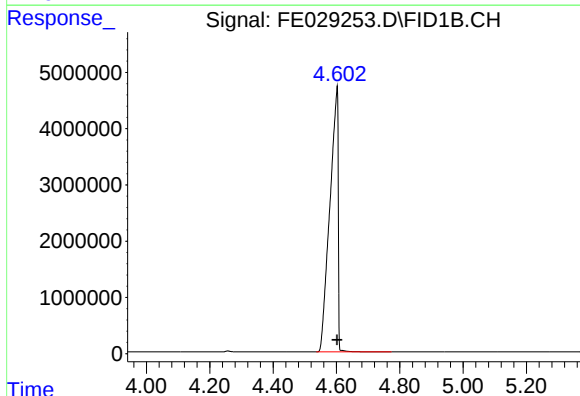


#3 N-DECANE

R.T.: 4.602 min
Delta R.T.: 0.000 min
Response: 85742333
Conc: 400.00 ug/ml

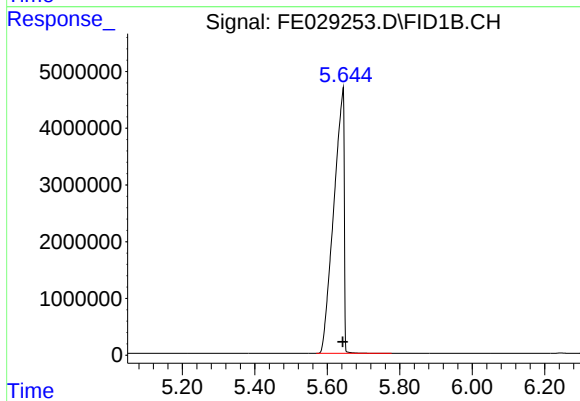


#4 N-UNDECANE

R.T.: 5.643 min
Delta R.T.: 0.000 min
Response: 92481395
Conc: 600.00 ug/ml

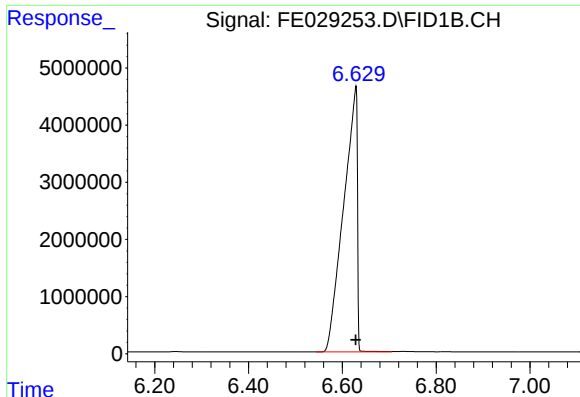


#5 N-DODECANE

R.T.: 6.628 min
Delta R.T.: 0.000 min
Response: 93878232
Conc: 600.00 ug/ml

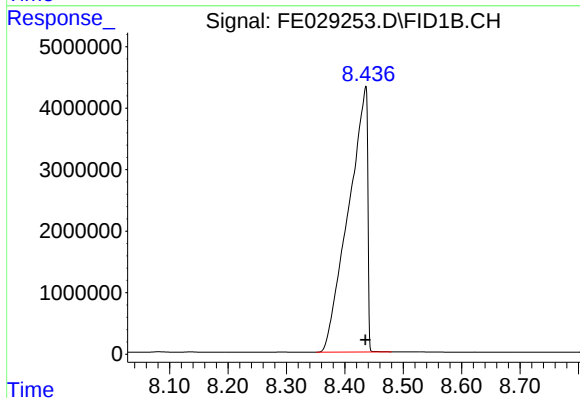


#6 N-TETRADECANE

R.T.: 8.435 min
Delta R.T.: 0.000 min
Response: 97568548
Conc: 600.00 ug/ml

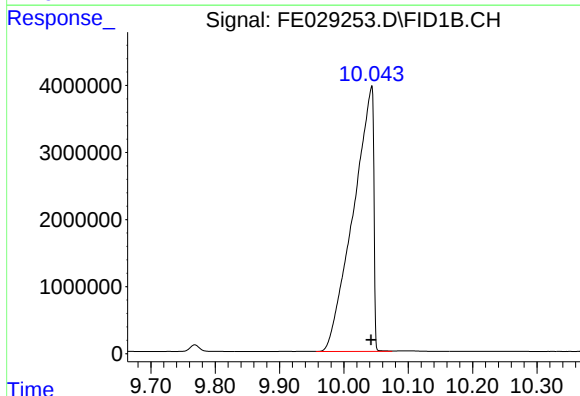


#7 N-HEXADECANE

R.T.: 10.042 min
Delta R.T.: 0.000 min
Response: 86579314
Conc: 500.00 ug/ml

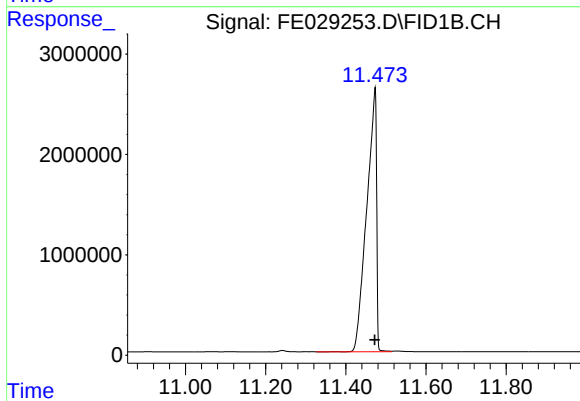


#8 N-OCTADECANE

R.T.: 11.472 min
Delta R.T.: 0.000 min
Response: 44659330
Conc: 250.00 ug/ml

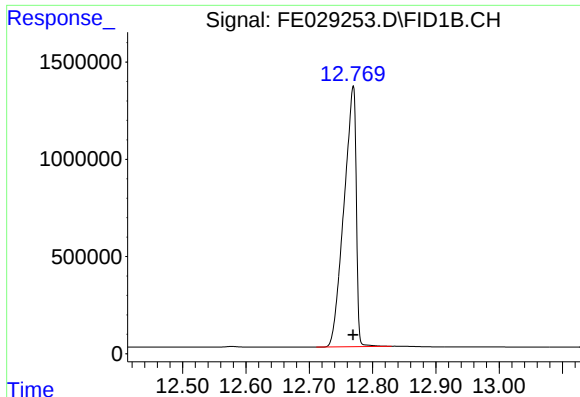


#9 N-EICOSANE

R.T.: 12.769 min
Delta R.T.: 0.000 min
Response: 18023351
Conc: 100.00 ug/ml

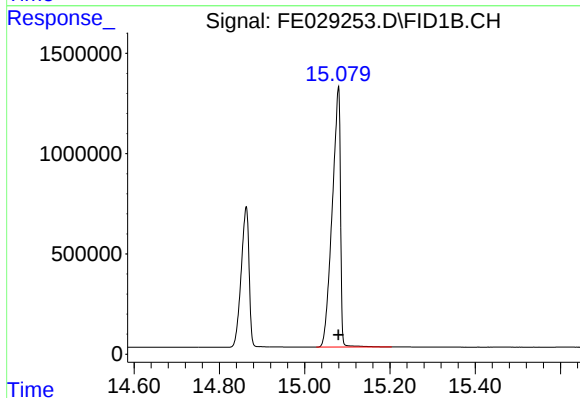


#10 N-TETRACOSANE

R.T.: 15.079 min
Delta R.T.: 0.000 min
Response: 17427830
Conc: 100.00 ug/ml

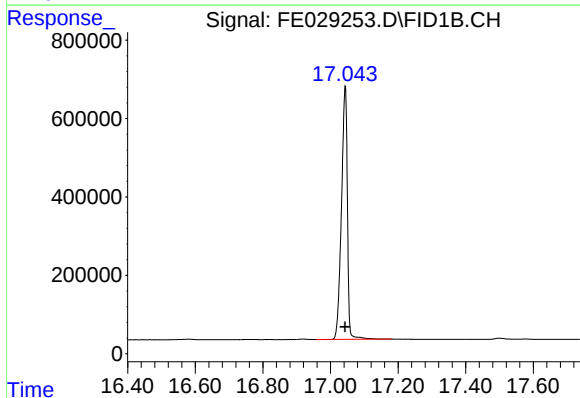


#11 N-OCTACOSANE

R.T.: 17.044 min
Delta R.T.: 0.000 min
Response: 7897386
Conc: 50.00 ug/ml

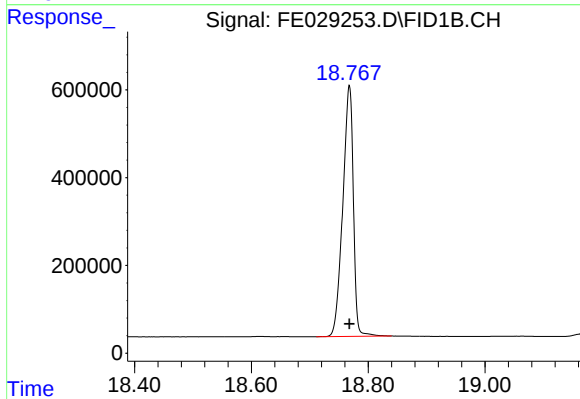


#12 N-DOTRIACONTANE

R.T.: 18.768 min
Delta R.T.: 0.000 min
Response: 7192303
Conc: 50.00 ug/ml

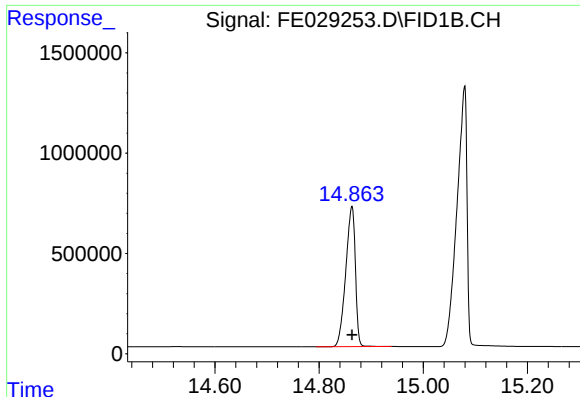


#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.863 min
Delta R.T.: 0.000 min
Response: 8947843
Conc: 50.00 ug/ml

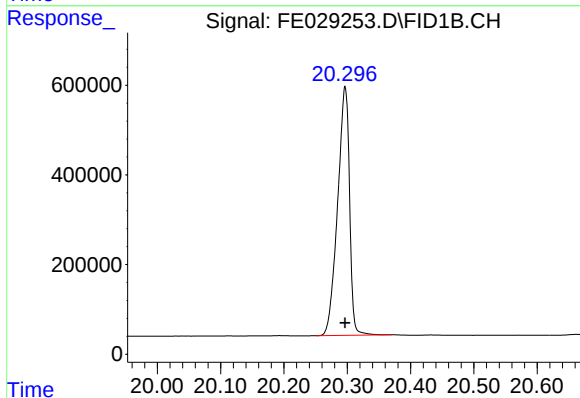


#14 N-HEXATRIACONTANE

R.T.: 20.297 min
Delta R.T.: 0.000 min
Response: 7277260
Conc: 50.00 ug/ml

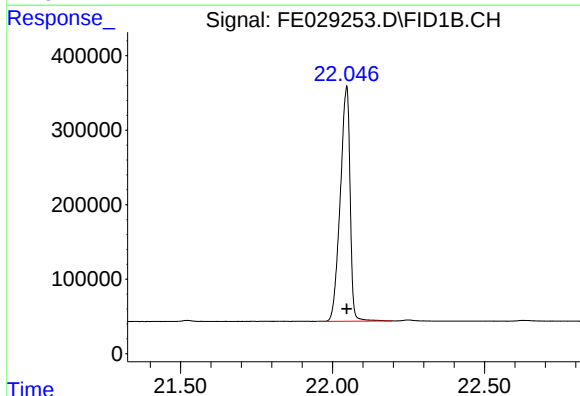

#15 N-TETRACONTANE

R.T.: 22.047 min
Delta R.T.: 0.000 min
Response: 7072466
Conc: 50.00 ug/ml

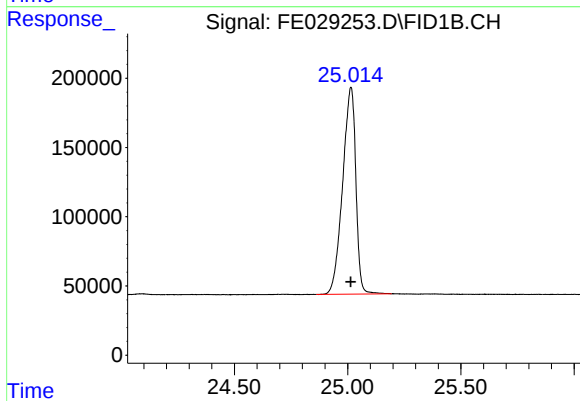

#16 N-TETRTETRACOOCTANE

R.T.: 25.014 min
Delta R.T.: 0.000 min
Response: 6061208
Conc: 50.00 ug/ml