

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111622AL\
 Data File : FE038788.D
 Signal(s) : FID1B.ch
 Acq On : 16 Nov 2022 08:17
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 MECL2

Integration File: autoint1.e
 Quant Time: Nov 17 03:31:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 102522.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 26 04:49:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10) T	n-Eicosane (C20)	12.935	263278	1.634 ug/ml
11) T	n-Heneicosane (C21)	13.552	240401	1.488 ug/ml
13) T	n-Docosane (C22)	14.143	242178	1.500 ug/ml
14) T	n-Tetracosane (C24)	15.247	242239	1.510 ug/ml
15) T	n-Hexacosane (C26)	16.271	142846	0.899 ug/ml
16) T	n-Octacosane (C28)	17.220	136343	0.869 ug/ml
17) T	n-Tricontane (C30)	18.107	68817	0.431 ug/ml
18) T	n-Dotriacontane (C32)	18.938	166905	1.059 ug/ml
20) T	n-Hexatriacontane (C36)	20.463	5743	0.040 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111622AL\
Data File : FE038788.D
Signal(s) : FID1B.ch
Acq On : 16 Nov 2022 08:17
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Nov 17 03:31:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_D\methods\Aliphatic EPH 102522.M
Quant Title : GC Extractables
QLast Update : Wed Oct 26 04:49:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

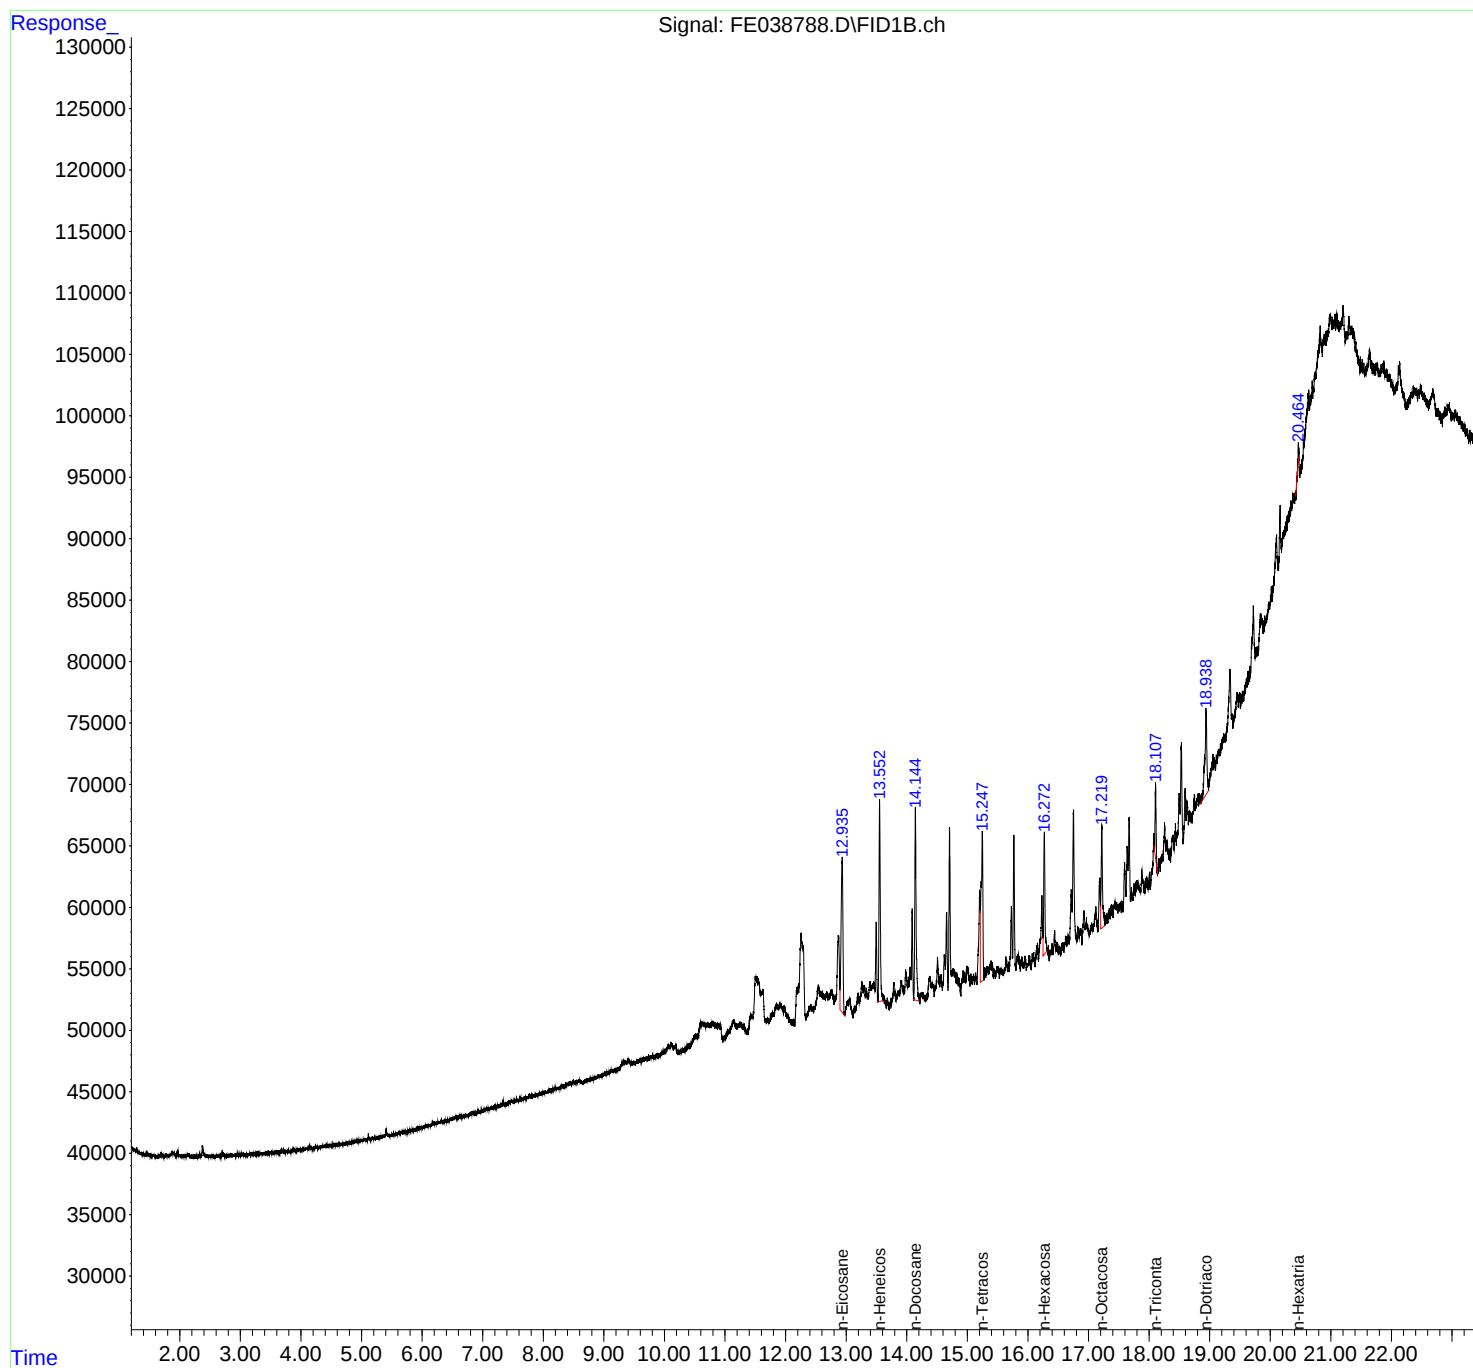


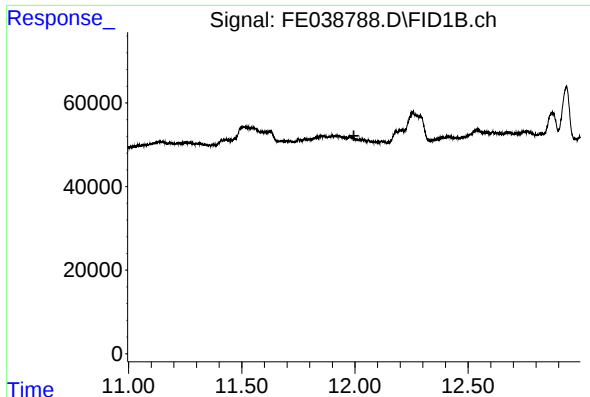

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.996 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
MECL2

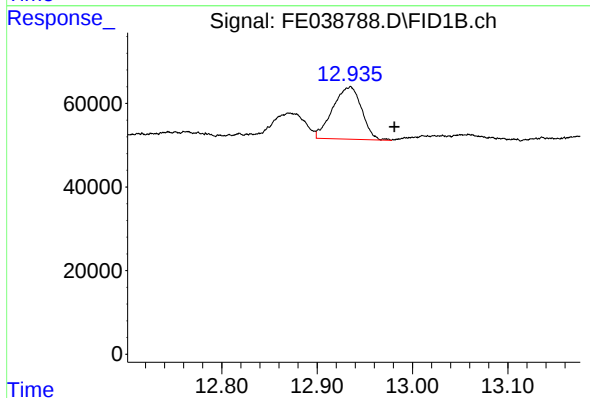


#10 n-Eicosane (C20)

R.T.: 12.935 min
Delta R.T.: -0.046 min
Response: 263278
Conc: 1.63 ug/ml

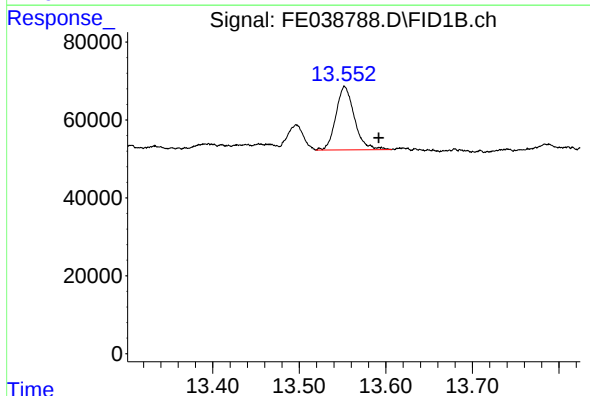


#11 n-Heneicosane (C21)

R.T.: 13.552 min
Delta R.T.: -0.040 min
Response: 240401
Conc: 1.49 ug/ml

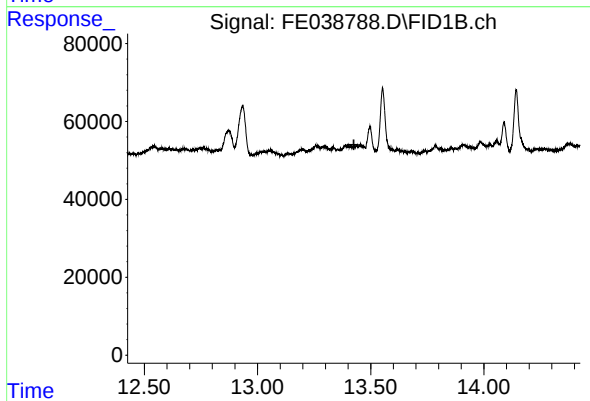

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.426 min
Response: 0
Conc: N.D.

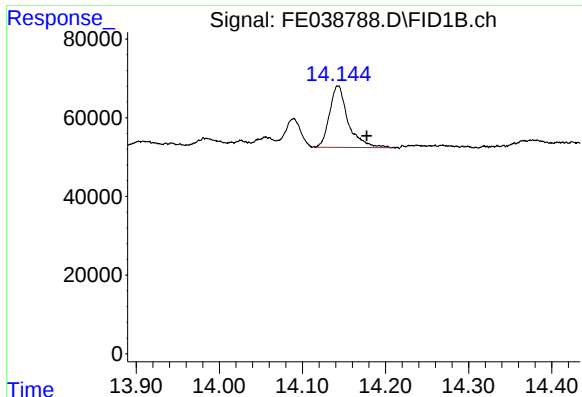

#13 n-Docosane (C22)


R.T.: 14.143 min
Delta R.T.: -0.035 min
Response: 242178
Conc: 1.50 ug/ml

Instrument :
FID_E
ClientSampleId :
MECL2

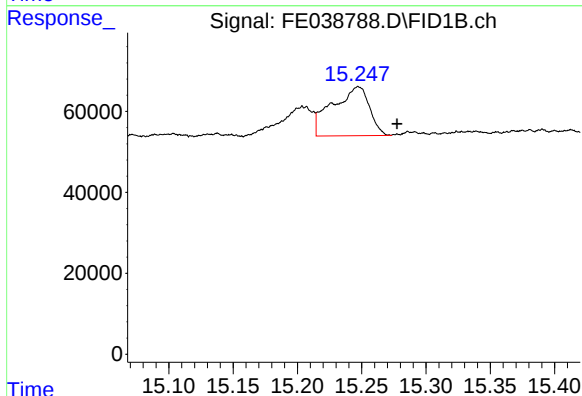


#14 n-Tetracosane (C24)

R.T.: 15.247 min
Delta R.T.: -0.030 min
Response: 242239
Conc: 1.51 ug/ml

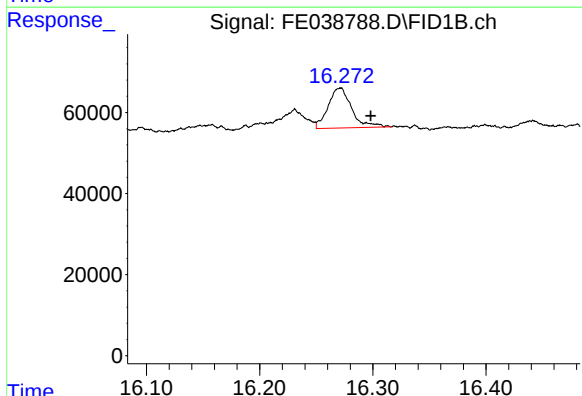


#15 n-Hexacosane (C26)

R.T.: 16.271 min
Delta R.T.: -0.027 min
Response: 142846
Conc: 0.90 ug/ml

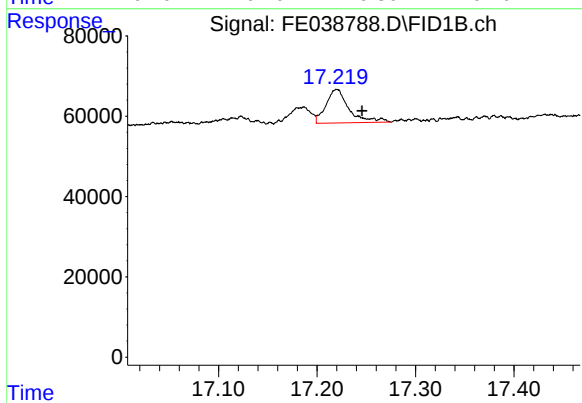

#16 n-Octacosane (C28)


R.T.: 17.220 min
Delta R.T.: -0.026 min
Response: 136343
Conc: 0.87 ug/ml

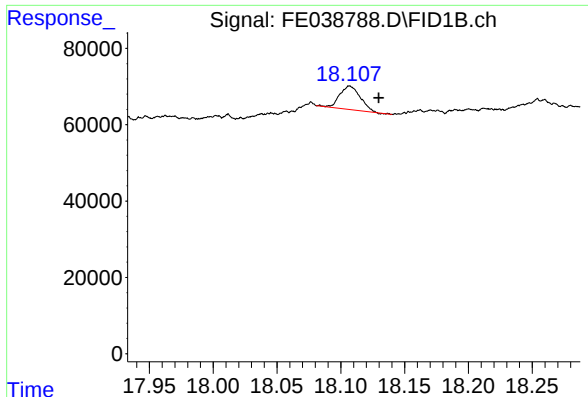

#17 n-Tricontane (C30)


R.T.: 18.107 min
Delta R.T.: -0.023 min
Response: 68817
Conc: 0.43 ug/ml

Instrument :
FID_E
ClientSampleId :
MECL2

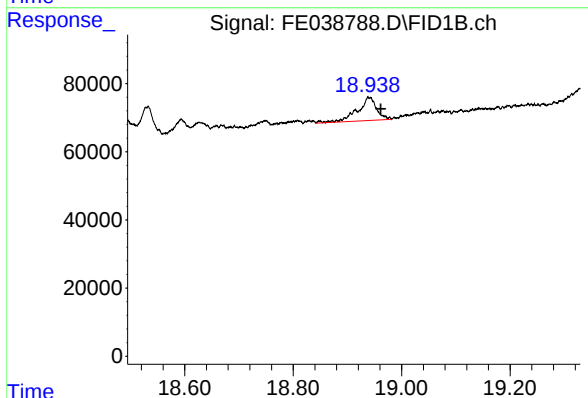

#18 n-Dotriacontane (C32)

R.T.: 18.938 min
Delta R.T.: -0.023 min
Response: 166905
Conc: 1.06 ug/ml

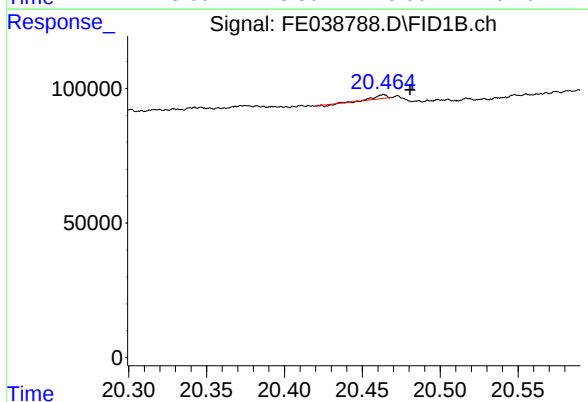

#20 n-Hexatriacontane (C36)

R.T.: 20.463 min
Delta R.T.: -0.017 min
Response: 5743
Conc: 0.04 ug/ml