

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111623AL\
 Data File : FE045385.D
 Signal(s) : FID1B.ch
 Acq On : 16 Nov 2023 06:47
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 16 23:21:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 110423.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 05:16:05 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	12.864	236580	1.493 ug/ml
11) T n-Heneicosane (C21)	13.483	252895	1.645 ug/ml
13) T n-Docosane (C22)	14.074	260259	1.718 ug/ml
14) T n-Tetracosane (C24)	15.181	146587	0.990 ug/ml
15) T n-Hexacosane (C26)	16.205	142486	0.978 ug/ml
16) T n-Octacosane (C28)	17.157	150331	1.029 ug/ml
17) T n-Tricontane (C30)	18.046	114294	0.752 ug/ml
18) T n-Dotriacontane (C32)	18.881	263993	1.690 ug/ml
19) T n-Tetratriacontane (C34)	19.667	82879	0.531 ug/ml
20) T n-Hexatriacontane (C36)	20.407	93294	0.575 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111623AL\
Data File : FE045385.D
Signal(s) : FID1B.ch
Acq On : 16 Nov 2023 06:47
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 16 23:21:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 110423.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 05:16:05 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

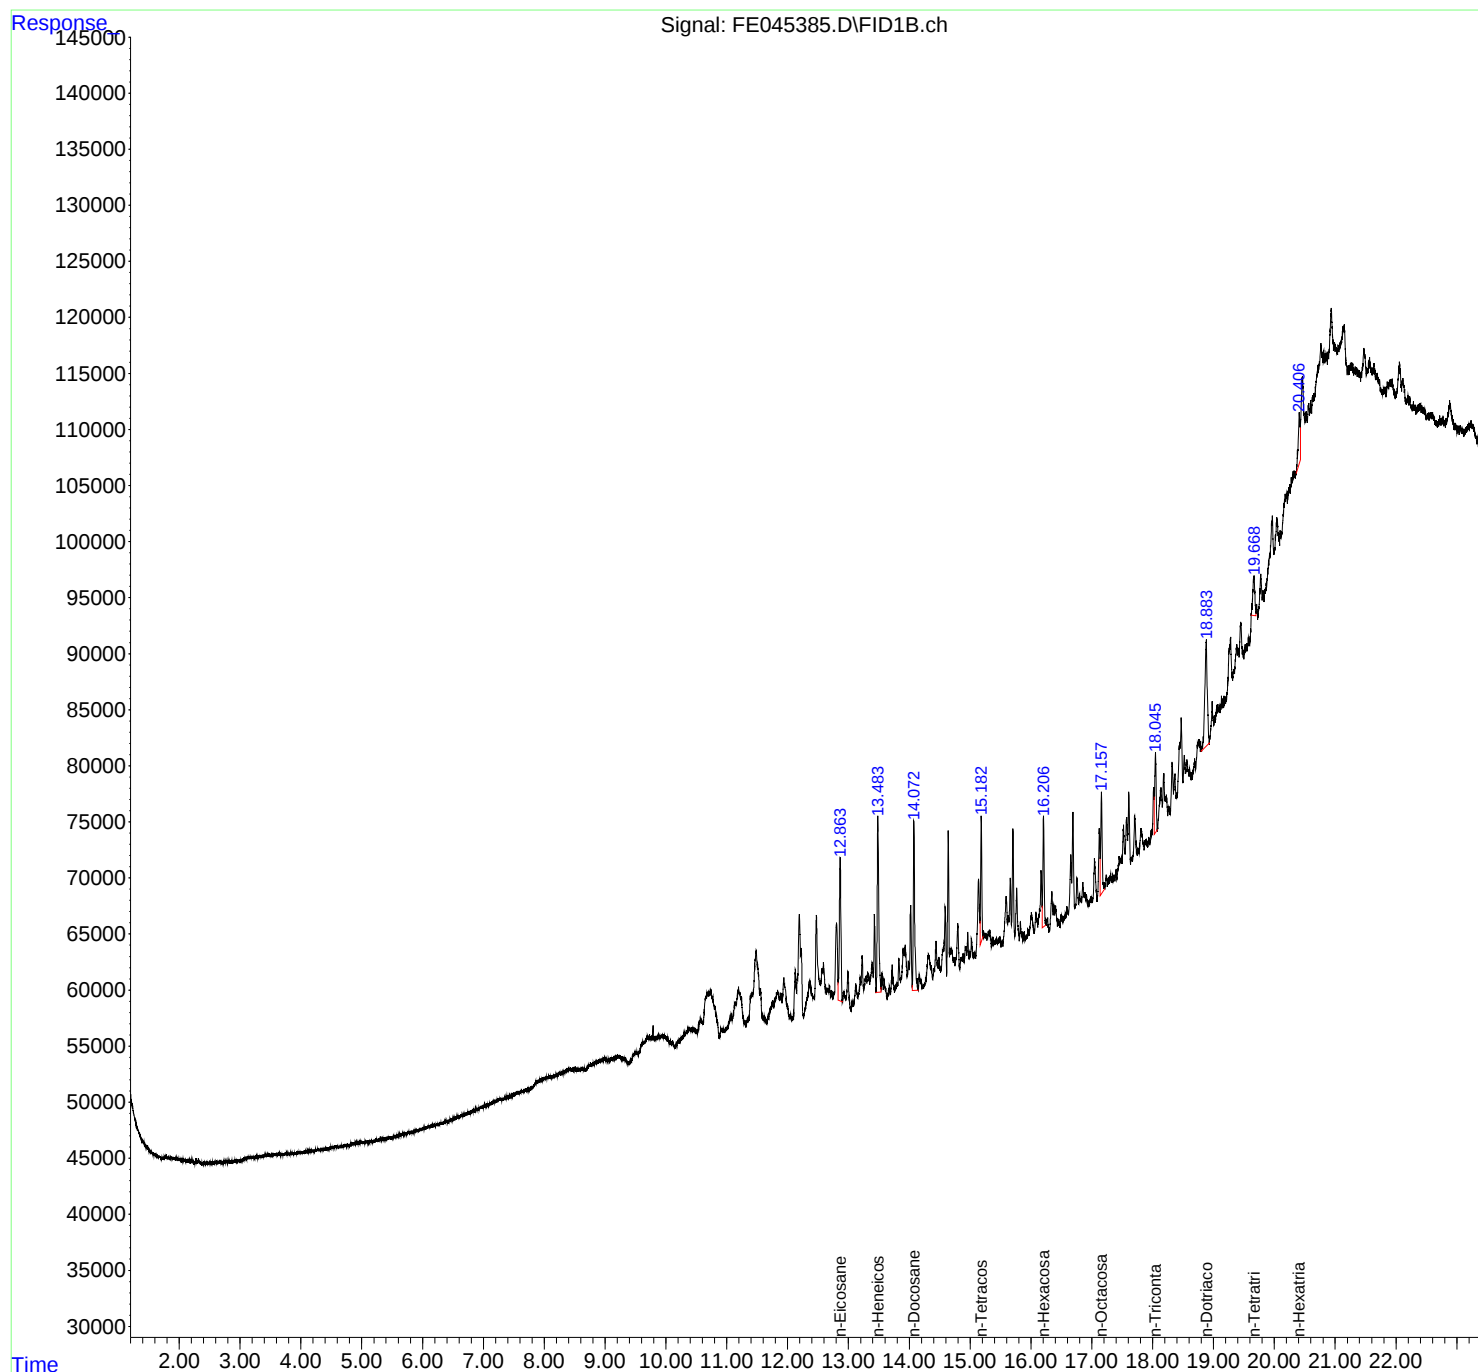


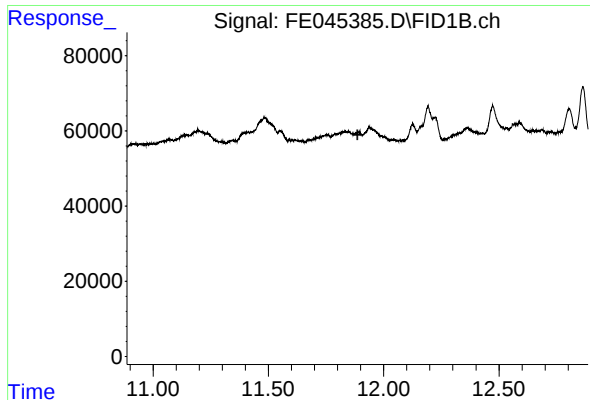

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.887 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

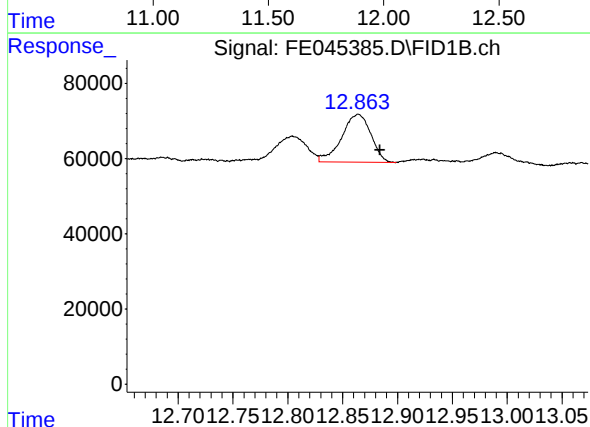


#10 n-Eicosane (C20)

R.T.: 12.864 min
Delta R.T.: -0.020 min
Response: 236580
Conc: 1.49 ug/ml

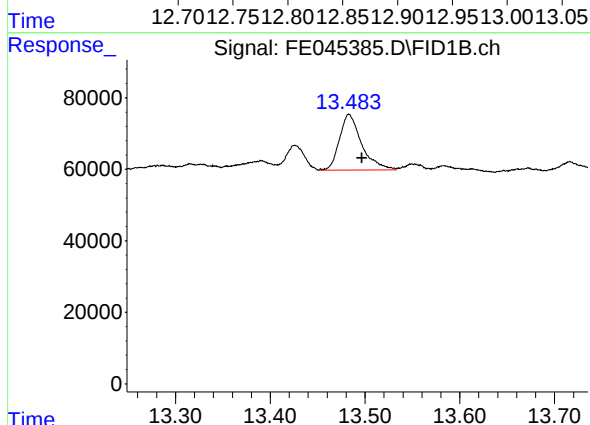


#11 n-Heneicosane (C21)

R.T.: 13.483 min
Delta R.T.: -0.014 min
Response: 252895
Conc: 1.64 ug/ml

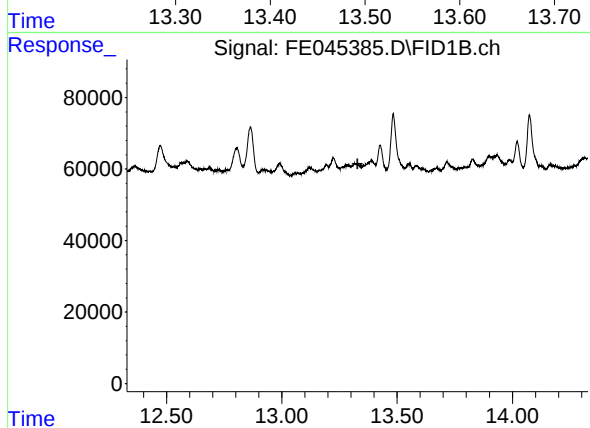

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.328 min
Response: 0
Conc: N.D.

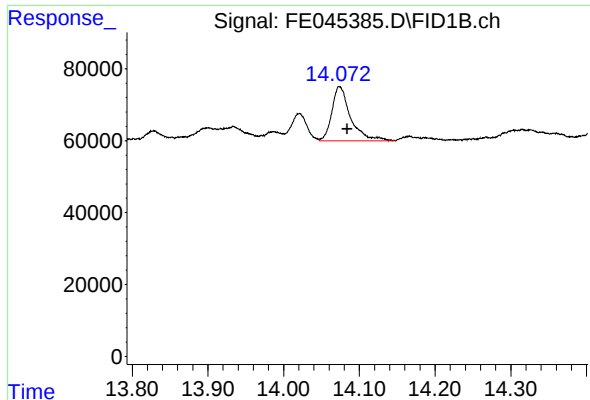

#13 n-Docosane (C22)


R.T.: 14.074 min
Delta R.T.: -0.010 min
Response: 260259
Conc: 1.72 ug/ml

Instrument :
FID_E
ClientSampleId :

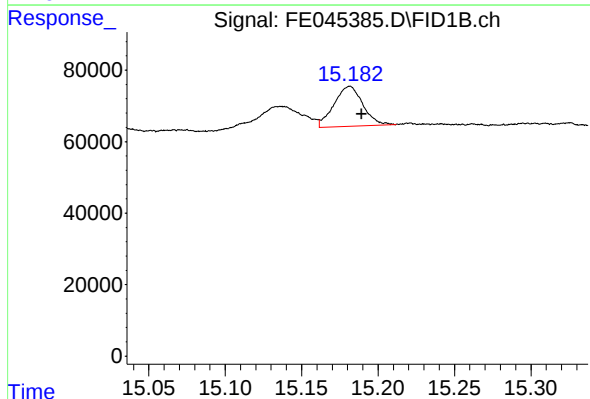


#14 n-Tetracosane (C24)

R.T.: 15.181 min
Delta R.T.: -0.008 min
Response: 146587
Conc: 0.99 ug/ml

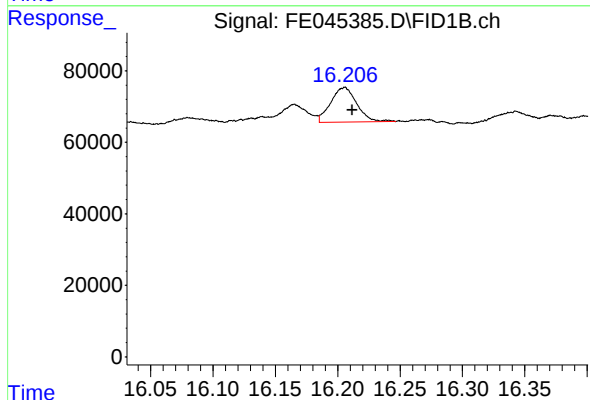


#15 n-Hexacosane (C26)

R.T.: 16.205 min
Delta R.T.: -0.006 min
Response: 142486
Conc: 0.98 ug/ml

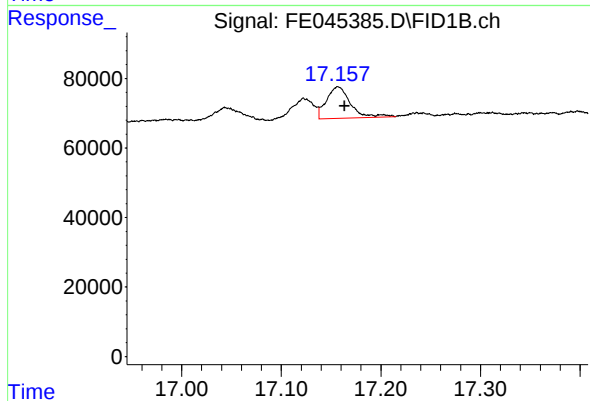

#16 n-Octacosane (C28)


R.T.: 17.157 min
Delta R.T.: -0.006 min
Response: 150331
Conc: 1.03 ug/ml

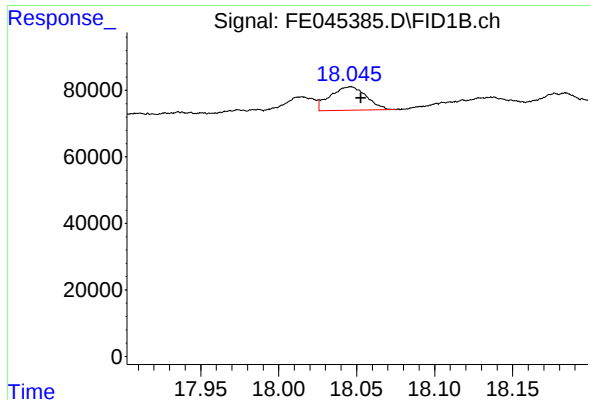

#17 n-Tricontane (C30)


R.T.: 18.046 min
Delta R.T.: -0.007 min
Response: 114294
Conc: 0.75 ug/ml

Instrument :
FID_E
ClientSampleId :

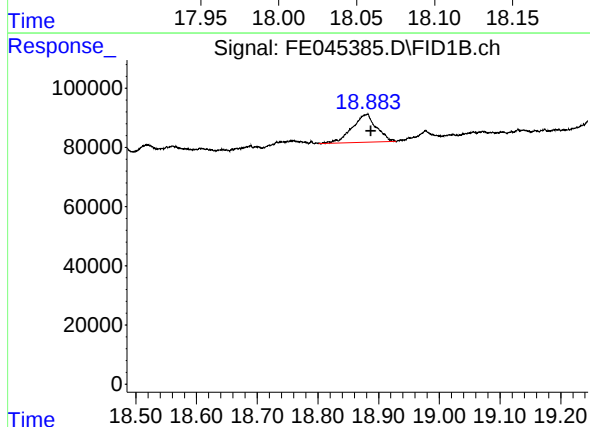


#18 n-Dotriacontane (C32)

R.T.: 18.881 min
Delta R.T.: -0.006 min
Response: 263993
Conc: 1.69 ug/ml

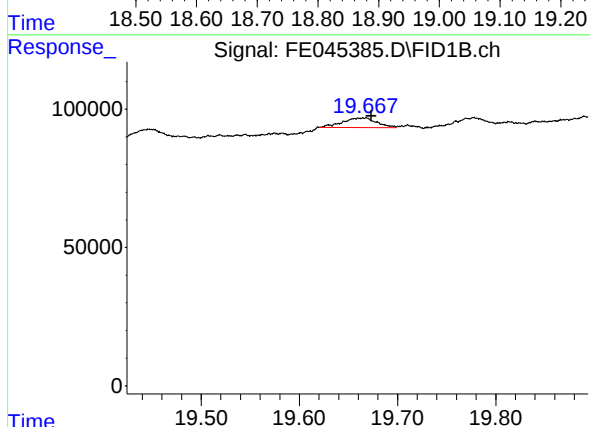

#19 n-Tetatriacontane (C34)

R.T.: 19.667 min
Delta R.T.: -0.006 min
Response: 82879
Conc: 0.53 ug/ml

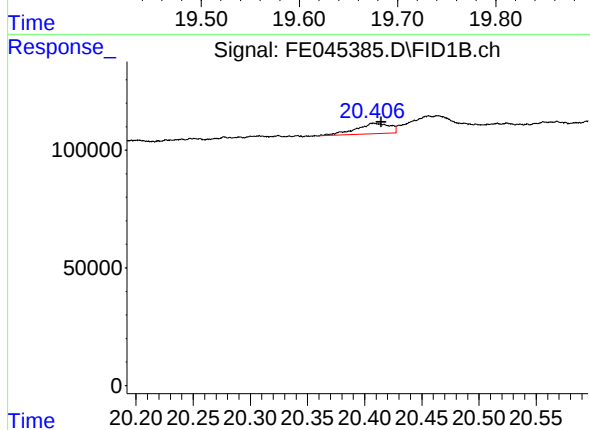

#20 n-Hexatriacontane (C36)

R.T.: 20.407 min
Delta R.T.: -0.007 min
Response: 93294
Conc: 0.57 ug/ml