

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE111723AL\  
 Data File : FE045417.D  
 Signal(s) : FID1B.ch  
 Acq On : 17 Nov 2023 10:05  
 Operator : YP\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :

Integration File: autoint1.e  
 Quant Time: Nov 17 21:33:29 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 110423.M  
 Quant Title : GC Extractables  
 QLast Update : Sat Nov 04 05:16:05 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                      | R.T.   | Response | Conc Units  |
|-------------------------------|--------|----------|-------------|
| -----                         |        |          |             |
| System Monitoring Compounds   |        |          |             |
| Target Compounds              |        |          |             |
| 18) T n-Dotriacontane (C32)   | 18.891 | 132639   | 0.849 ug/ml |
| 20) T n-Hexatriacontane (C36) | 20.449 | 151494   | 0.933 ug/ml |
| 22) T n-Tetracontane (C40)    | 22.102 | 159286   | 0.933 ug/ml |
| -----                         |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE111723AL\  
Data File : FE045417.D  
Signal(s) : FID1B.ch  
Acq On : 17 Nov 2023 10:05  
Operator : YP\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :

Integration File: autoint1.e  
Quant Time: Nov 17 21:33:29 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 110423.M  
Quant Title : GC Extractables  
QLast Update : Sat Nov 04 05:16:05 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

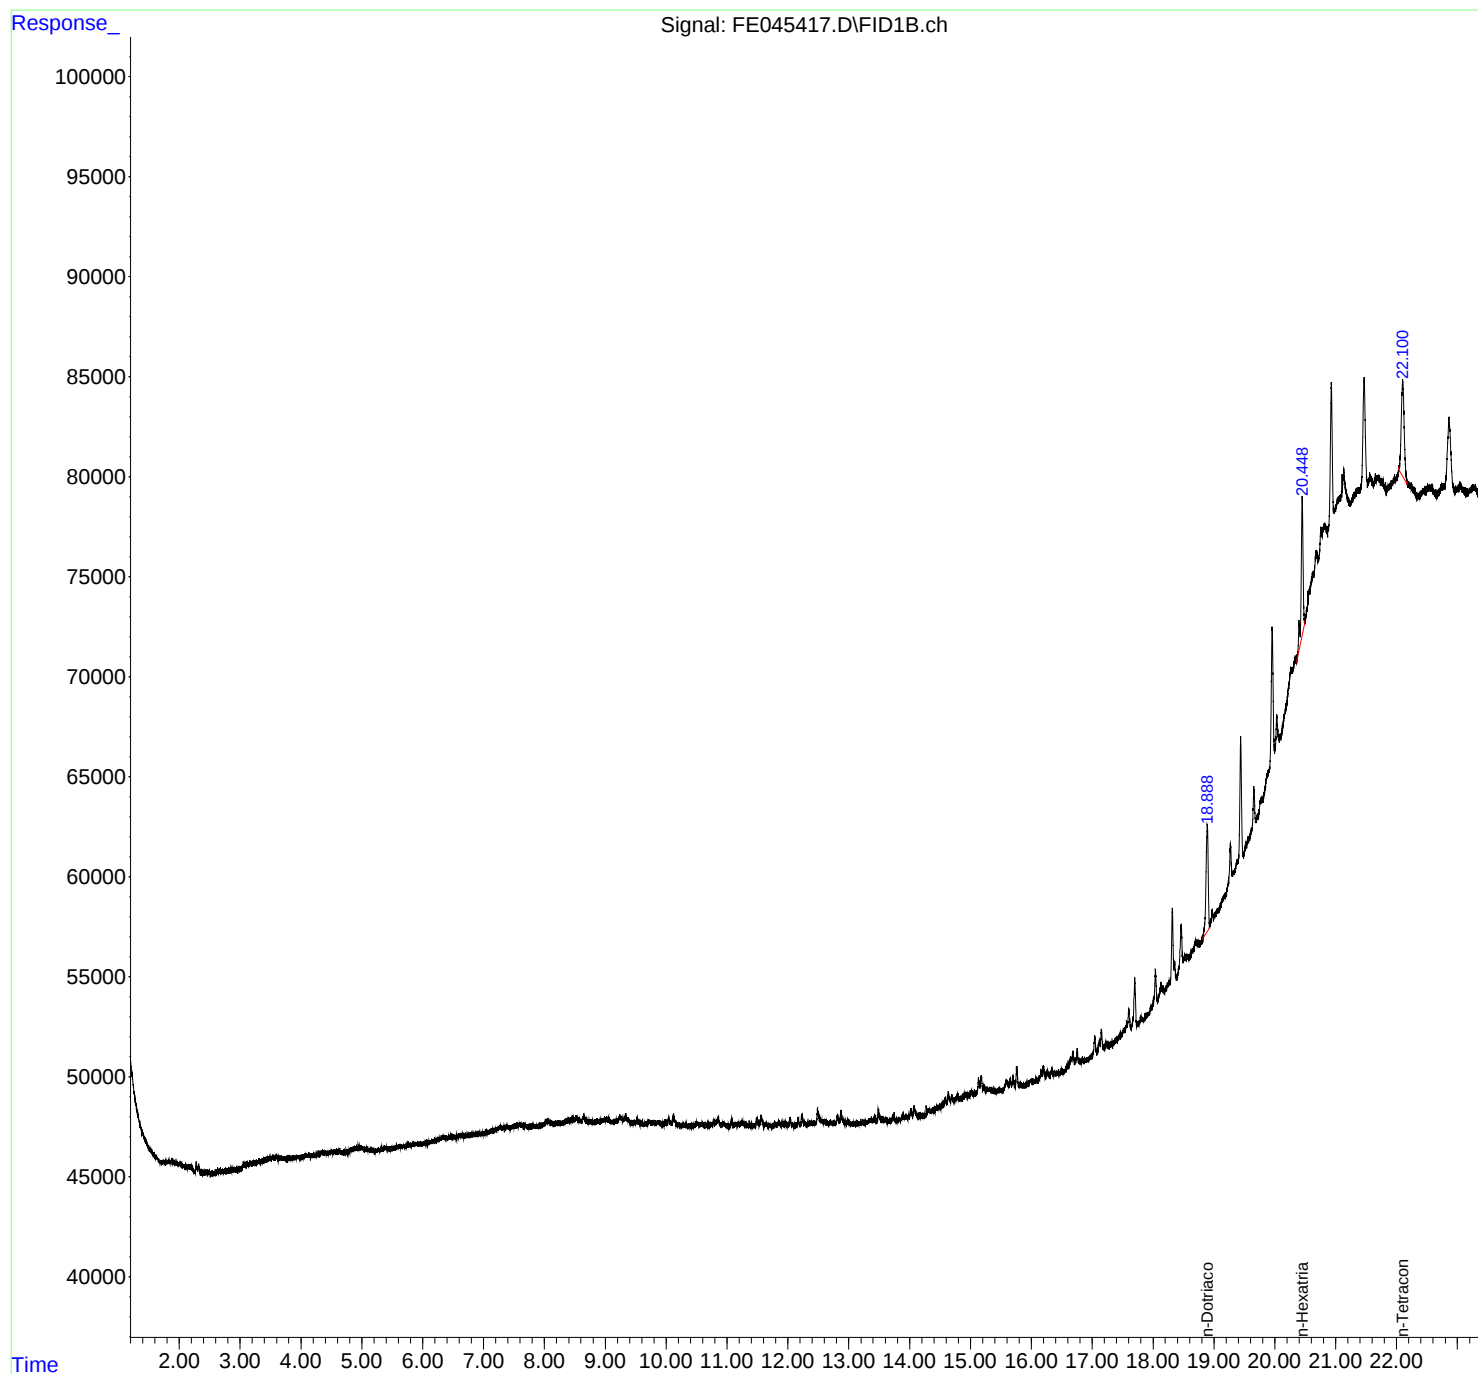


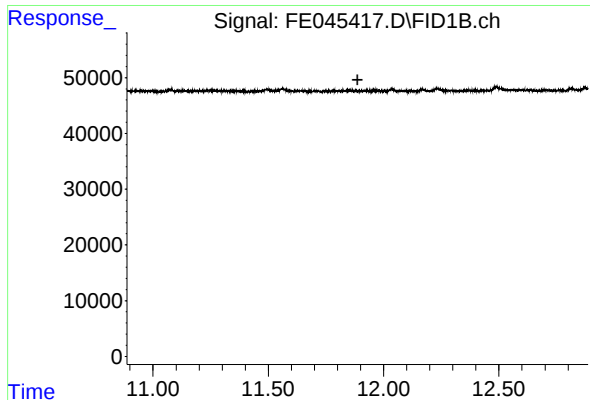

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min  
Exp R.T.: 11.887 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_E  
ClientSampleId :

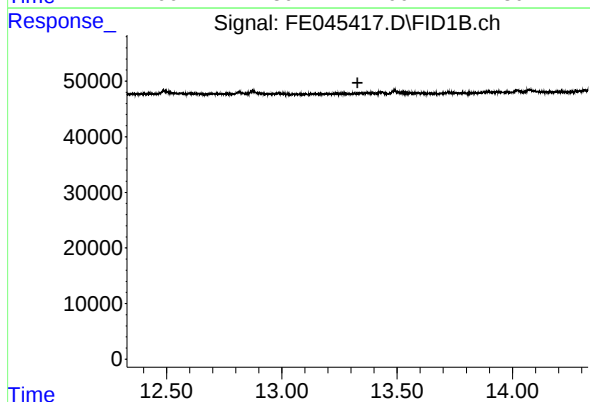


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min  
Exp R.T.: 13.328 min  
Response: 0  
Conc: N.D.

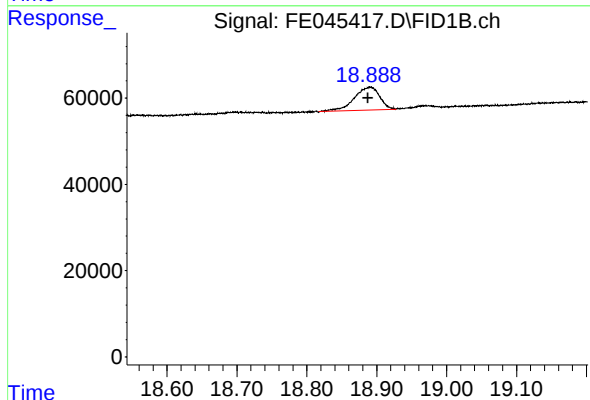


#18 n-Dotriacontane (C32)

R.T.: 18.891 min  
Delta R.T.: 0.003 min  
Response: 132639  
Conc: 0.85 ug/ml

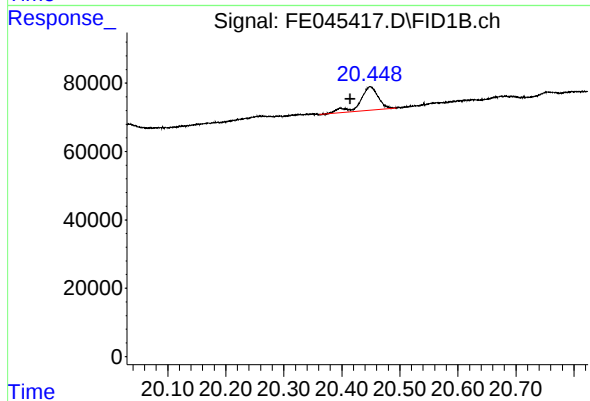

#20 n-Hexatriacontane (C36)

R.T.: 20.449 min  
Delta R.T.: 0.034 min  
Response: 151494  
Conc: 0.93 ug/ml

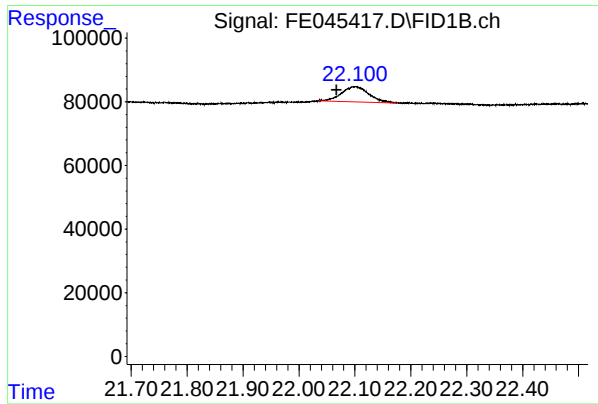

#22 n-Tetracontane (C40)

R.T.: 22.102 min  
Delta R.T.: 0.034 min  
Response: 159286  
Conc: 0.93 ug/ml

Instrument :  
FID\_E  
ClientSampleId :