

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111725AL\
Data File : FE056892.D
Signal(s) : FID1B.ch
Acq On : 18 Nov 2025 03:44
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 18 11:51:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 103025.M
Quant Title : GC Extractables
QLast Update : Thu Oct 30 12:50:27 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
19) T	n-Tetratriacontane (C34)	19.729	286838	1.662 ug/ml
20) T	n-Hexatriacontane (C36)	20.486	128126	0.886 ug/ml
21) T	n-Octatriacontane (C38)	21.325f	39404	0.313 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111725AL\
Data File : FE056892.D
Signal(s) : FID1B.ch
Acq On : 18 Nov 2025 03:44
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 18 11:51:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 103025.M
Quant Title : GC Extractables
QLast Update : Thu Oct 30 12:50:27 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

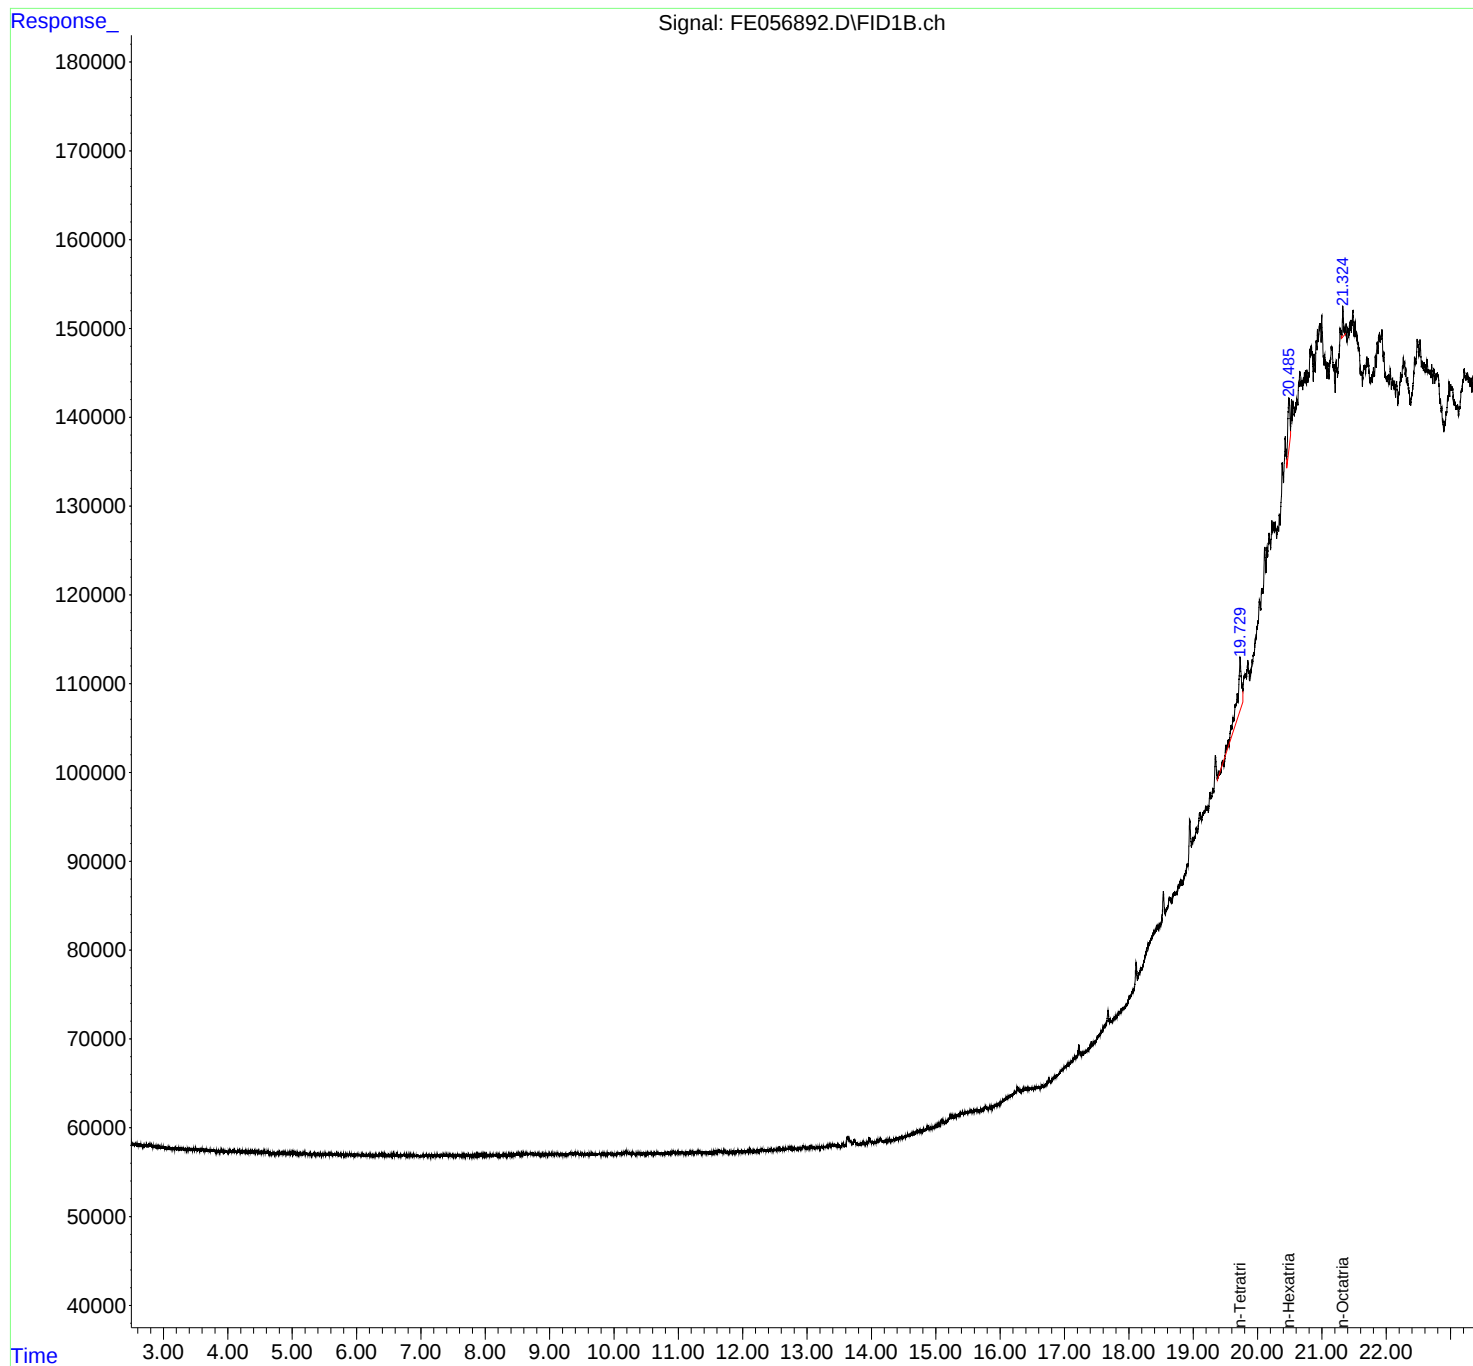


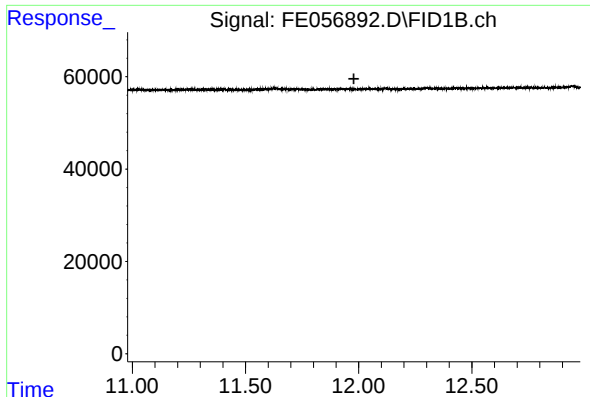

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.979 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

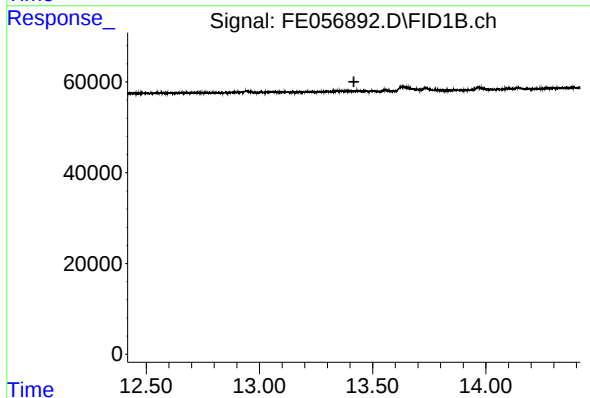


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.417 min
Response: 0
Conc: N.D.

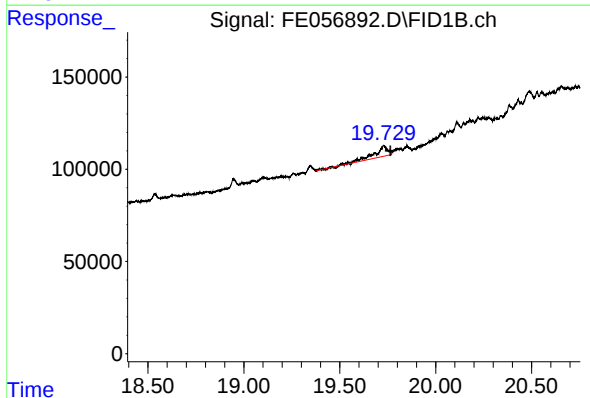


#19 n-Tetratriacontane (C34)

R.T.: 19.729 min
Delta R.T.: -0.036 min
Response: 286838
Conc: 1.66 ug/ml

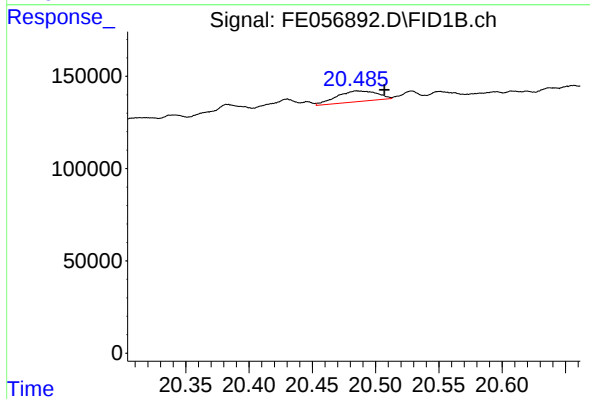

#20 n-Hexatriacontane (C36)

R.T.: 20.486 min
Delta R.T.: -0.020 min
Response: 128126
Conc: 0.89 ug/ml

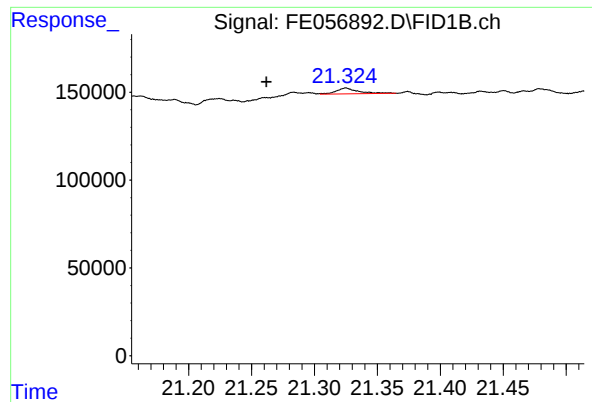

#21 n-Octatriacontane (C38)

R.T.: 21.325 min
Delta R.T.: 0.063 min
Response: 39404
Conc: 0.31 ug/ml

Instrument :

FID_E

ClientSampleId :