

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111819\
 Data File : FE030888.D
 Signal(s) : FID1B.CH
 Acq On : 18 Nov 2019 12:31
 Operator : DD\AJ
 Sample : K5864-08 50X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 19 00:25:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
 Quant Title :
 QLast Update : Thu Oct 31 08:47:02 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.421	252040	0.662 ug/ml
4) N-TETRADECANE	8.243	483473	1.291 ug/ml
5) N-HEXADECANE	9.760f	633149	1.698 ug/ml
7) N-EICOSANE	12.617	357041	0.977 ug/ml
13) N-TRIACONTANE	17.726	258305	0.778 ug/ml
14) N-DOTRIACONTANE	18.561	531629	1.665 ug/ml
15) N-TETRATRIACONTANE	19.346	491008	1.613 ug/ml
16) N-HEXATRIACONTANE	20.089	2881168	10.494 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111819\
Data File : FE030888.D
Signal(s) : FID1B.CH
Acq On : 18 Nov 2019 12:31
Operator : DD\AJ
Sample : K5864-08 50X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 19 00:25:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
Quant Title :
QLast Update : Thu Oct 31 08:47:02 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

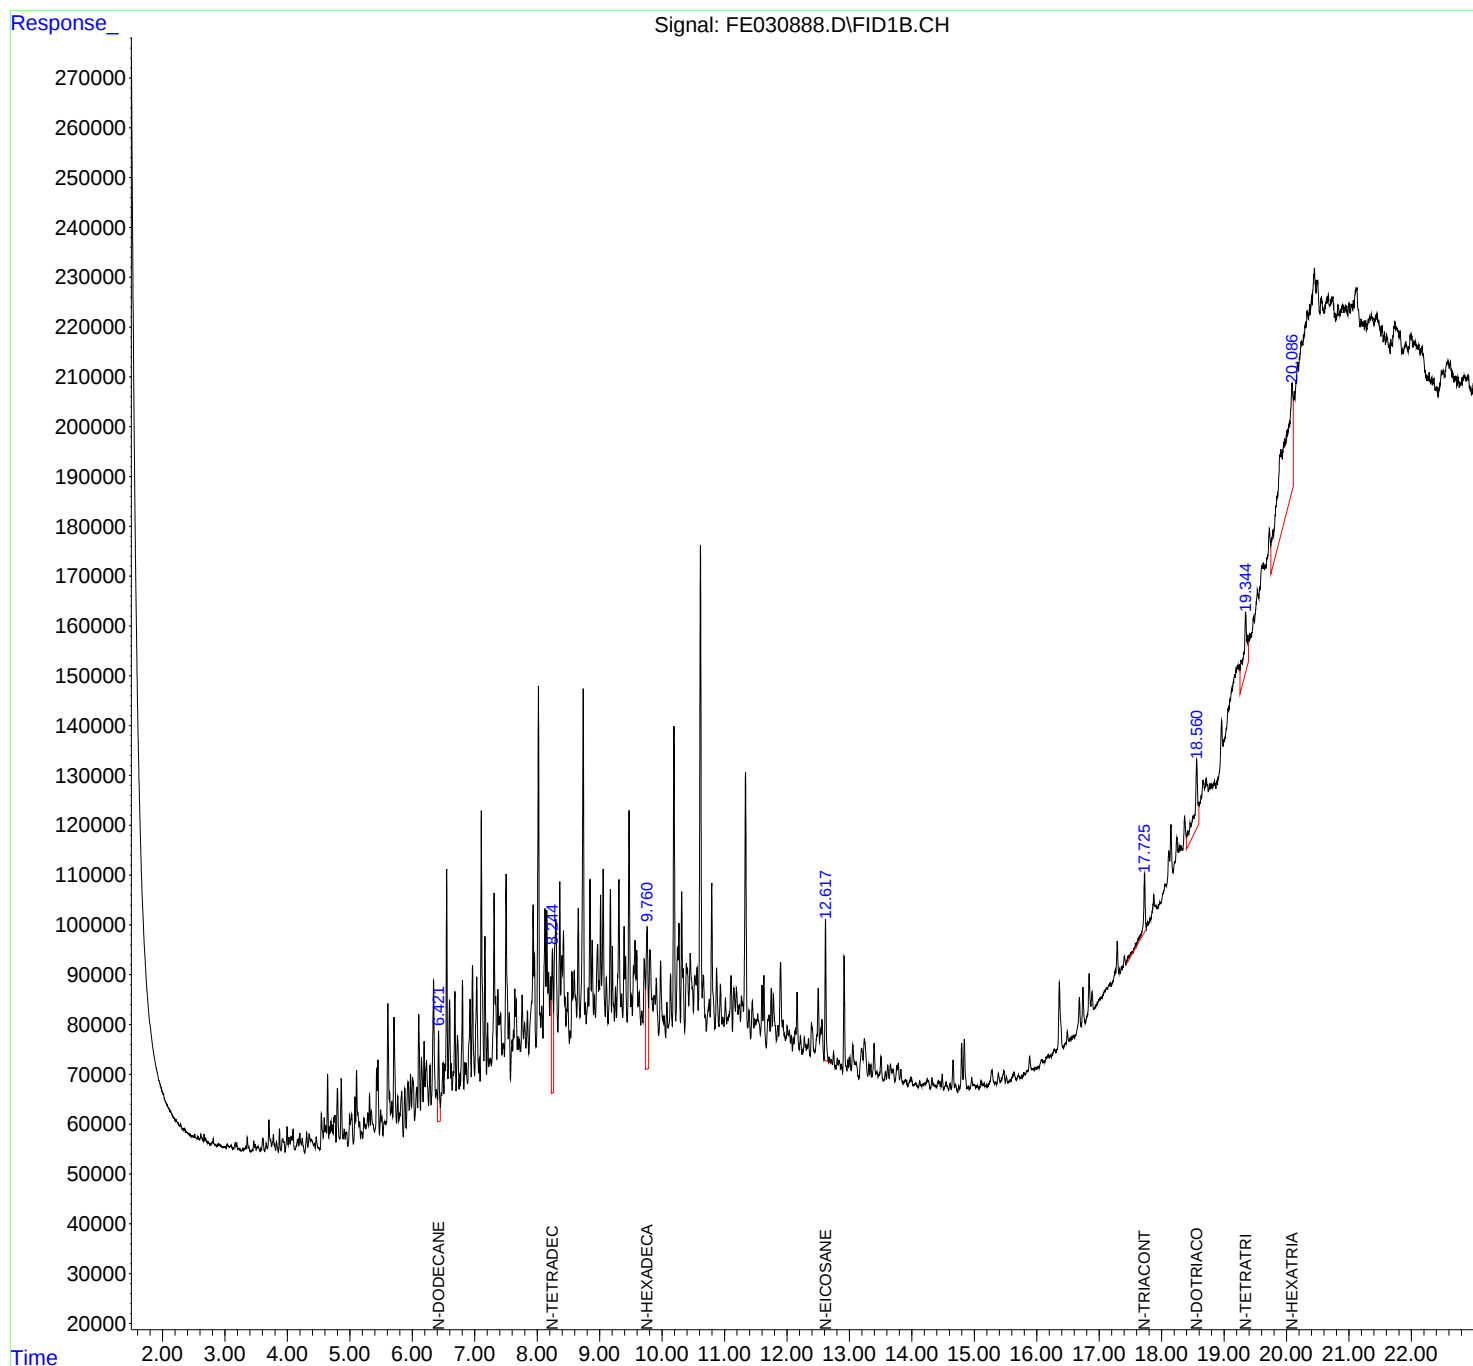


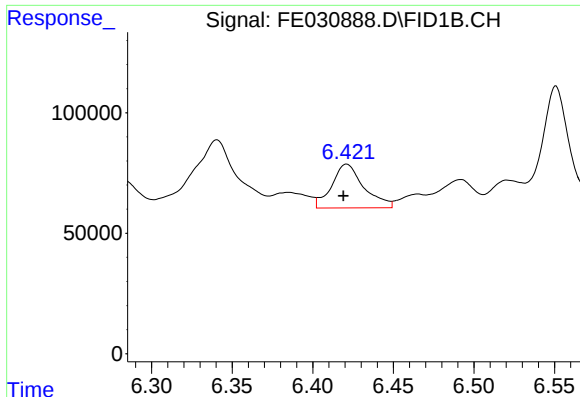

#3 N-DODECANE


R.T.: 6.421 min
Delta R.T.: 0.002 min
Response: 252040
Conc: 0.66 ug/ml

Instrument :
FID_E
ClientSampleId :

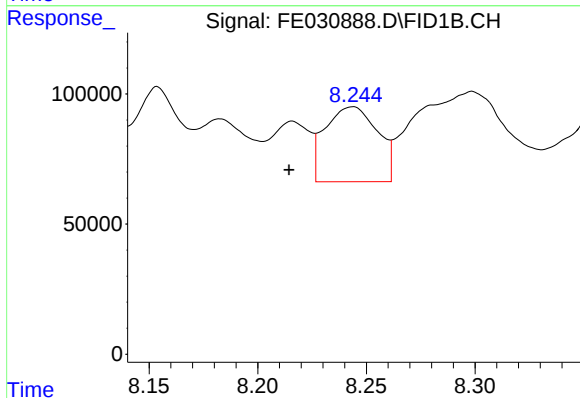


#4 N-TETRADECANE

R.T.: 8.243 min
Delta R.T.: 0.029 min
Response: 483473
Conc: 1.29 ug/ml

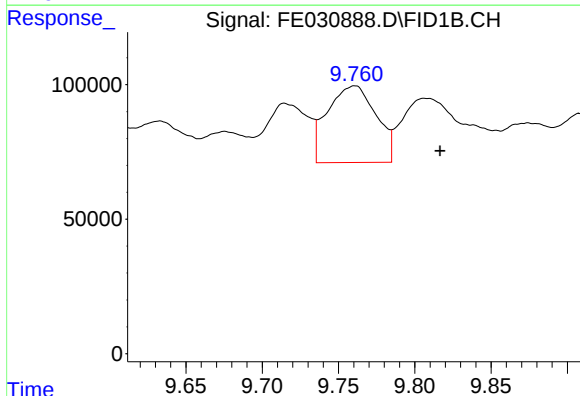


#5 N-HEXADECANE

R.T.: 9.760 min
Delta R.T.: -0.057 min
Response: 633149
Conc: 1.70 ug/ml

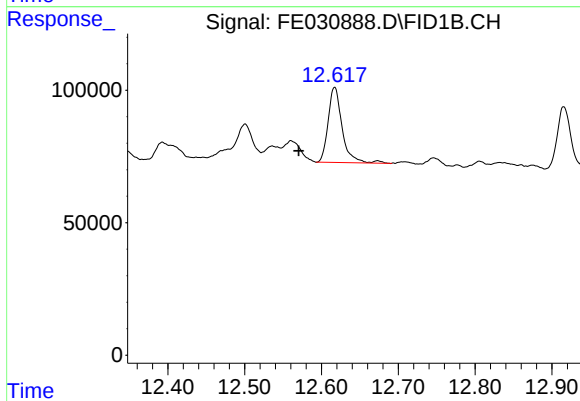

#7 N-EICOSANE


R.T.: 12.617 min
Delta R.T.: 0.047 min
Response: 357041
Conc: 0.98 ug/ml

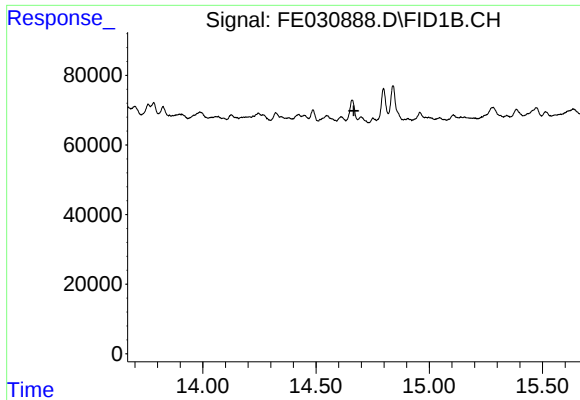

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.667 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

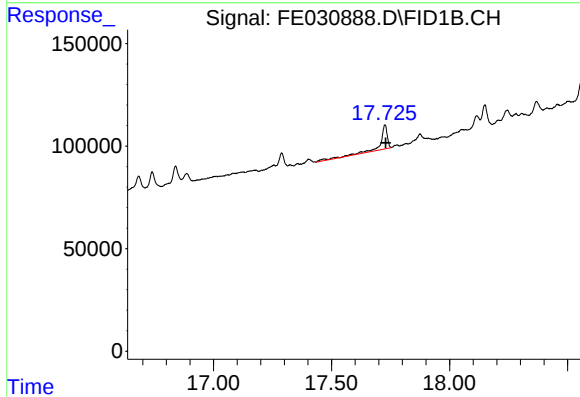


#13 N-TRIACONTANE

R.T.: 17.726 min
Delta R.T.: -0.004 min
Response: 258305
Conc: 0.78 ug/ml

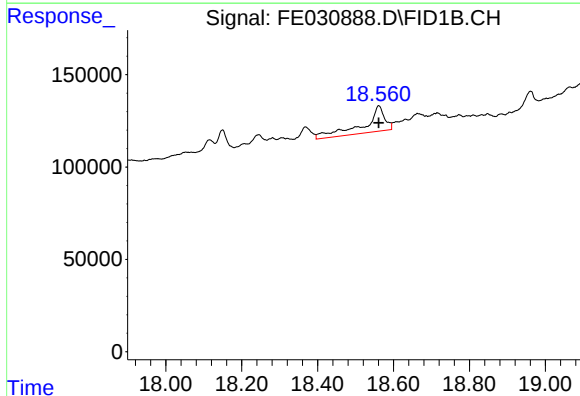


#14 N-DOTRIACONTANE

R.T.: 18.561 min
Delta R.T.: 0.000 min
Response: 531629
Conc: 1.67 ug/ml

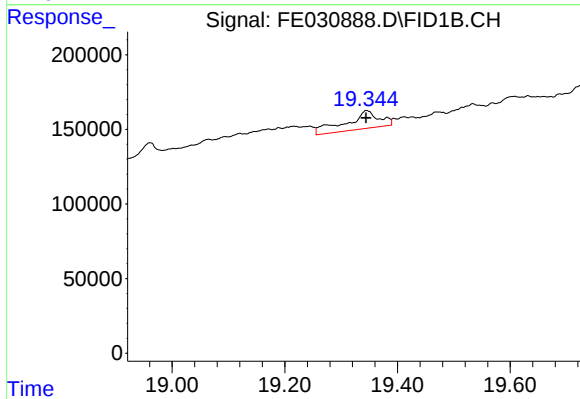

#15 N-TETRATRIACONTANE

R.T.: 19.346 min
Delta R.T.: 0.001 min
Response: 491008
Conc: 1.61 ug/ml

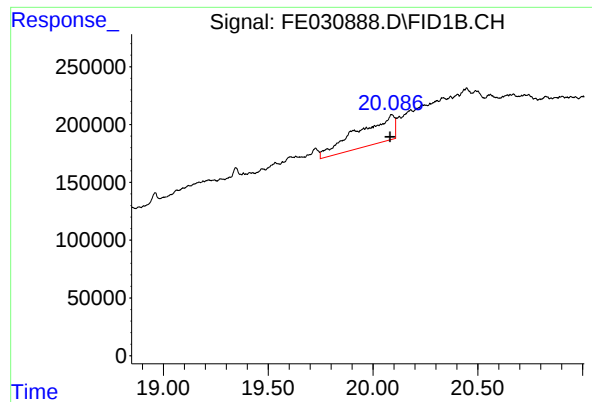

#16 N-HEXATRIACONTANE

R.T.: 20.089 min
Delta R.T.: 0.007 min
Response: 2881168
Conc: 10.49 ug/ml

Instrument :
FID_E
ClientSampleId :