

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111919\
 Data File : FE030901.D
 Signal(s) : FID1B.CH
 Acq On : 19 Nov 2019 16:59
 Operator : DD\AJ
 Sample : PB124941BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 20 00:52:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
 Quant Title :
 QLast Update : Thu Oct 31 08:47:02 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.662	4962395	15.967 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.558	213120	0.668 ug/ml
15) N-TETRATRIACONTANE	19.350	142338	0.467 ug/ml
16) N-HEXATRIACONTANE	20.021f	133122	0.485 ug/ml
18) N-TETRACONTANE	21.731	412986	1.572 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE111919\
Data File : FE030901.D
Signal(s) : FID1B.CH
Acq On : 19 Nov 2019 16:59
Operator : DD\AJ
Sample : PB124941BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 20 00:52:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
Quant Title :
QLast Update : Thu Oct 31 08:47:02 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

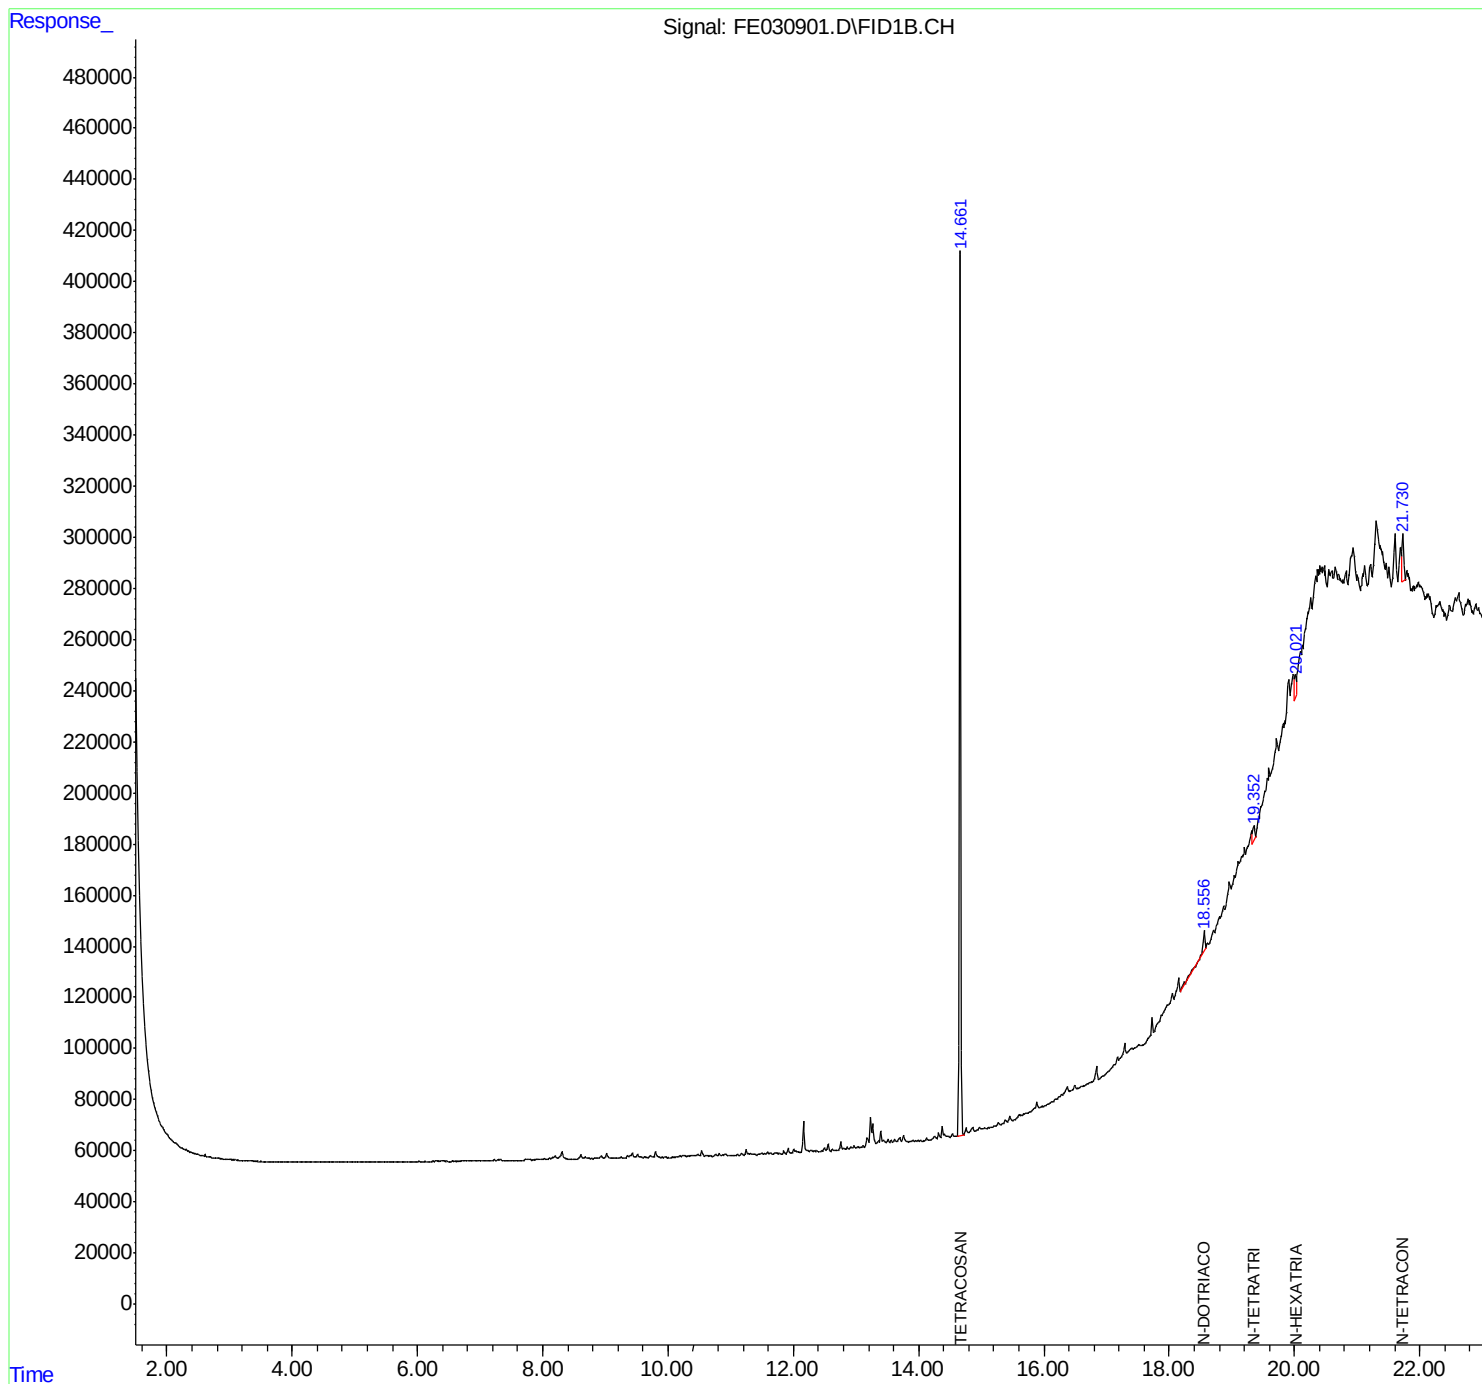

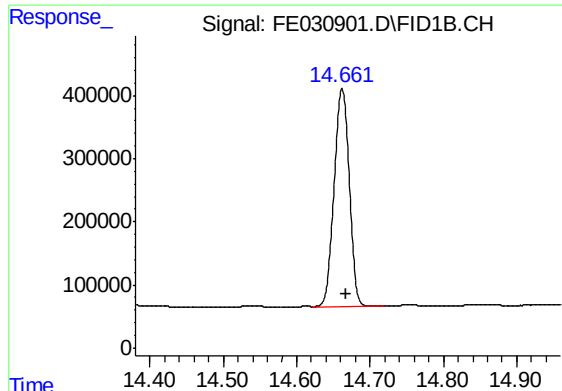


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.662 min
Delta R.T.: -0.005 min
Response: 4962395
Conc: 15.97 ug/ml

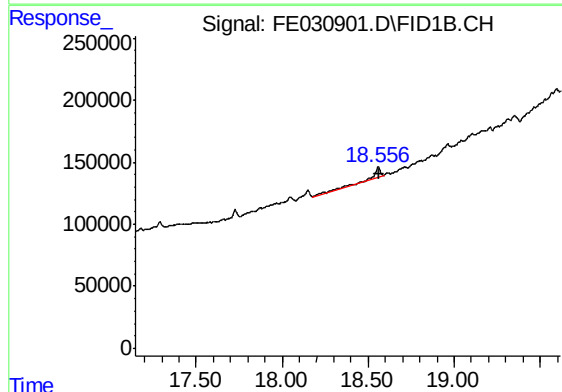


#14 N-DOTRIACONTANE

R.T.: 18.558 min
Delta R.T.: -0.003 min
Response: 213120
Conc: 0.67 ug/ml

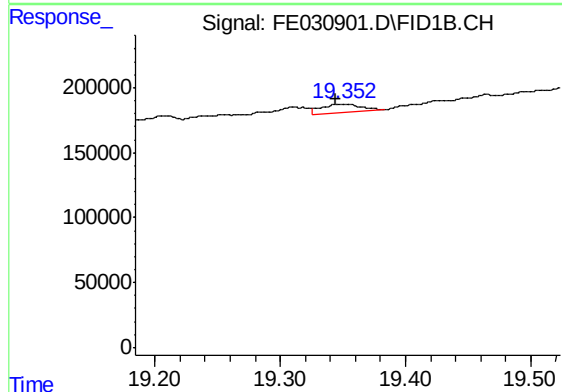


#15 N-TETRATRIACONTANE

R.T.: 19.350 min
Delta R.T.: 0.006 min
Response: 142338
Conc: 0.47 ug/ml

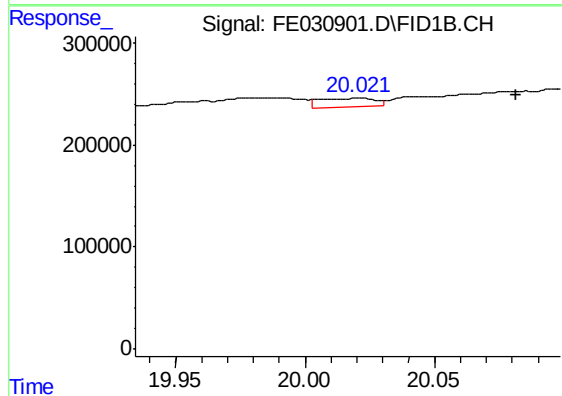

#16 N-HEXATRIACONTANE

R.T.: 20.021 min
Delta R.T.: -0.061 min
Response: 133122
Conc: 0.48 ug/ml

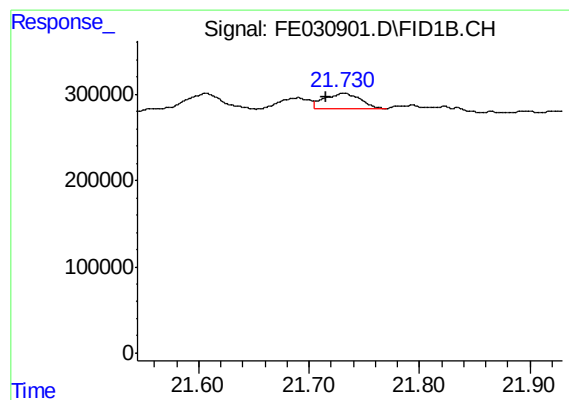

#18 N-TETRACONTANE

R.T.: 21.731 min
Delta R.T.: 0.015 min
Response: 412986
Conc: 1.57 ug/ml