

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112018\
 Data File : FE029264.D
 Signal(s) : FID1B.CH
 Acq On : 20 Nov 2018 15:29
 Operator : AJ\SJ
 Sample : J6010-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 21 06:14:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE111618.M
 Quant Title :
 QLast Update : Fri Nov 16 14:56:57 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.852	3790145	20.536 ug/ml
Target Compounds			
4) N-UNDECANE	5.628	55273	0.348 ug/ml
5) N-DODECANE	6.645	105052	0.649 ug/ml
6) N-TETRADECANE	8.416	927879	5.498 ug/ml
7) N-HEXADECANE	10.012	16368321	90.160 ug/ml
8) N-OCTADECANE	11.456	17552549	93.397 ug/ml
10) N-TETRACOSANE	15.099	2723735	15.090 ug/ml
11) N-OCTACOSANE	17.041	598906	3.690 ug/ml
12) N-DOTRIACONTANE	18.759	459150	3.029 ug/ml
14) N-HEXATRIACONTANE	20.330	64482	0.423 ug/ml
15) N-TETRACONTANE	22.038	605275	4.017 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112018\
Data File : FE029264.D
Signal(s) : FID1B.CH
Acq On : 20 Nov 2018 15:29
Operator : AJ\SJ
Sample : J6010-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 21 06:14:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE111618.M
Quant Title :
QLast Update : Fri Nov 16 14:56:57 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

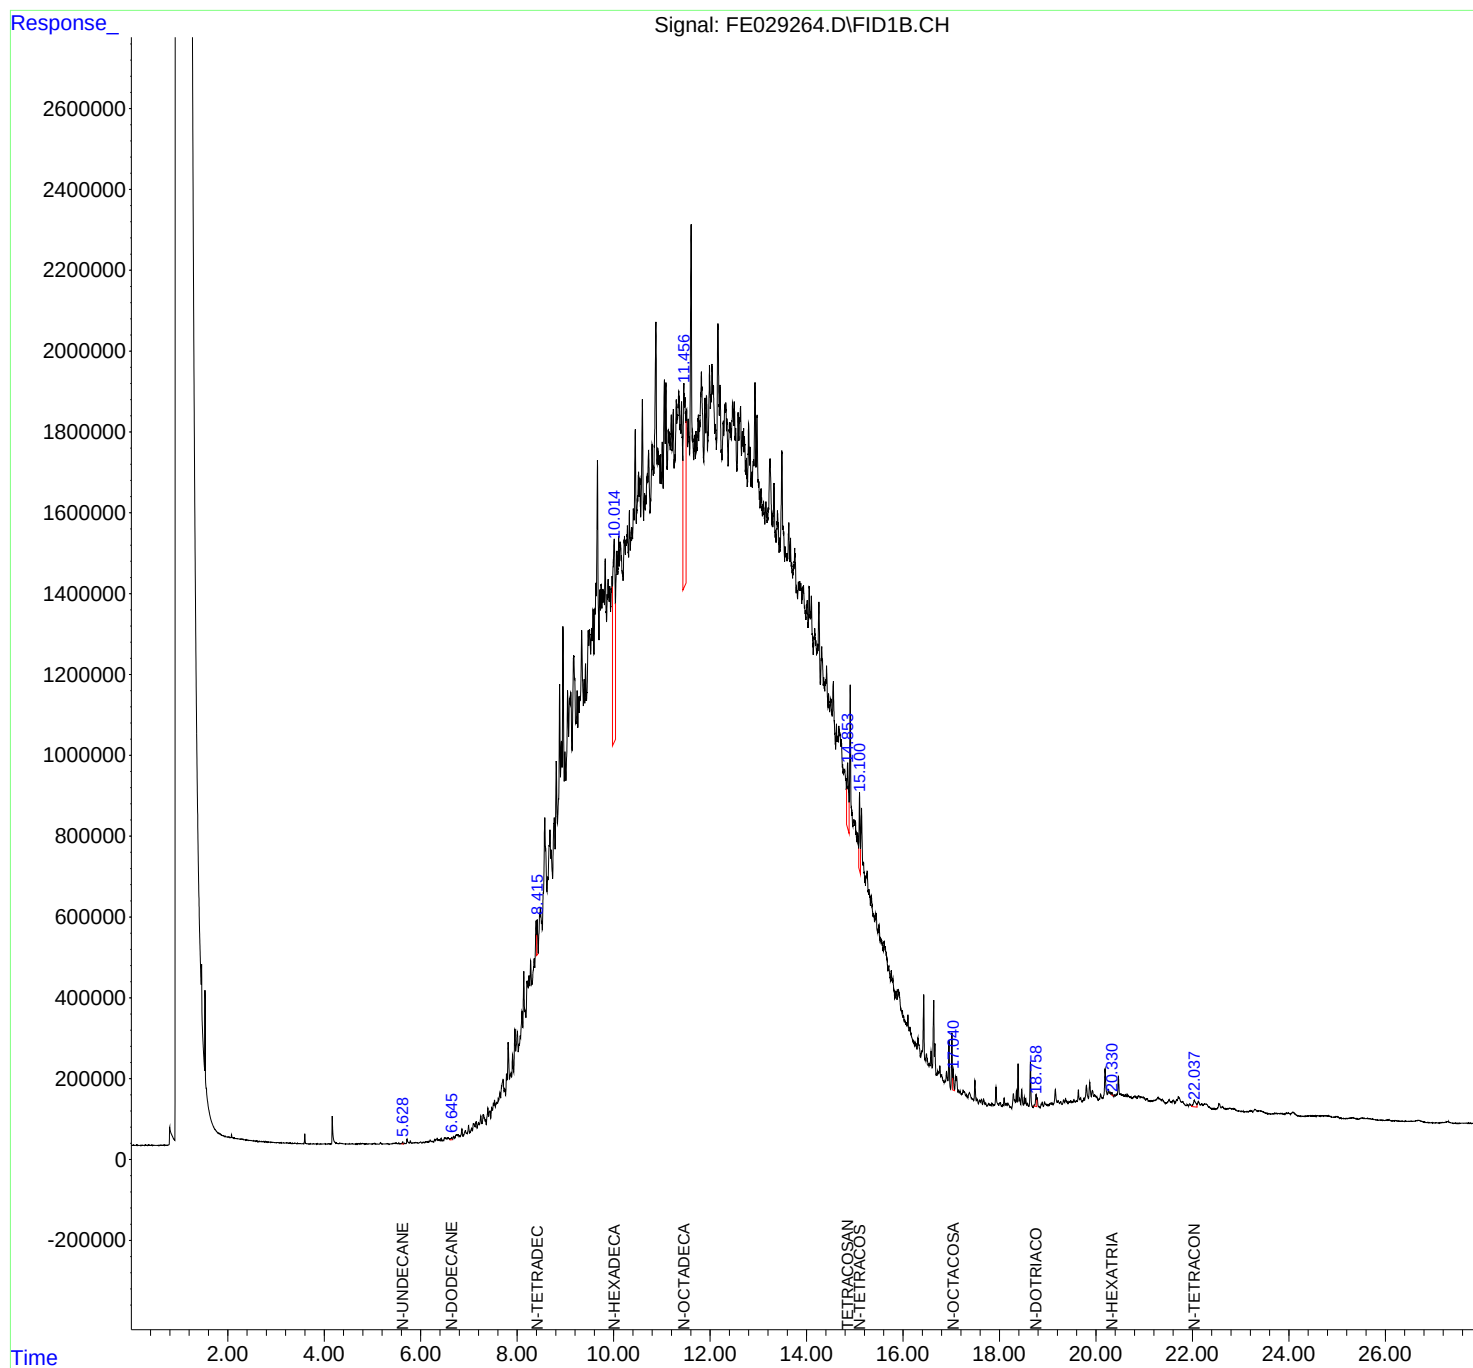

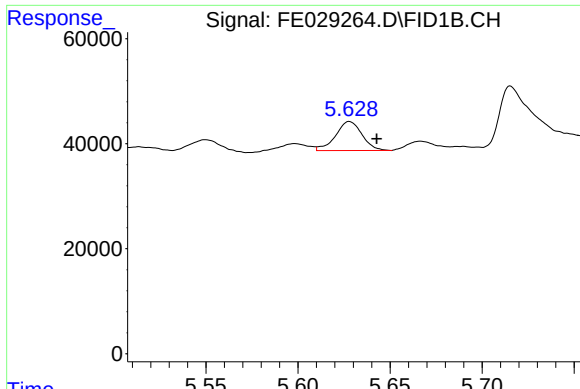


#4 N-UNDECANE

R.T.: 5.628 min
Delta R.T.: -0.015 min
Response: 55273
Conc: 0.35 ug/ml

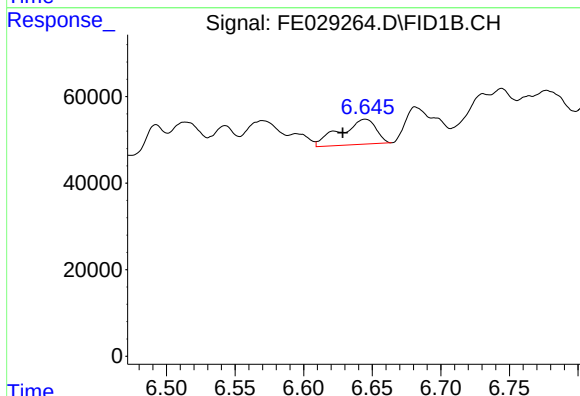


#5 N-DODECANE

R.T.: 6.645 min
Delta R.T.: 0.016 min
Response: 105052
Conc: 0.65 ug/ml

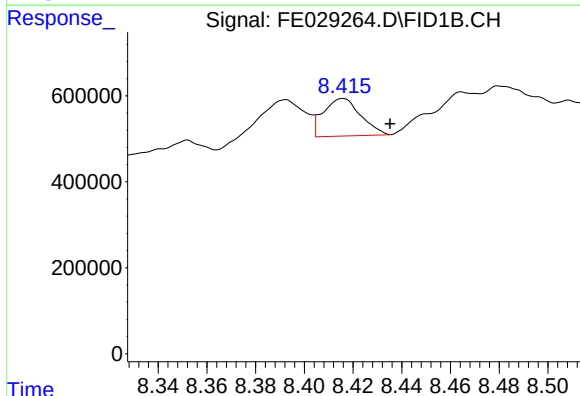


#6 N-TETRADECANE

R.T.: 8.416 min
Delta R.T.: -0.019 min
Response: 927879
Conc: 5.50 ug/ml

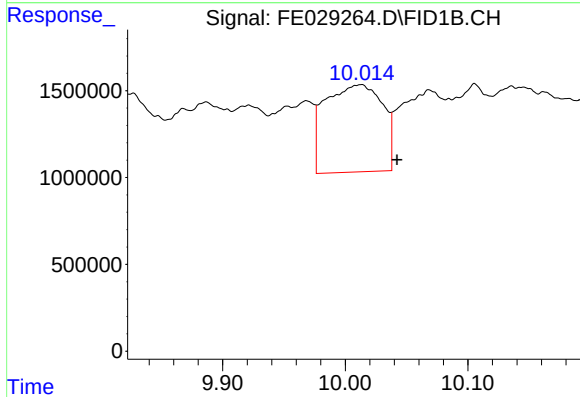


#7 N-HEXADECANE

R.T.: 10.012 min
Delta R.T.: -0.031 min
Response: 16368321
Conc: 90.16 ug/ml

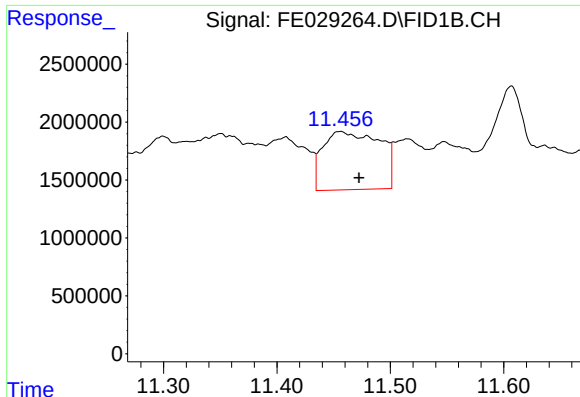


#8 N-OCTADECANE

R.T.: 11.456 min
Delta R.T.: -0.017 min
Response: 17552549
Conc: 93.40 ug/ml

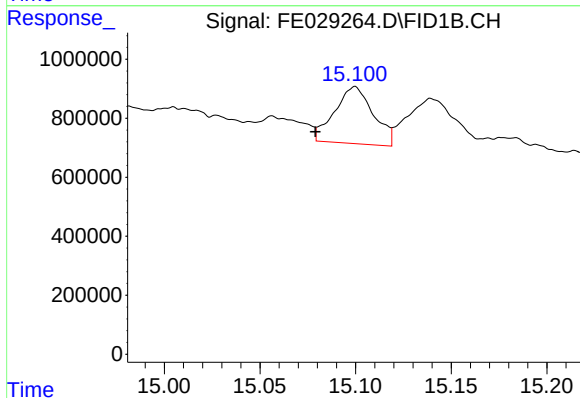


#10 N-TETRACOSANE

R.T.: 15.099 min
Delta R.T.: 0.020 min
Response: 2723735
Conc: 15.09 ug/ml

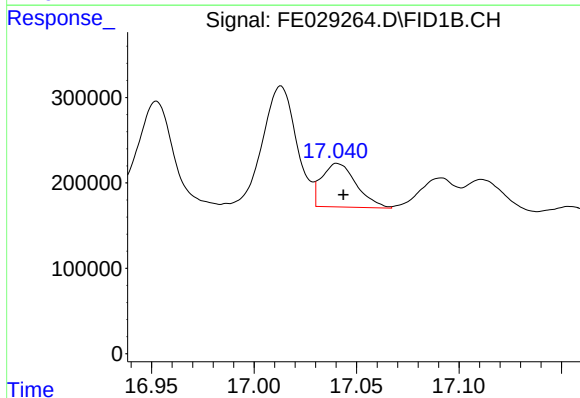


#11 N-OCTACOSANE

R.T.: 17.041 min
Delta R.T.: -0.003 min
Response: 598906
Conc: 3.69 ug/ml

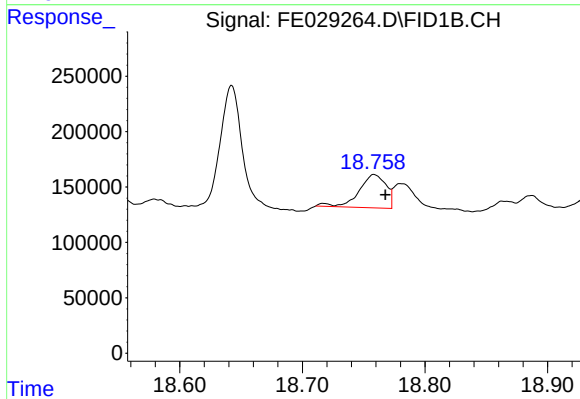


#12 N-DOTRIACONTANE

R.T.: 18.759 min
Delta R.T.: -0.009 min
Response: 459150
Conc: 3.03 ug/ml

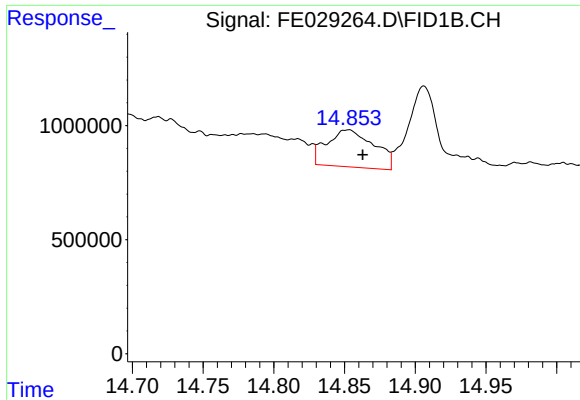


#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.852 min
Delta R.T.: -0.011 min
Response: 3790145
Conc: 20.54 ug/ml

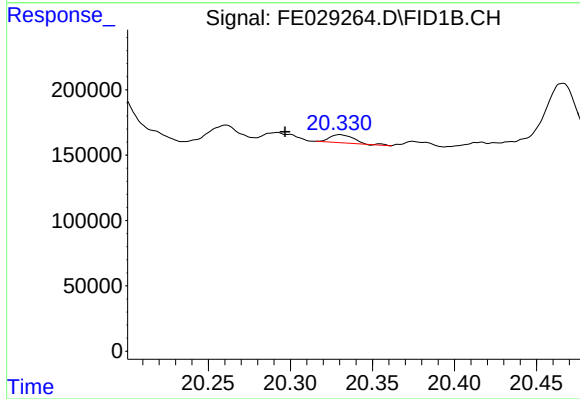

#14 N-HEXATRIACONTANE

R.T.: 20.330 min
Delta R.T.: 0.034 min
Response: 64482
Conc: 0.42 ug/ml

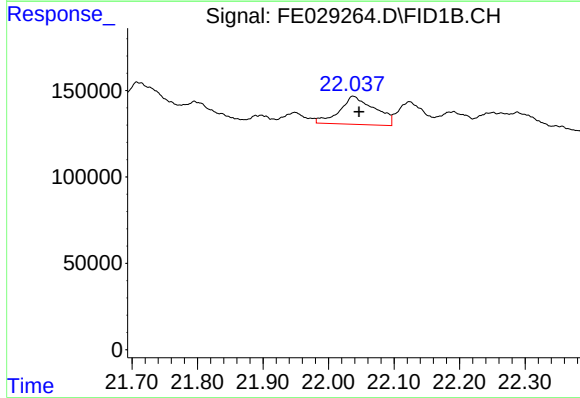

#15 N-TETRACONTANE

R.T.: 22.038 min
Delta R.T.: -0.009 min
Response: 605275
Conc: 4.02 ug/ml