

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112018\
 Data File : FE029268.D
 Signal(s) : FID1B.CH
 Acq On : 20 Nov 2018 18:01
 Operator : AJ\SJ
 Sample : J6006-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 21 06:15:44 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE111618.M
 Quant Title :
 QLast Update : Fri Nov 16 14:56:57 2018
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.850	2655379	14.387 ug/ml
Target Compounds			
5) N-DODECANE	6.590	115123	0.711 ug/ml
6) N-TETRADECANE	8.450	128651	0.762 ug/ml
7) N-HEXADECANE	9.983	50674	0.279 ug/ml
8) N-OCTADECANE	11.429	76776	0.409 ug/ml
9) N-EICOSANE	12.744	52501	0.281 ug/ml
10) N-TETRACOSANE	15.050	141053	0.781 ug/ml
11) N-OCTACOSANE	17.027	344508	2.123 ug/ml
12) N-DOTRIACONTANE	18.747	276589	1.824 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112018\
Data File : FE029268.D
Signal(s) : FID1B.CH
Acq On : 20 Nov 2018 18:01
Operator : AJ\SJ
Sample : J6006-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 21 06:15:44 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE111618.M
Quant Title :
QLast Update : Fri Nov 16 14:56:57 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

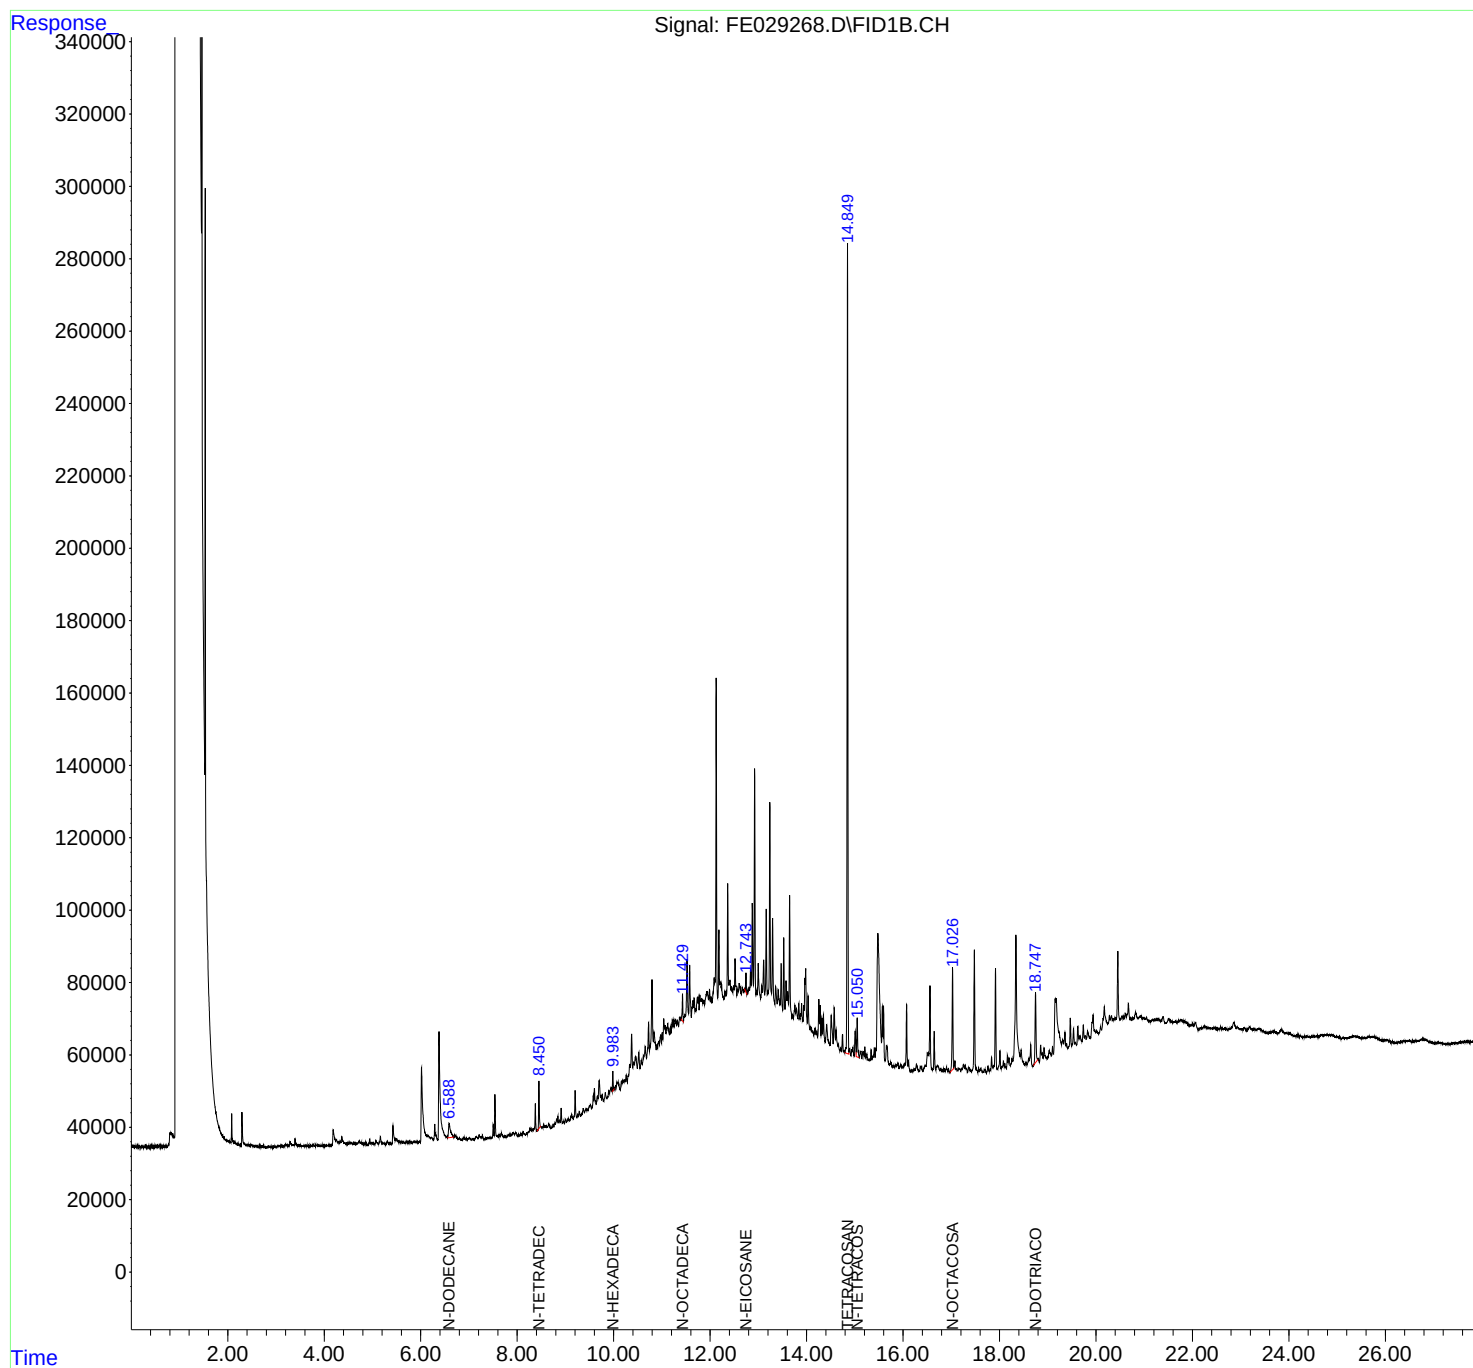

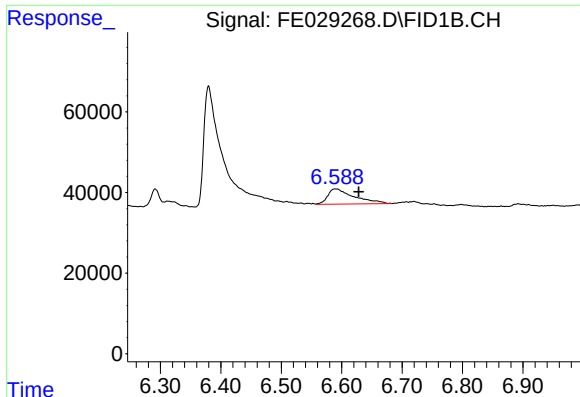


#5 N-DODECANE

R.T.: 6.590 min
Delta R.T.: -0.039 min
Response: 115123
Conc: 0.71 ug/ml

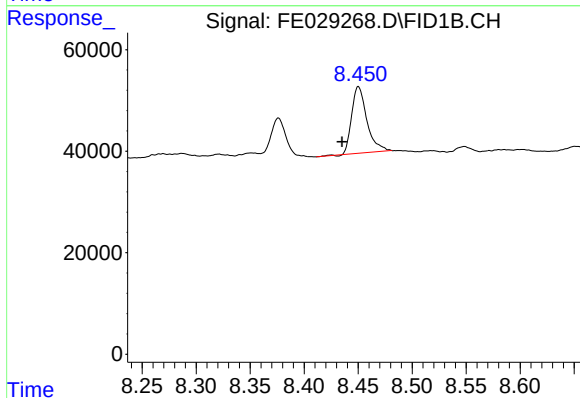


#6 N-TETRADECANE

R.T.: 8.450 min
Delta R.T.: 0.015 min
Response: 128651
Conc: 0.76 ug/ml

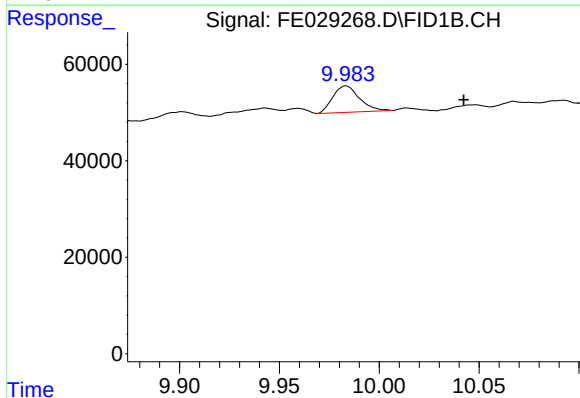


#7 N-HEXADECANE

R.T.: 9.983 min
Delta R.T.: -0.059 min
Response: 50674
Conc: 0.28 ug/ml

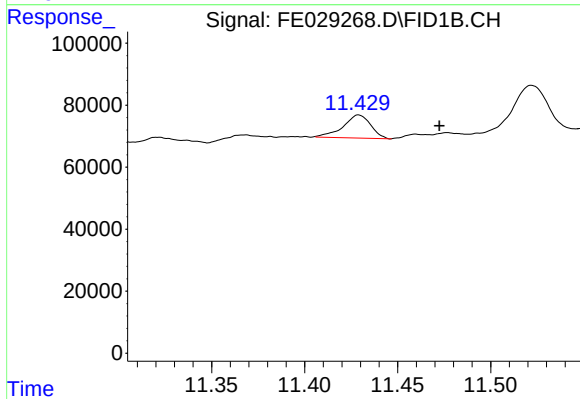


#8 N-OCTADECANE

R.T.: 11.429 min
Delta R.T.: -0.043 min
Response: 76776
Conc: 0.41 ug/ml

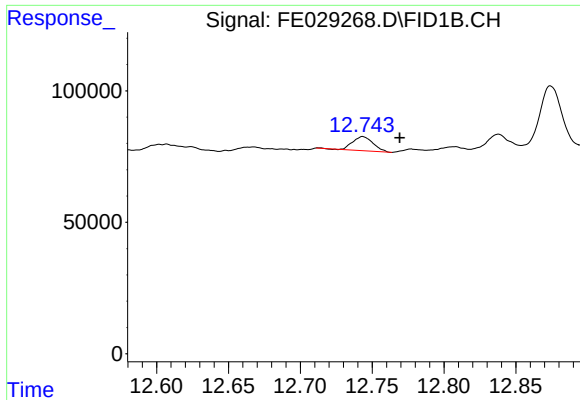


#9 N-EICOSANE

R.T.: 12.744 min
Delta R.T.: -0.026 min
Response: 52501
Conc: 0.28 ug/ml

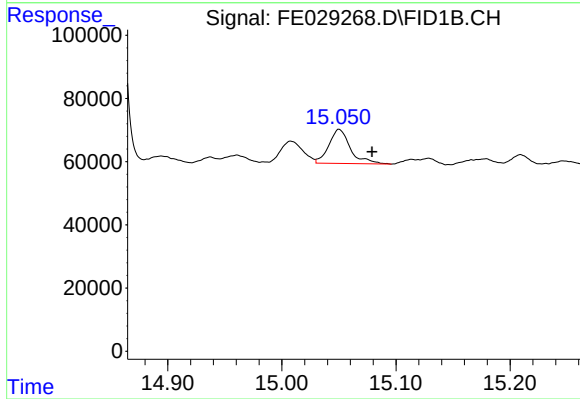


#10 N-TETRACOSANE

R.T.: 15.050 min
Delta R.T.: -0.029 min
Response: 141053
Conc: 0.78 ug/ml

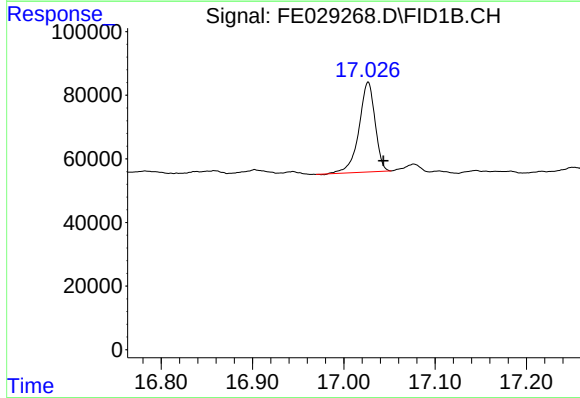


#11 N-OCTACOSANE

R.T.: 17.027 min
Delta R.T.: -0.017 min
Response: 344508
Conc: 2.12 ug/ml

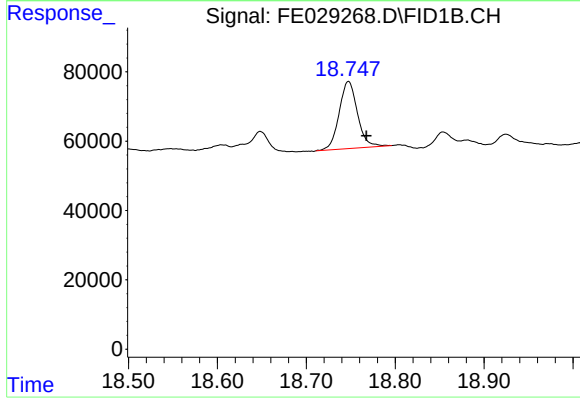

#12 N-DOTRIACONTANE

R.T.: 18.747 min
Delta R.T.: -0.020 min
Response: 276589
Conc: 1.82 ug/ml

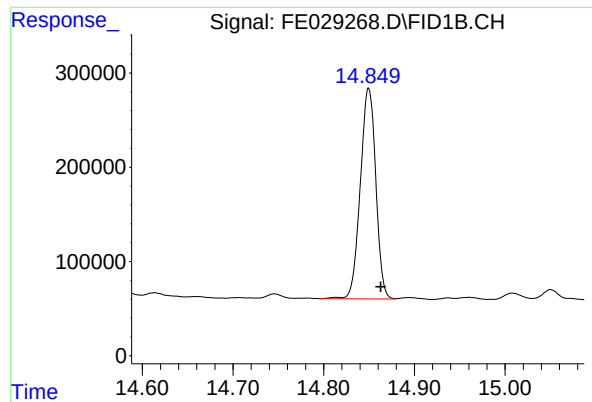

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.850 min
Delta R.T.: -0.013 min
Response: 2655379
Conc: 14.39 ug/ml