

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112020\
 Data File : FE033144.D
 Signal(s) : FID1B.CH
 Acq On : 20 Nov 2020 11:17
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 20 22:38:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE110220.M
 Quant Title :
 QLast Update : Tue Nov 03 00:53:10 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.385	8151779	24.194 ug/ml
12)	N-OCTACOSANE	16.788	8400756	24.140 ug/ml
13)	N-TRIACONTANE	17.673	354600	1.045 ug/ml
14)	N-DOTRIACONTANE	18.504	572656	1.843 ug/ml
15)	N-TETRATRIACONTANE	19.286	651330	2.514 ug/ml
16)	N-HEXATRIACONTANE	20.028	1217811	5.896 ug/ml
17)	N-OCTATRIACONTANE	20.762	1971785	11.312 ug/ml
18)	N-TETRACONTANE	21.664	2284434	13.940 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112020\
Data File : FE033144.D
Signal(s) : FID1B.CH
Acq On : 20 Nov 2020 11:17
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 20 22:38:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE110220.M
Quant Title :
QLast Update : Tue Nov 03 00:53:10 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

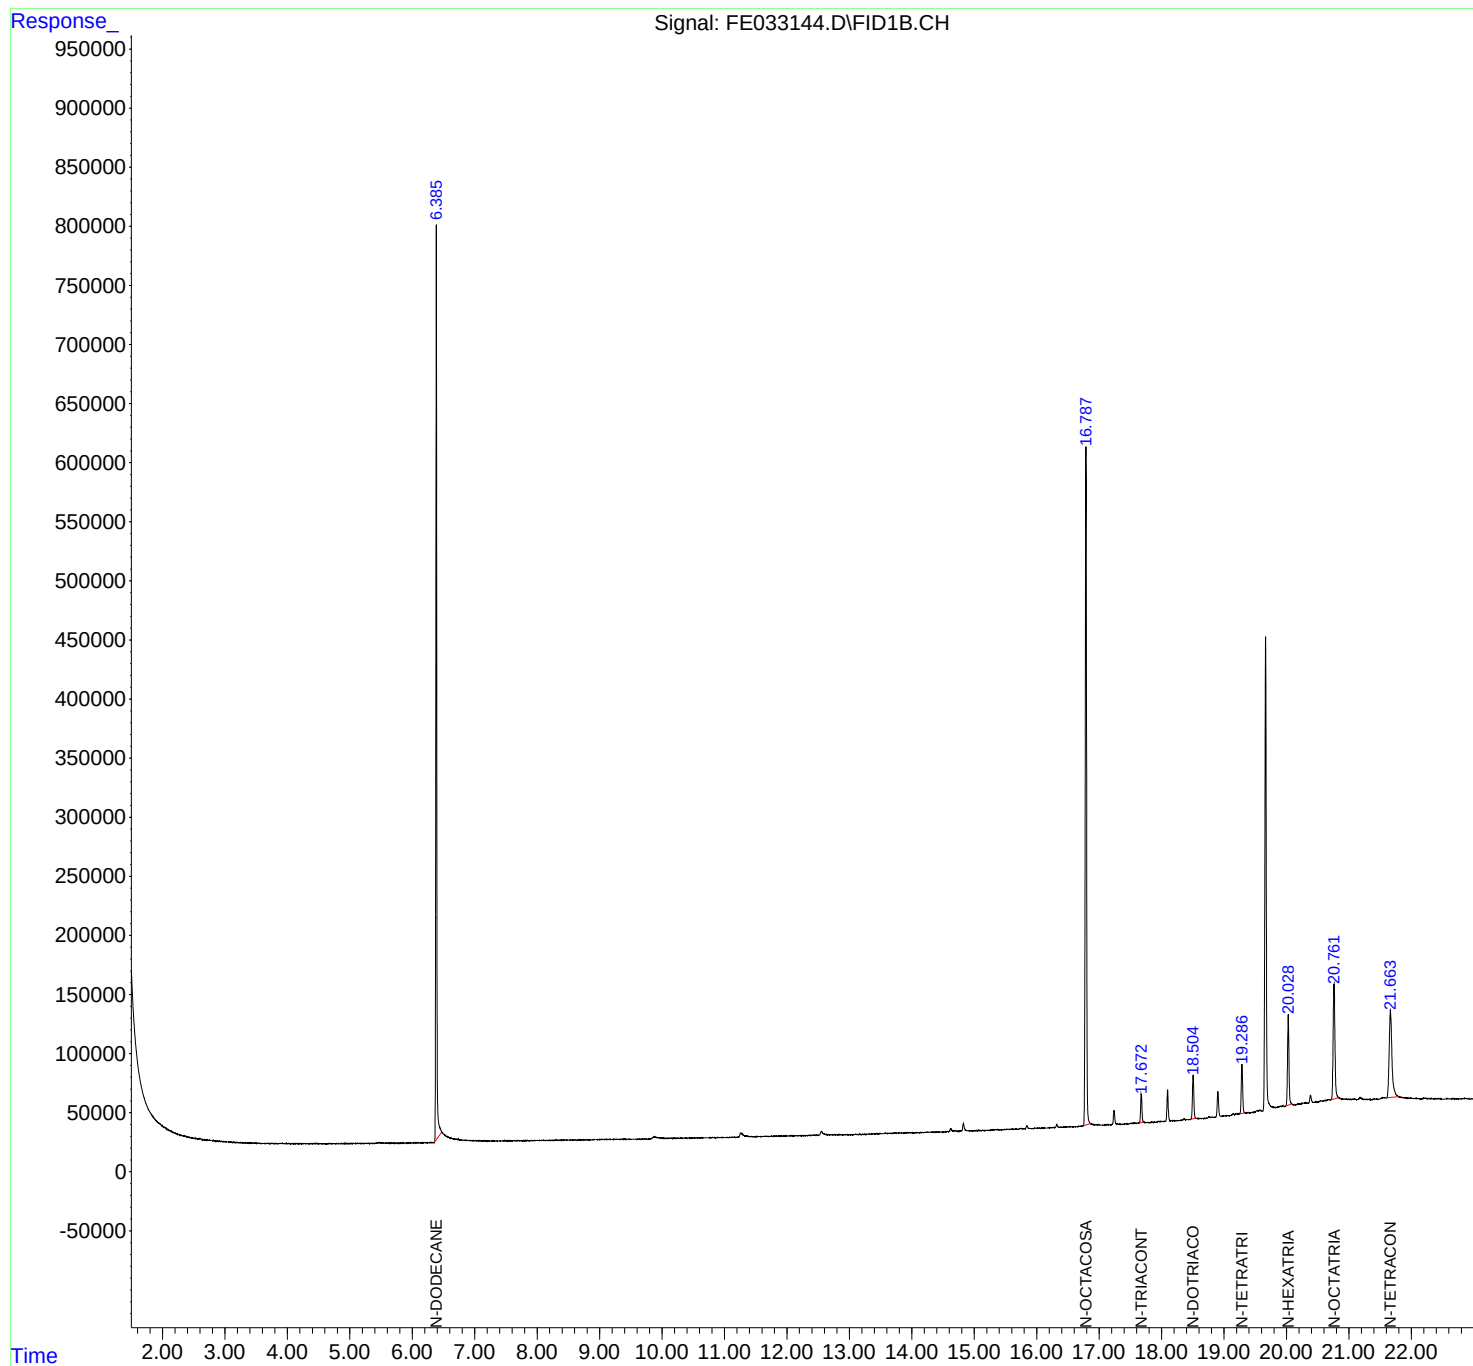


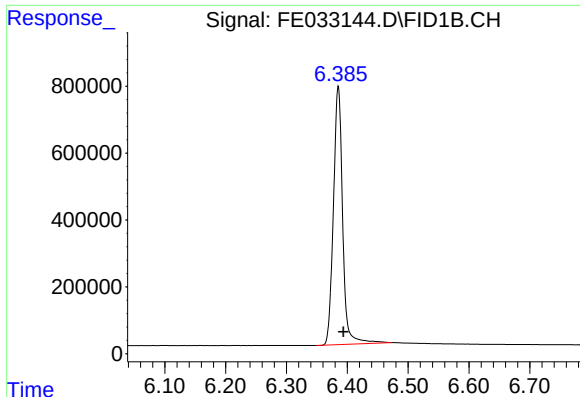

#3 N-DODECANE


R.T.: 6.385 min
Delta R.T.: -0.009 min
Response: 8151779
Conc: 24.19 ug/ml

Instrument :
FID_E
ClientSampleId :

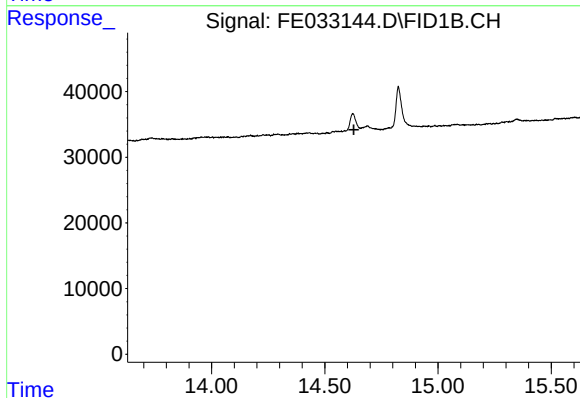


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.628 min
Response: 0
Conc: N.D.

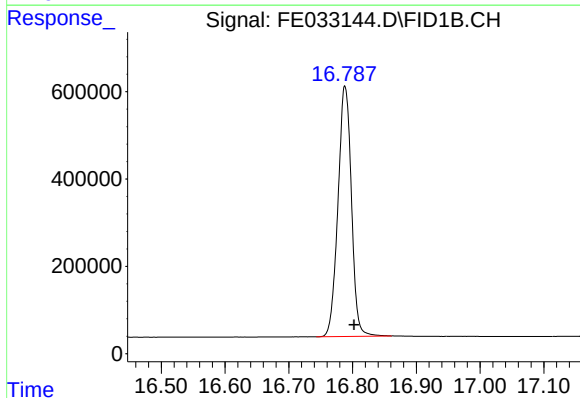


#12 N-OCTACOSANE

R.T.: 16.788 min
Delta R.T.: -0.014 min
Response: 8400756
Conc: 24.14 ug/ml

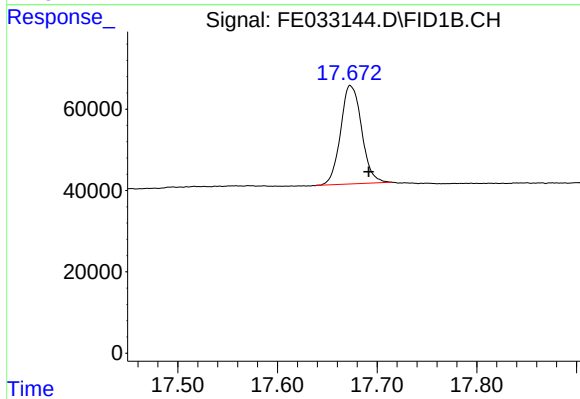

#13 N-TRIACONTANE


R.T.: 17.673 min
Delta R.T.: -0.018 min
Response: 354600
Conc: 1.05 ug/ml

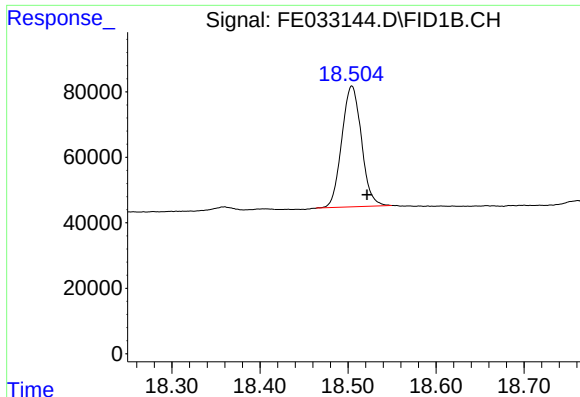

#14 N-DOTRIACONTANE


R.T.: 18.504 min
Delta R.T.: -0.017 min
Response: 572656
Conc: 1.84 ug/ml

Instrument :
FID_E
ClientSampleId :

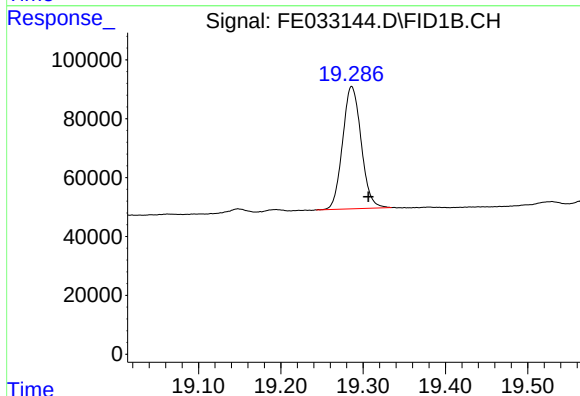


#15 N-TETRATRIACONTANE

R.T.: 19.286 min
Delta R.T.: -0.020 min
Response: 651330
Conc: 2.51 ug/ml

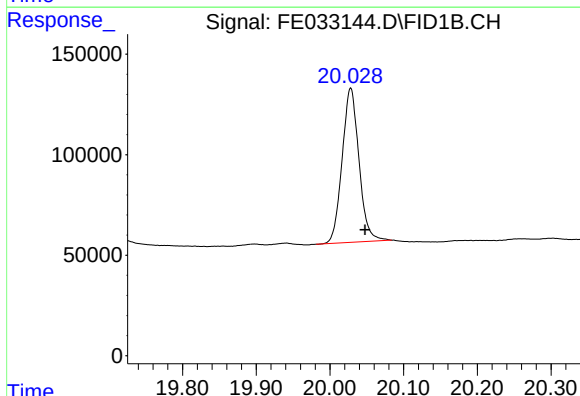


#16 N-HEXATRIACONTANE

R.T.: 20.028 min
Delta R.T.: -0.020 min
Response: 1217811
Conc: 5.90 ug/ml

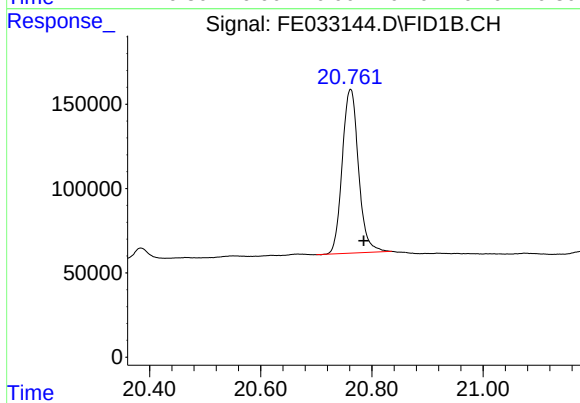

#17 N-OCTATRIACONTANE

R.T.: 20.762 min
Delta R.T.: -0.024 min
Response: 1971785
Conc: 11.31 ug/ml

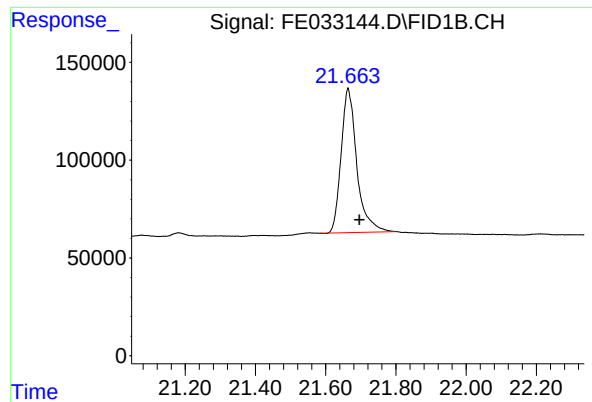

#18 N-TETRACONTANE

R.T.: 21.664 min
Delta R.T.: -0.033 min
Response: 2284434
Conc: 13.94 ug/ml

Instrument :
FID_E
ClientSampleId :