

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112025AR\
Data File : FF016750.D
Signal(s) : FID2B.ch
Acq On : 20 Nov 2025 09:37
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Nov 20 23:06:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aromatic EPH 102925.M
Quant Title : GC Extractables
QLast Update : Wed Oct 29 18:27:43 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

19) T	Indeno[1,2,3-cd]pyren...	18.545	60386	0.702 ug/ml
20) T	Dibenz[a,h]anthracene...	18.545	60386	0.459 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF112025AR\
Data File : FF016750.D
Signal(s) : FID2B.ch
Acq On : 20 Nov 2025 09:37
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Nov 20 23:06:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\Aromatic EPH 102925.M
Quant Title : GC Extractables
QLast Update : Wed Oct 29 18:27:43 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18µm

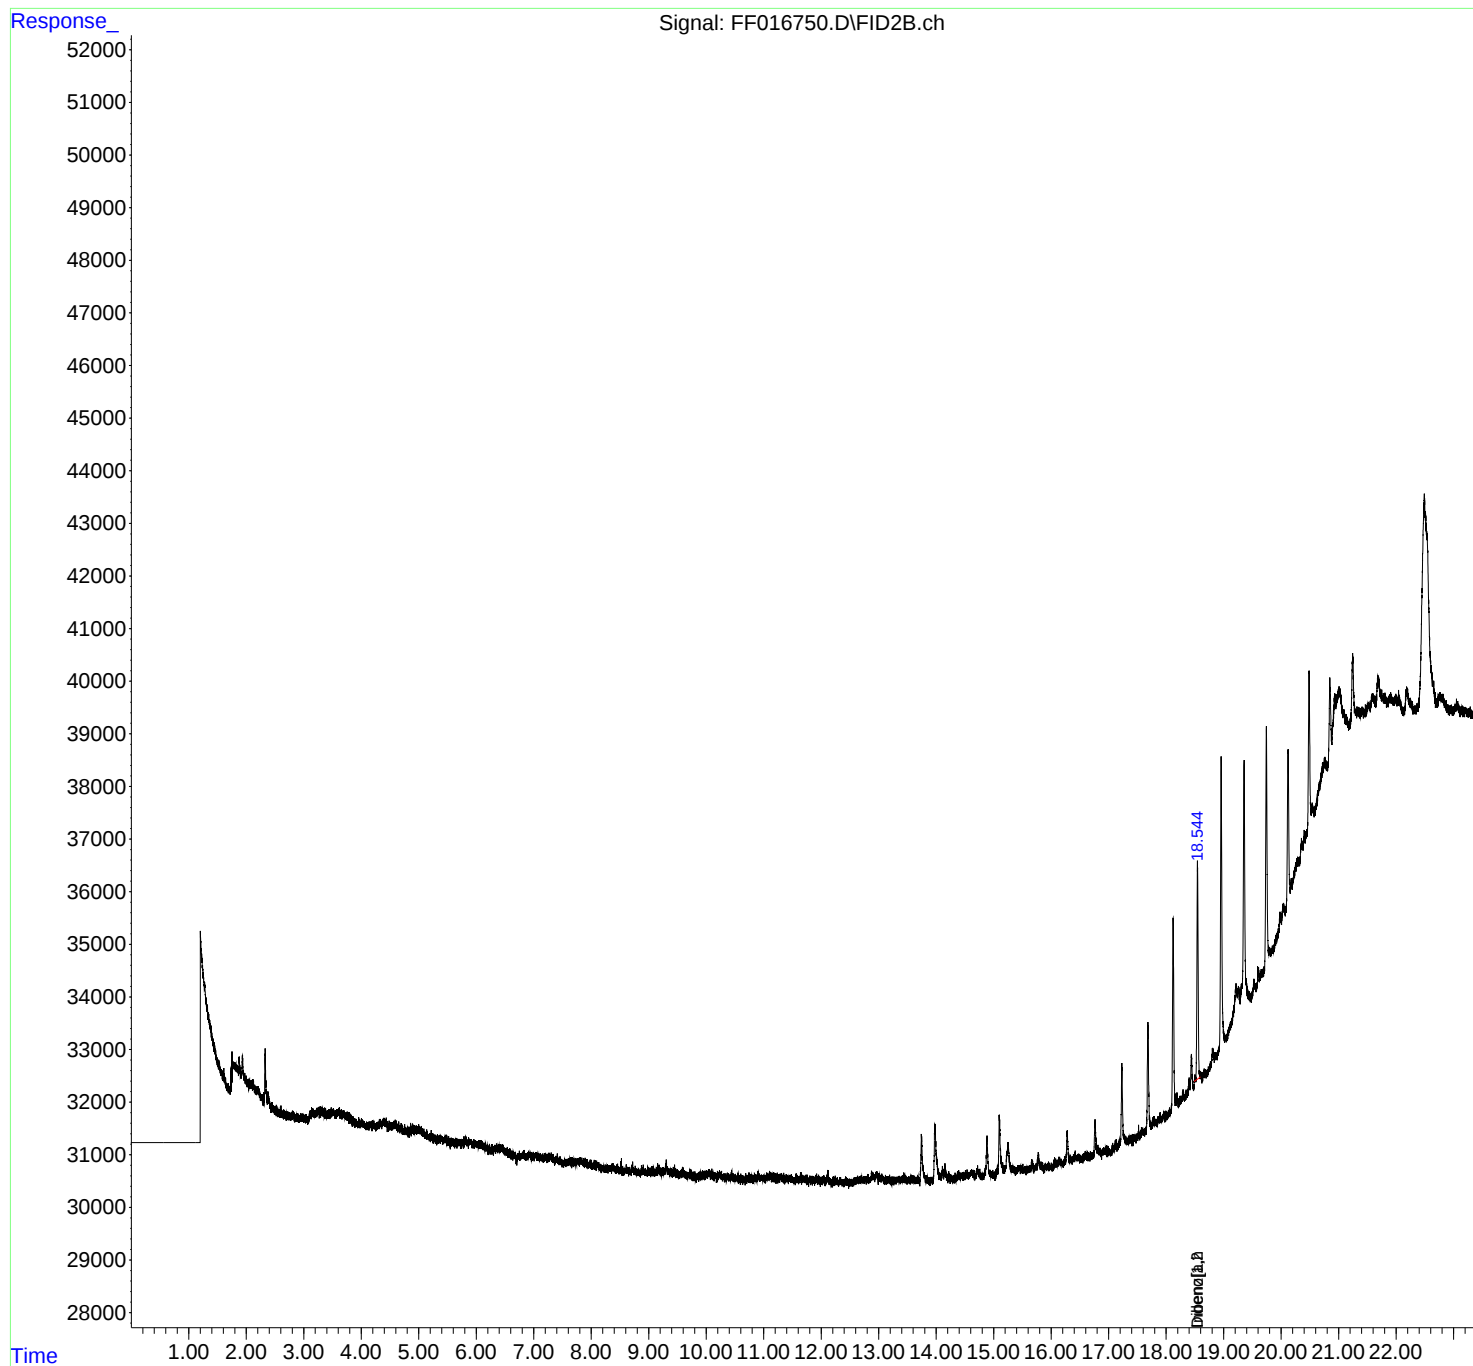


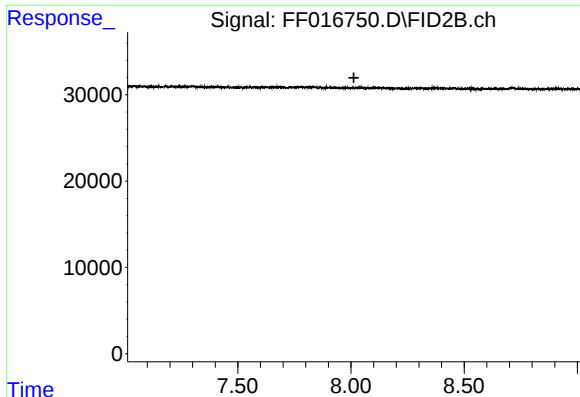

#4 2-Bromonaphthalene (SURRE)


R.T.: 0.000 min
Exp R.T. : 8.013 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
MECL2

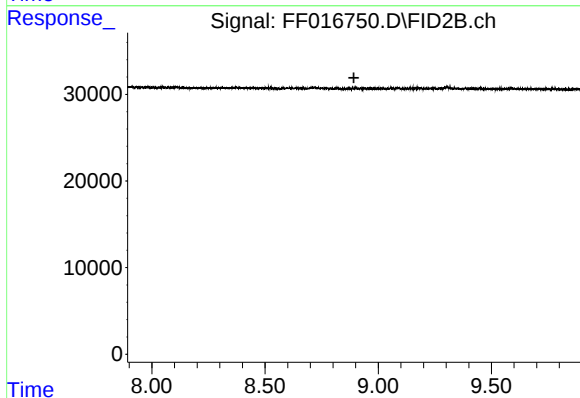


#6 2-Fluorobiphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 8.892 min
Response: 0
Conc: N.D.

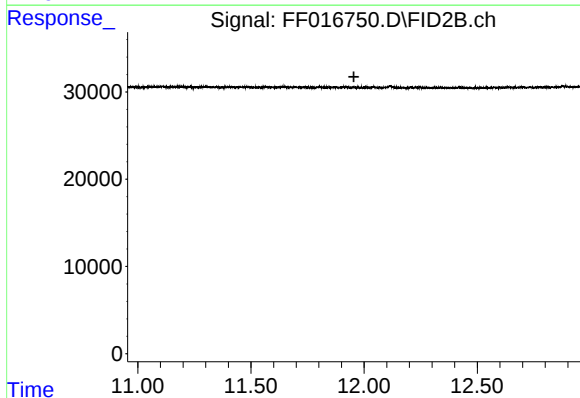


#11 ortho-Terphenyl (SURRE)

R.T.: 0.000 min
Exp R.T. : 11.955 min
Response: 0
Conc: N.D.

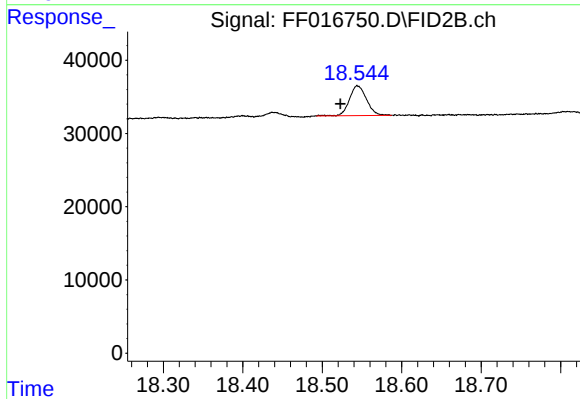

#19 Indeno[1,2,3-cd]pyrene (C35.01)

R.T.: 18.545 min
Delta R.T.: 0.022 min
Response: 60386
Conc: 0.70 ug/ml

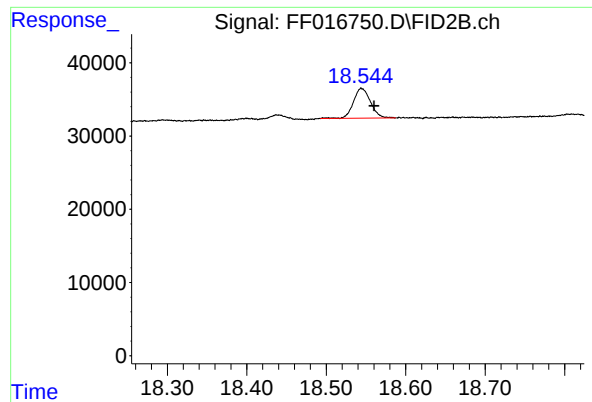

#20 Dibenz[a,h]anthracene (C30.36)

R.T.: 18.545 min
Delta R.T.: -0.016 min
Response: 60386
Conc: 0.46 ug/ml

Instrument :
FID_E
ClientSampleId :
MECL2