

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112025AL\
 Data File : FG016958.D
 Signal(s) : FID1A.ch
 Acq On : 20 Nov 2025 13:13
 Operator : YP\AJ
 Sample : Q3586-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 SED-3

Integration File: autoint1.e
 Quant Time: Nov 20 23:49:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 102925.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 29 16:21:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.483	8310854	69.008 ug/ml
Spiked Amount 50.000		Recovery =	138.02%
Target Compounds			
14) T n-Tetracosane (C24)	15.349	77741	0.529 ug/ml
15) T n-Hexacosane (C26)	16.377	98698	0.673 ug/ml
16) T n-Octacosane (C28)	17.333	113771	0.773 ug/ml
17) T n-Tricontane (C30)	18.226	137888	0.911 ug/ml
18) T n-Dotriacontane (C32)	19.064	140092	0.950 ug/ml
19) T n-Tetratriacontane (C34)	19.853	88724	0.688 ug/ml
20) T n-Hexatriacontane (C36)	20.599	52294	0.505 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_G\Data\FG112025AL\
Data File : FG016958.D
Signal(s) : FID1A.ch
Acq On : 20 Nov 2025 13:13
Operator : YP\AJ
Sample : Q3586-03
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
SED-3

Integration File: autoint1.e
Quant Time: Nov 20 23:49:48 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_G\Method\Aliphatic EPH 102925.M
Quant Title : GC Extractables
QLast Update : Wed Oct 29 16:21:47 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

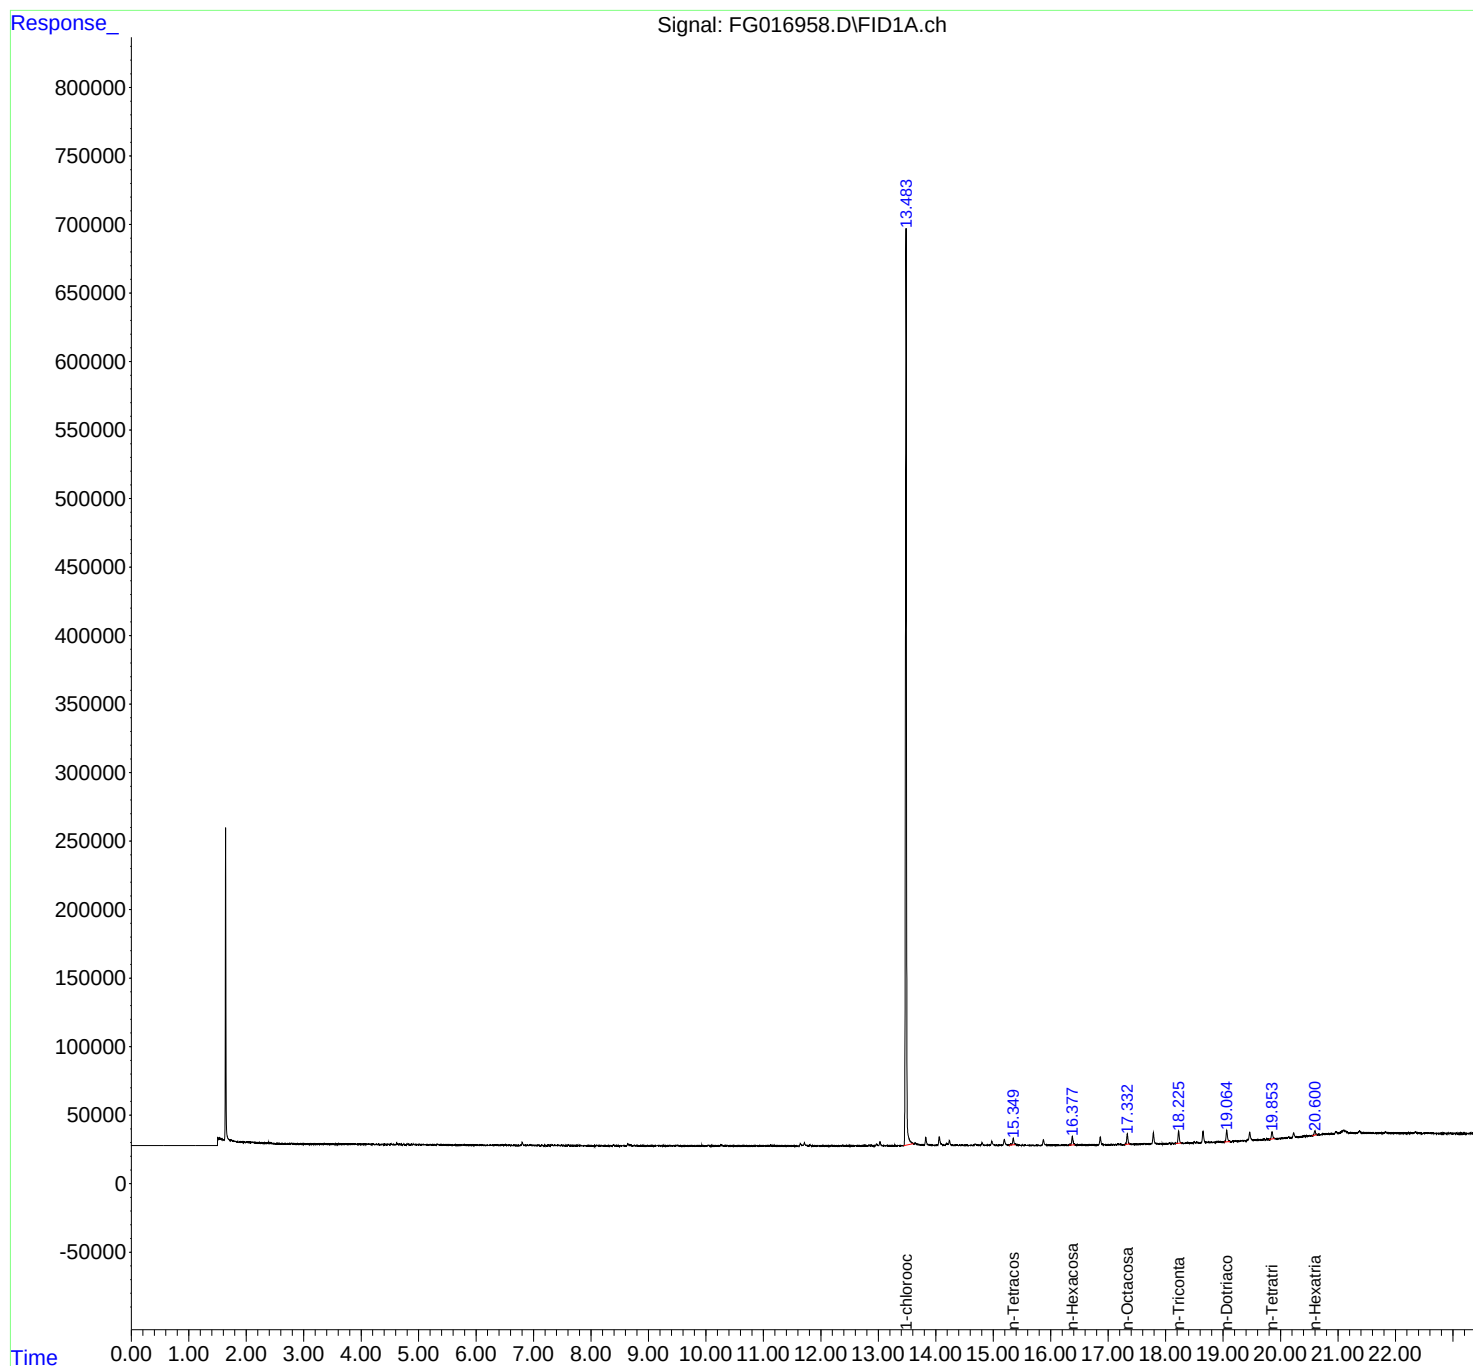


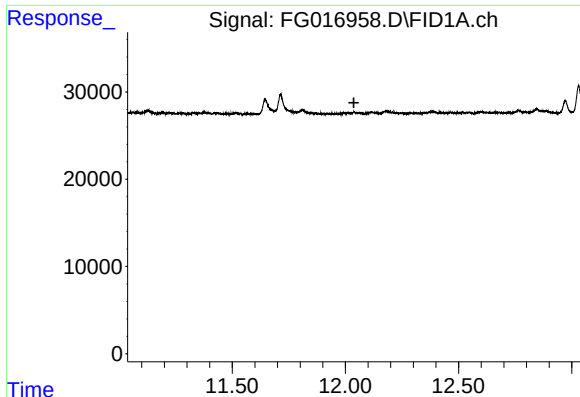

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 12.038 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
SED-3

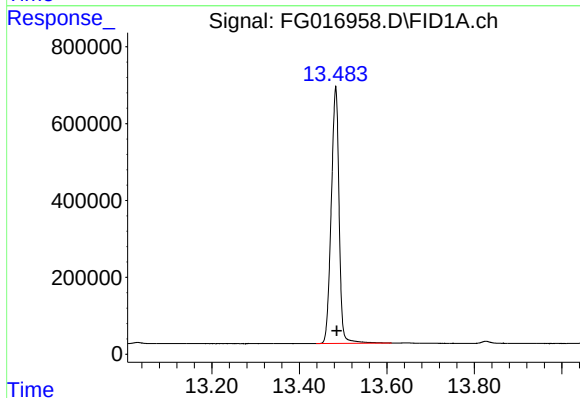


#12 1-chlorooctadecane (SURR)

R.T.: 13.483 min
Delta R.T.: -0.002 min
Response: 8310854
Conc: 69.01 ug/ml

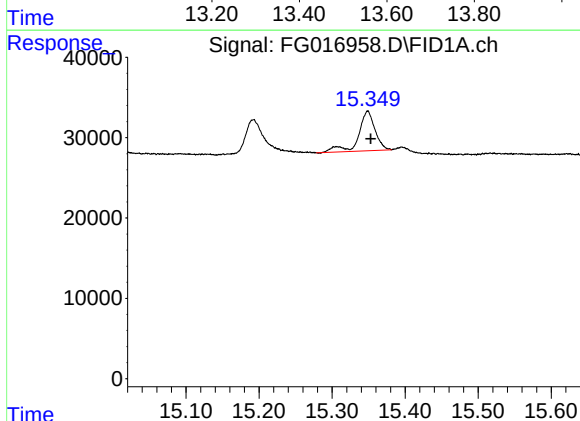


#14 n-Tetracosane (C24)

R.T.: 15.349 min
Delta R.T.: -0.004 min
Response: 77741
Conc: 0.53 ug/ml

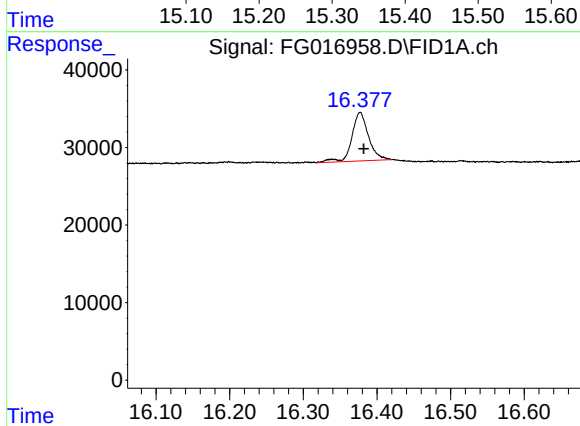

#15 n-Hexacosane (C26)


R.T.: 16.377 min
Delta R.T.: -0.005 min
Response: 98698
Conc: 0.67 ug/ml

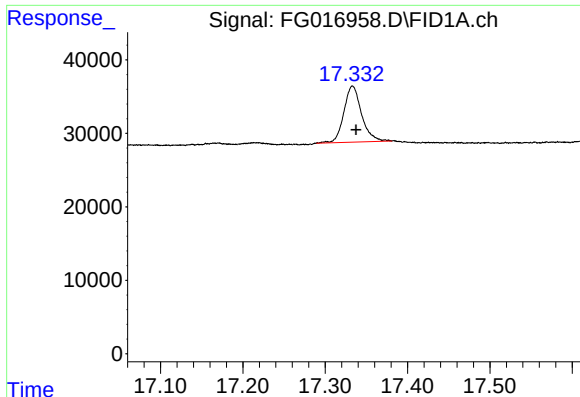

#16 n-Octacosane (C28)


R.T.: 17.333 min
Delta R.T.: -0.004 min
Response: 113771
Conc: 0.77 ug/ml

Instrument :
FID_E
ClientSampleId :
SED-3

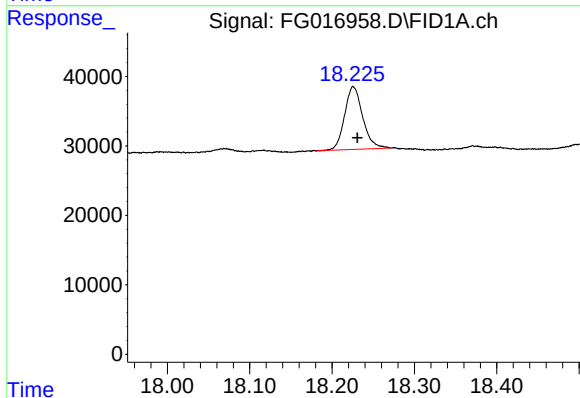


#17 n-Tricontane (C30)

R.T.: 18.226 min
Delta R.T.: -0.005 min
Response: 137888
Conc: 0.91 ug/ml

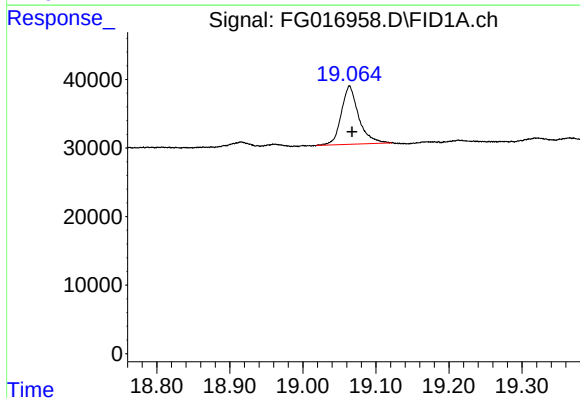


#18 n-Dotriacontane (C32)

R.T.: 19.064 min
Delta R.T.: -0.003 min
Response: 140092
Conc: 0.95 ug/ml

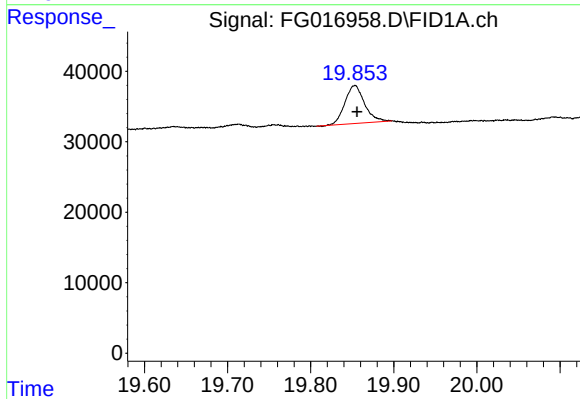

#19 n-Tetratriacontane (C34)

R.T.: 19.853 min
Delta R.T.: -0.003 min
Response: 88724
Conc: 0.69 ug/ml

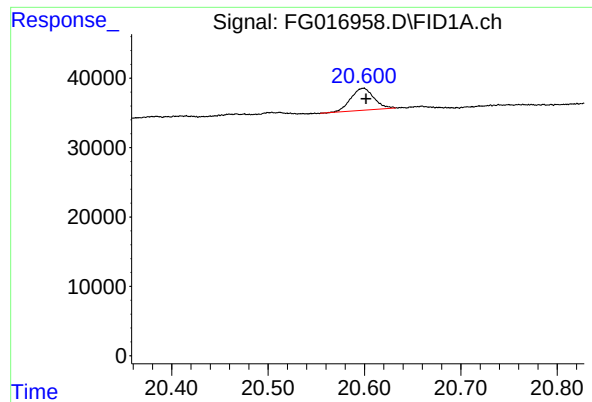

#20 n-Hexatriacontane (C36)

R.T.: 20.599 min
Delta R.T.: -0.003 min
Response: 52294
Conc: 0.51 ug/ml

Instrument :
FID_E
ClientSampleId :
SED-3