

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112120\
 Data File : FE033154.D
 Signal(s) : FID1B.CH
 Acq On : 21 Nov 2020 10:00
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 23 00:36:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE110220.M
 Quant Title :
 QLast Update : Tue Nov 03 00:53:10 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds			
3) N-DODECANE	6.385	8806990	26.139 ug/ml
12) N-OCTACOSANE	16.790	9254678	26.594 ug/ml
13) N-TRIACONTANE	17.673	639995	1.886 ug/ml
14) N-DOTRIACONTANE	18.503	950826	3.061 ug/ml
15) N-TETRATRIACONTANE	19.285	1005175	3.880 ug/ml
16) N-HEXATRIACONTANE	20.027	1653277	8.004 ug/ml
17) N-OCTATRIACONTANE	20.759	2407713	13.813 ug/ml
18) N-TETRACONTANE	21.661	2545942	15.536 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112120\
Data File : FE033154.D
Signal(s) : FID1B.CH
Acq On : 21 Nov 2020 10:00
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 23 00:36:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE110220.M
Quant Title :
QLast Update : Tue Nov 03 00:53:10 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

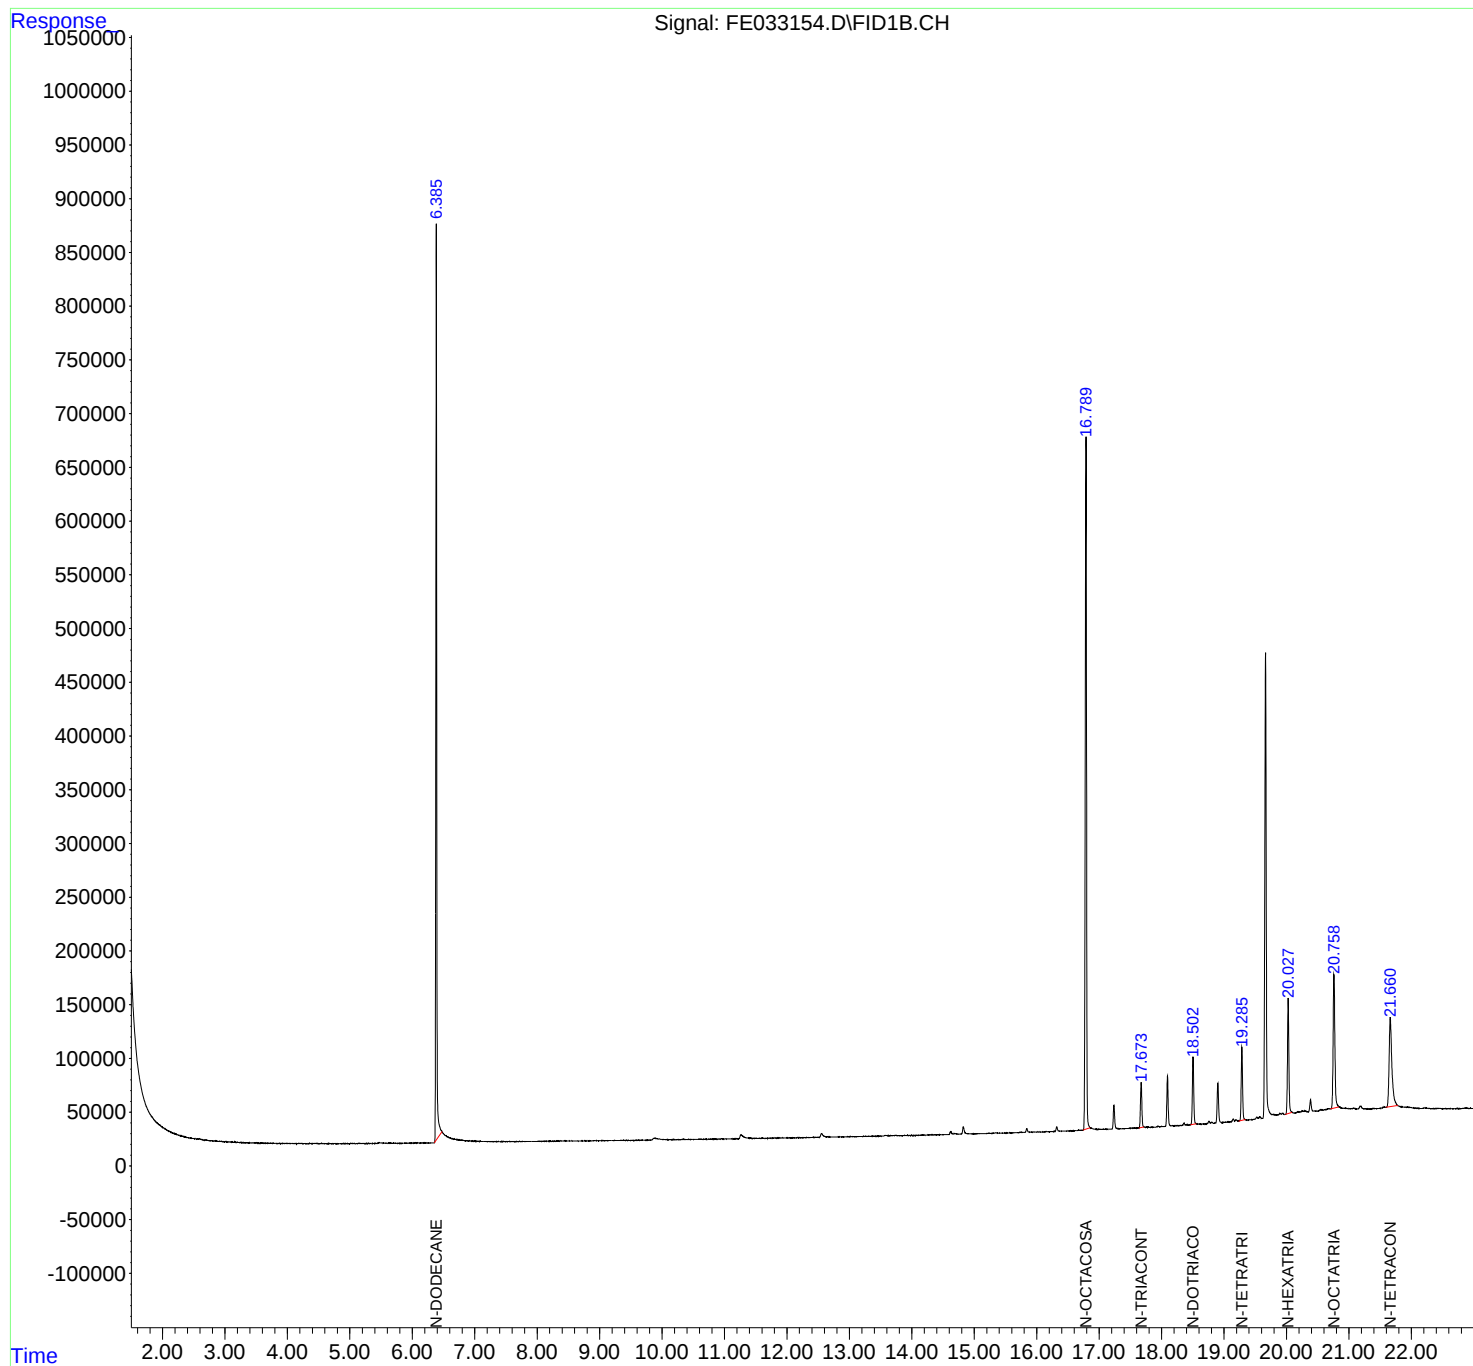


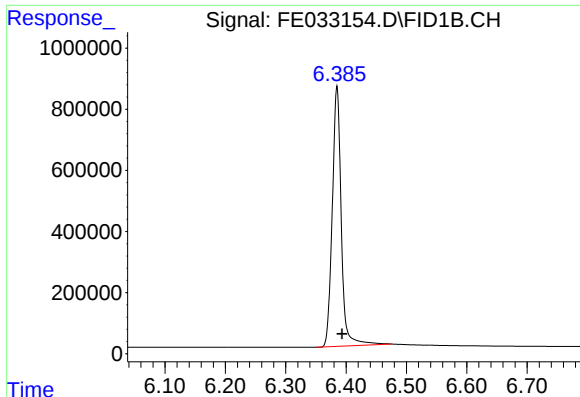

#3 N-DODECANE


R.T.: 6.385 min
Delta R.T.: -0.009 min
Response: 8806990
Conc: 26.14 ug/ml

Instrument :
FID_E
ClientSampleId :

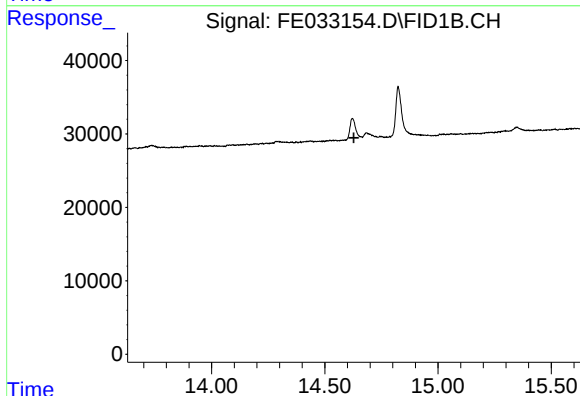


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.628 min
Response: 0
Conc: N.D.

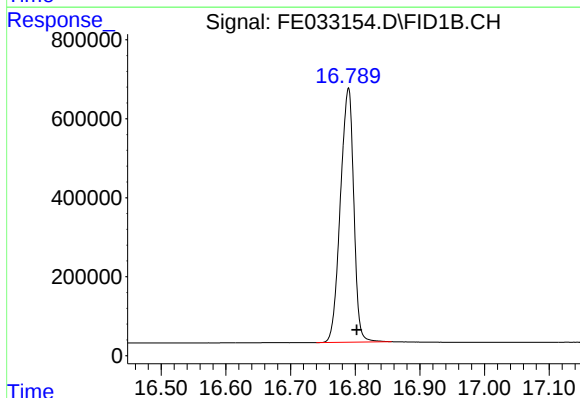


#12 N-OCTACOSANE

R.T.: 16.790 min
Delta R.T.: -0.012 min
Response: 9254678
Conc: 26.59 ug/ml

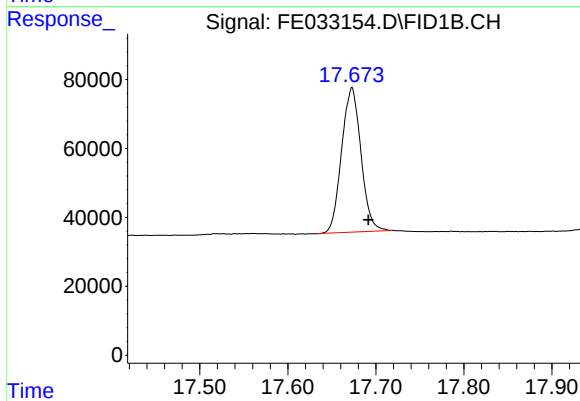

#13 N-TRIACONTANE


R.T.: 17.673 min
Delta R.T.: -0.018 min
Response: 639995
Conc: 1.89 ug/ml

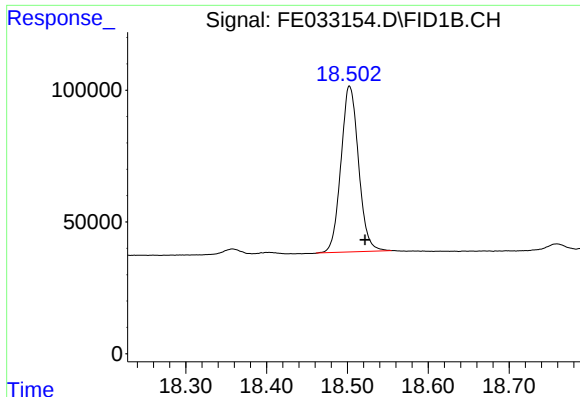

#14 N-DOTRIACONTANE


R.T.: 18.503 min
Delta R.T.: -0.019 min
Response: 950826
Conc: 3.06 ug/ml

Instrument :
FID_E
ClientSampleId :

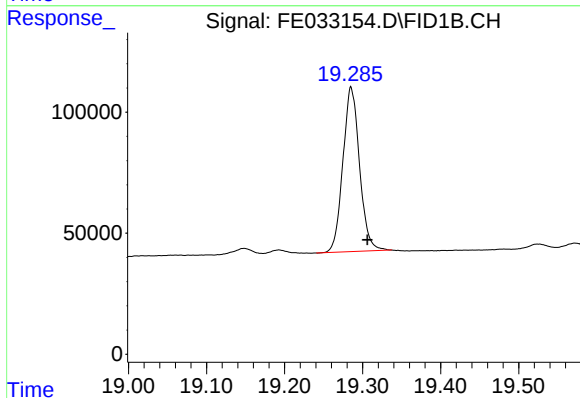


#15 N-TETRATRIACONTANE

R.T.: 19.285 min
Delta R.T.: -0.021 min
Response: 1005175
Conc: 3.88 ug/ml

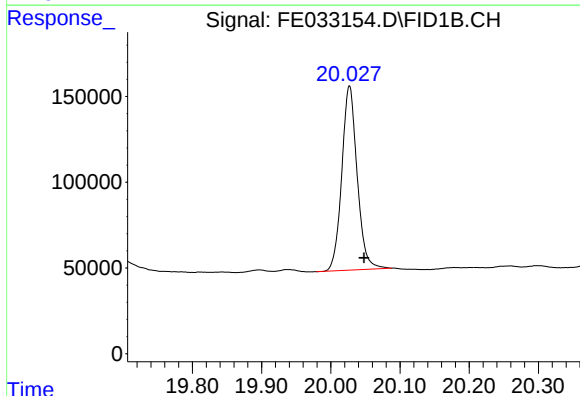


#16 N-HEXATRIACONTANE

R.T.: 20.027 min
Delta R.T.: -0.021 min
Response: 1653277
Conc: 8.00 ug/ml

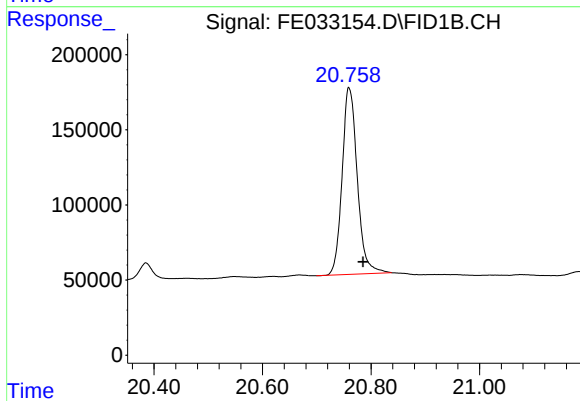

#17 N-OCTATRIACONTANE

R.T.: 20.759 min
Delta R.T.: -0.026 min
Response: 2407713
Conc: 13.81 ug/ml

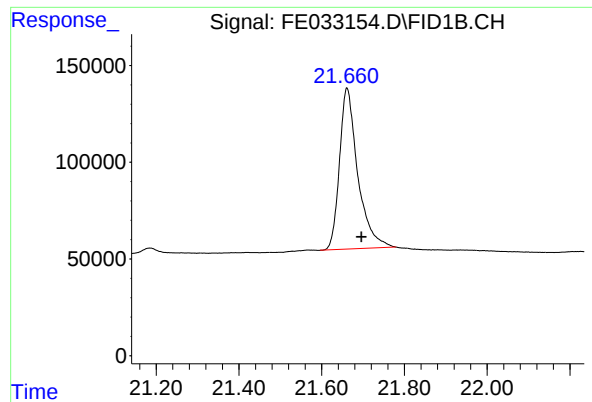

#18 N-TETRACONTANE

R.T.: 21.661 min
Delta R.T.: -0.035 min
Response: 2545942
Conc: 15.54 ug/ml

Instrument :
FID_E
ClientSampleId :