

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112120\
 Data File : FE033155.D
 Signal(s) : FID1B.CH
 Acq On : 21 Nov 2020 10:33
 Operator : DD\AJ
 Sample : PB133136BS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 PB133136BS

Integration File: autoint1.e
 Quant Time: Nov 23 00:36:59 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE110220.M
 Quant Title :
 QLast Update : Tue Nov 03 00:53:10 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.613	5894765	18.666 ug/ml
Target Compounds			
2) N-DECANE	4.377	6961980	20.553 ug/ml
3) N-DODECANE	6.384	7243123	21.497 ug/ml
4) N-TETRADECANE	8.175	7550717	22.139 ug/ml
5) N-HEXADECANE	9.773	7633982	21.873 ug/ml
6) N-OCTADECANE	11.213	7711269	21.543 ug/ml
7) N-EICOSANE	12.520	7792957	21.635 ug/ml
8) N-DOCOSANE	13.717	7667033	21.473 ug/ml
10) N-TETRACOSANE	14.818	7436852	20.750 ug/ml
11) N-HEXACOSANE	15.838	7165054	20.353 ug/ml
12) N-OCTACOSANE	16.786	7019160	20.170 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112120\
Data File : FE033155.D
Signal(s) : FID1B.CH
Acq On : 21 Nov 2020 10:33
Operator : DD\AJ
Sample : PB133136BS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB133136BS

Integration File: autoint1.e
Quant Time: Nov 23 00:36:59 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE110220.M
Quant Title :
QLast Update : Tue Nov 03 00:53:10 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

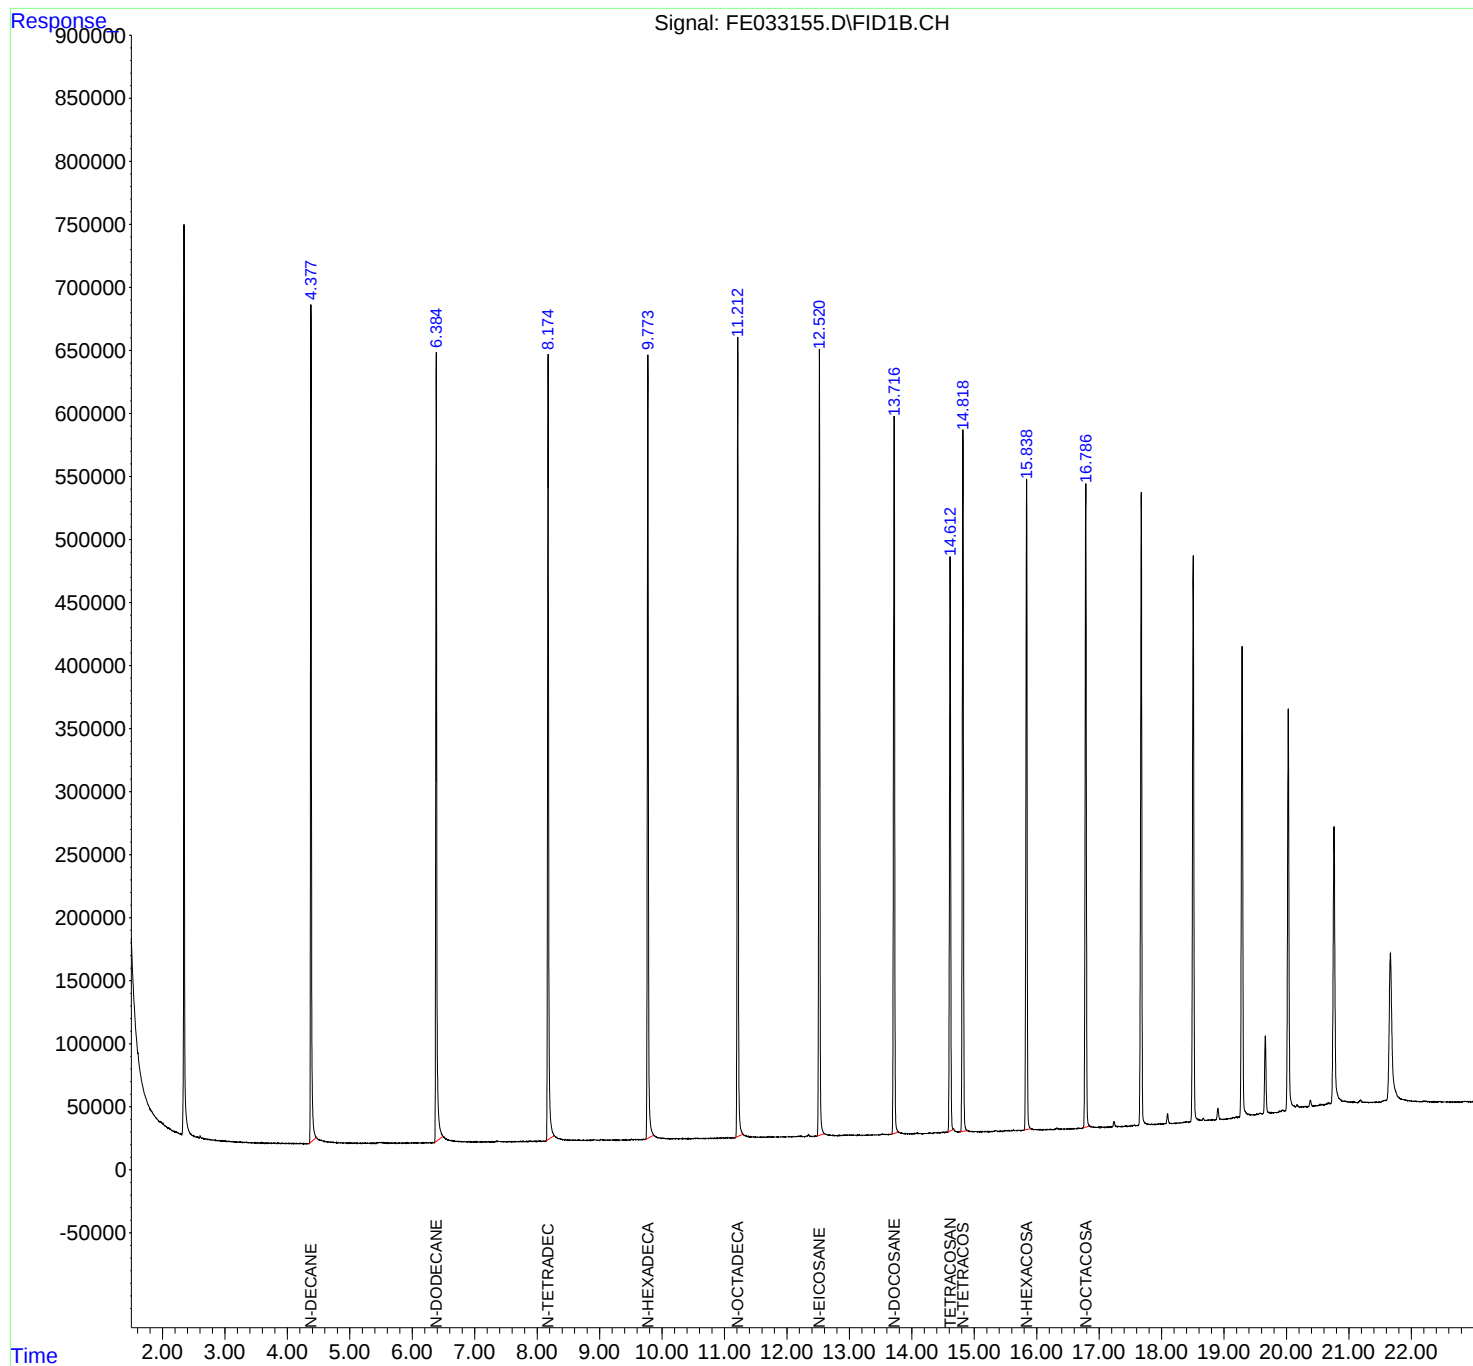


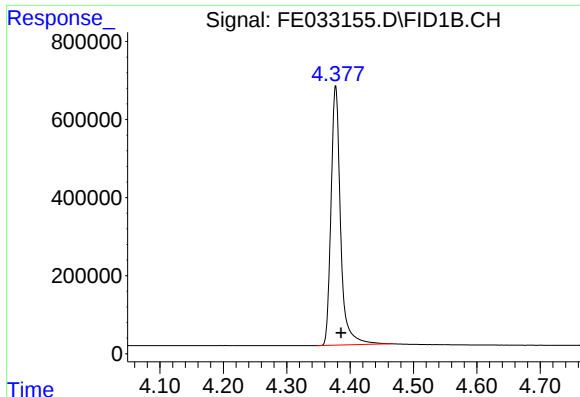

#2 N-DECANE


R.T.: 4.377 min
Delta R.T.: -0.008 min
Response: 6961980
Conc: 20.55 ug/ml

Instrument :
FID_E
ClientSampleId :
PB133136BS

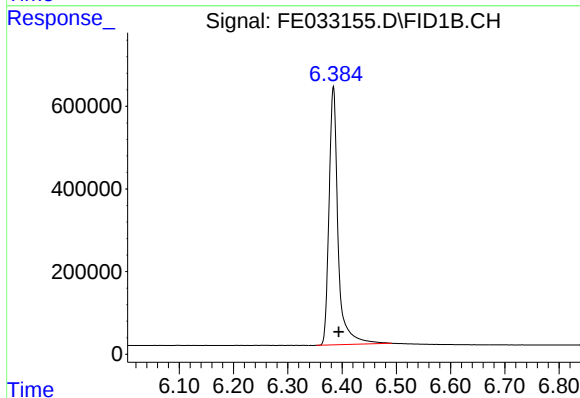


#3 N-DODECANE

R.T.: 6.384 min
Delta R.T.: -0.010 min
Response: 7243123
Conc: 21.50 ug/ml

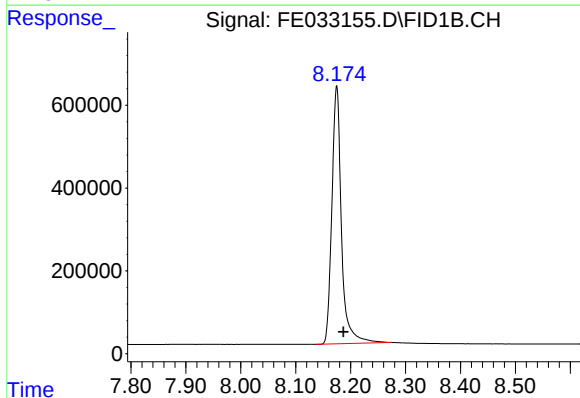


#4 N-TETRADECANE

R.T.: 8.175 min
Delta R.T.: -0.012 min
Response: 7550717
Conc: 22.14 ug/ml

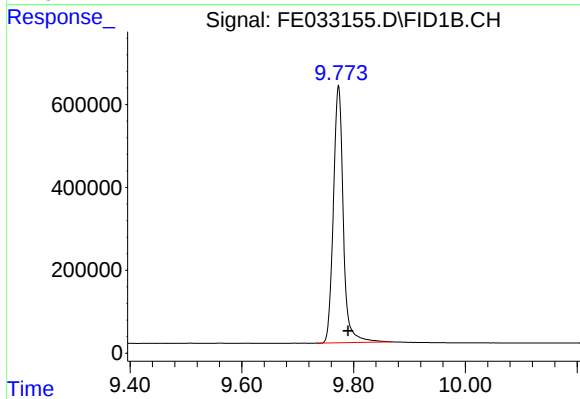

#5 N-HEXADECANE


R.T.: 9.773 min
Delta R.T.: -0.017 min
Response: 7633982
Conc: 21.87 ug/ml

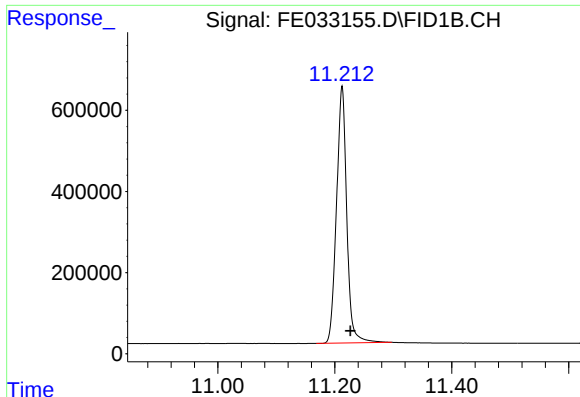

#6 N-OCTADECANE


R.T.: 11.213 min
Delta R.T.: -0.014 min
Response: 7711269
Conc: 21.54 ug/ml

Instrument :
FID_E
ClientSampleId :
PB133136BS

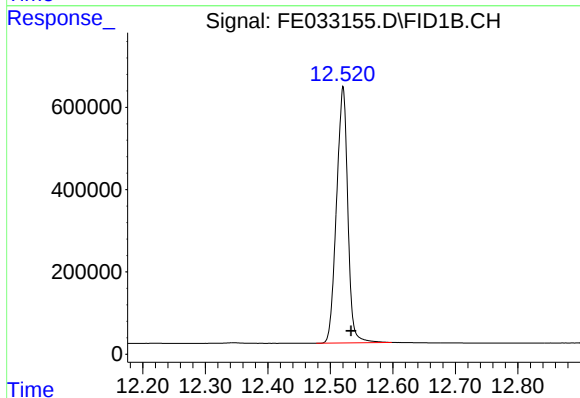


#7 N-EICOSANE

R.T.: 12.520 min
Delta R.T.: -0.013 min
Response: 7792957
Conc: 21.64 ug/ml

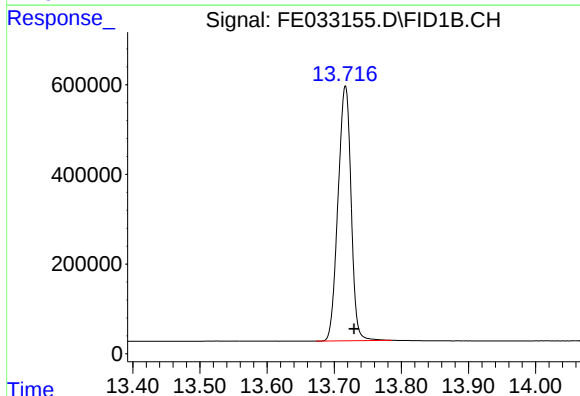


#8 N-DOCOSANE

R.T.: 13.717 min
Delta R.T.: -0.013 min
Response: 7667033
Conc: 21.47 ug/ml

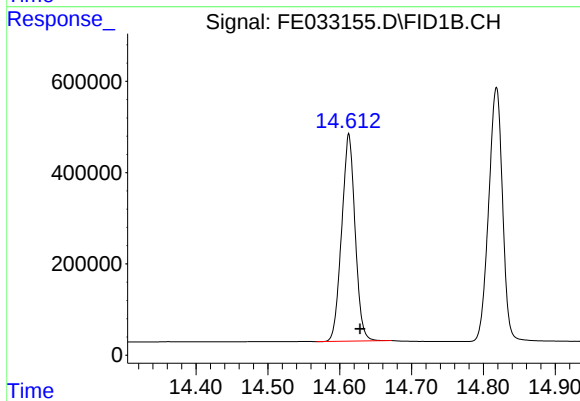

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.613 min
Delta R.T.: -0.015 min
Response: 5894765
Conc: 18.67 ug/ml

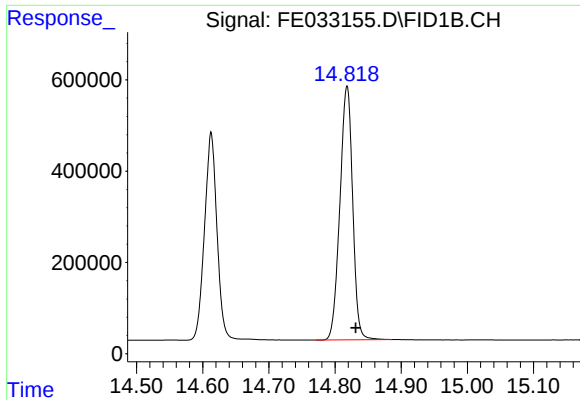

#10 N-TETRACOSANE


R.T.: 14.818 min
Delta R.T.: -0.013 min
Response: 7436852
Conc: 20.75 ug/ml

Instrument :
FID_E
ClientSampleId :
PB133136BS

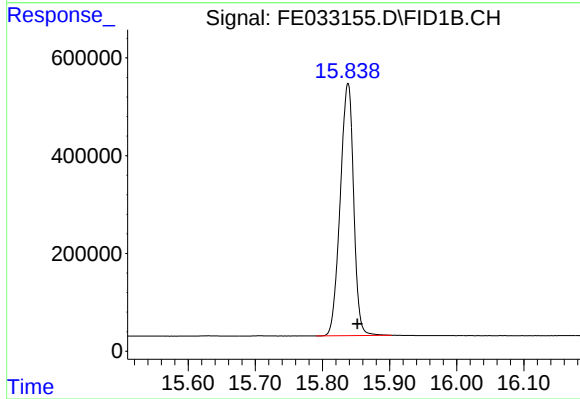

#11 N-HEXACOSANE

R.T.: 15.838 min
Delta R.T.: -0.014 min
Response: 7165054
Conc: 20.35 ug/ml

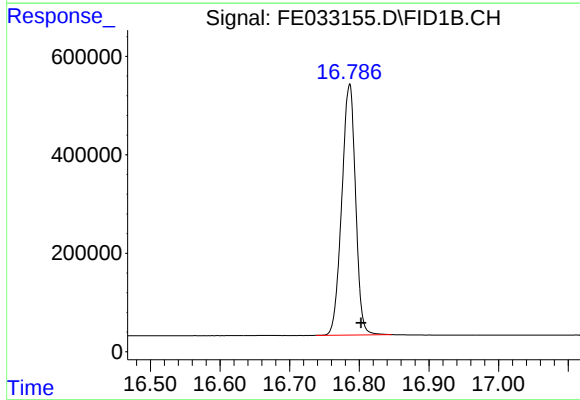

#12 N-OCTACOSANE

R.T.: 16.786 min
Delta R.T.: -0.016 min
Response: 7019160
Conc: 20.17 ug/ml