

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112219\
 Data File : FE030929.D
 Signal(s) : FID1B.CH
 Acq On : 22 Nov 2019 11:49
 Operator : DD\AJ
 Sample : RT MARKER
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Nov 22 21:07:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
 Quant Title :
 QLast Update : Thu Oct 31 08:47:02 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
3) N-DODECANE	6.403	12841676	33.750 ug/ml
11) N-HEXACOSANE	15.883	195200	0.560 ug/ml
12) N-OCTACOSANE	16.847	12106876	35.511 ug/ml
13) N-TRIACONTANE	17.726	997631	3.004 ug/ml
14) N-DOTRIACONTANE	18.560	1052050	3.295 ug/ml
15) N-TETRATRIACONTANE	19.345	704055	2.312 ug/ml
16) N-HEXATRIACONTANE	20.086	1226687	4.468 ug/ml
17) N-OCTATRIACONTANE	20.822	887150	3.509 ug/ml
18) N-TETRACONTANE	21.727	788367	3.001 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112219\
Data File : FE030929.D
Signal(s) : FID1B.CH
Acq On : 22 Nov 2019 11:49
Operator : DD\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Nov 22 21:07:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE103019.M
Quant Title :
QLast Update : Thu Oct 31 08:47:02 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

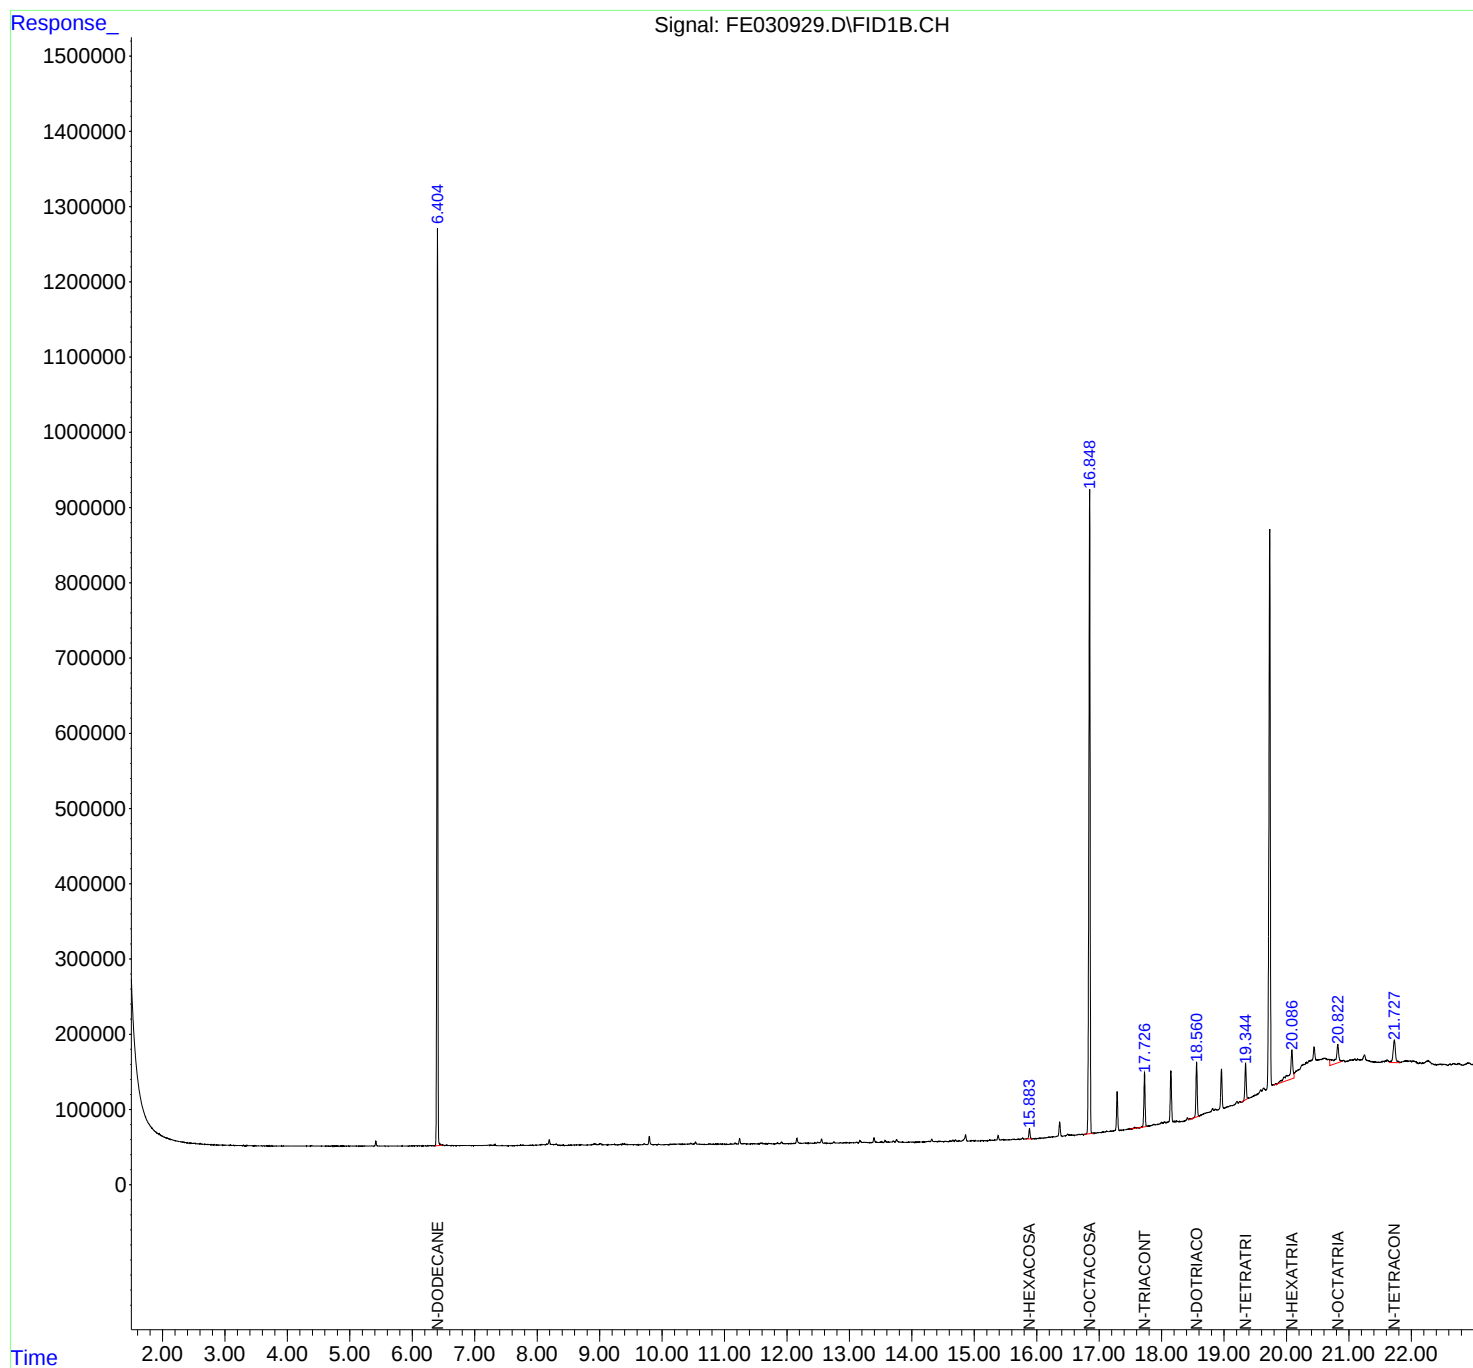

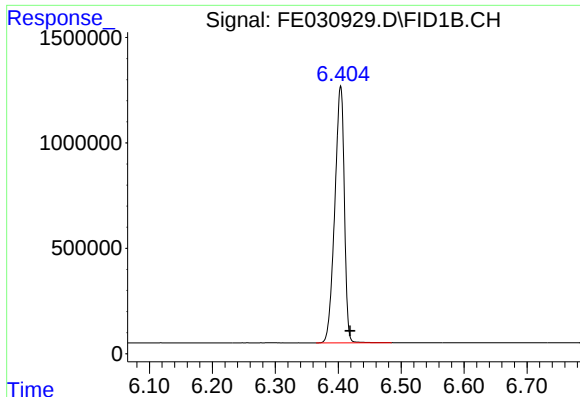


#3 N-DODECANE

R.T.: 6.403 min
Delta R.T.: -0.016 min
Response: 12841676
Conc: 33.75 ug/ml

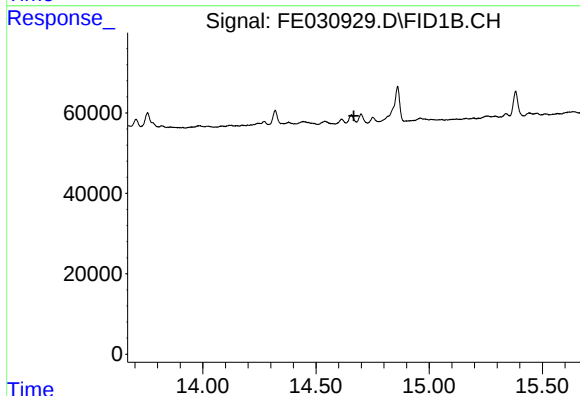


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.667 min
Response: 0
Conc: N.D.

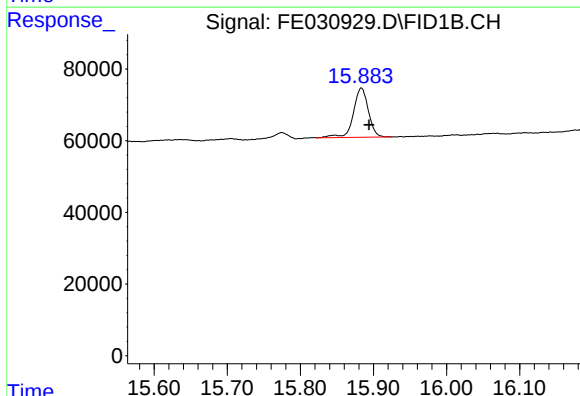


#11 N-HEXACOSANE

R.T.: 15.883 min
Delta R.T.: -0.011 min
Response: 195200
Conc: 0.56 ug/ml

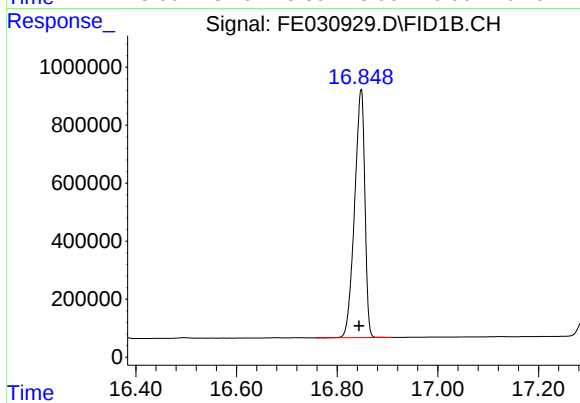


#12 N-OCTACOSANE

R.T.: 16.847 min
Delta R.T.: 0.004 min
Response: 12106876
Conc: 35.51 ug/ml

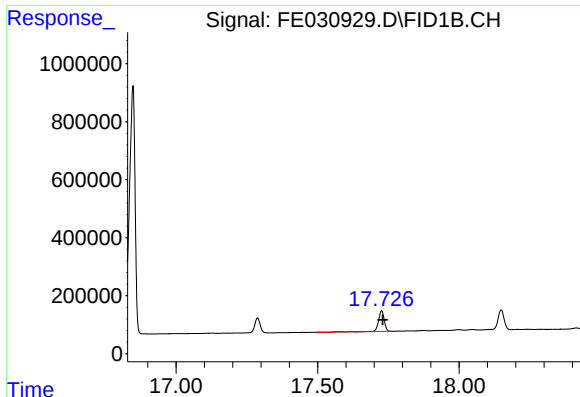


#13 N-TRIACONTANE

R.T.: 17.726 min
Delta R.T.: -0.004 min
Response: 997631
Conc: 3.00 ug/ml

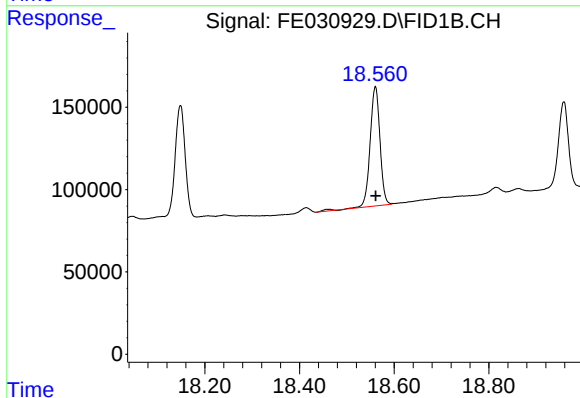


#14 N-DOTRIACONTANE

R.T.: 18.560 min
Delta R.T.: -0.001 min
Response: 1052050
Conc: 3.30 ug/ml

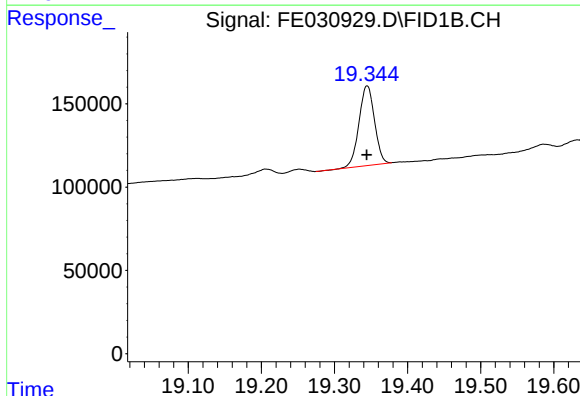


#15 N-TETRATRIACONTANE

R.T.: 19.345 min
Delta R.T.: 0.000 min
Response: 704055
Conc: 2.31 ug/ml

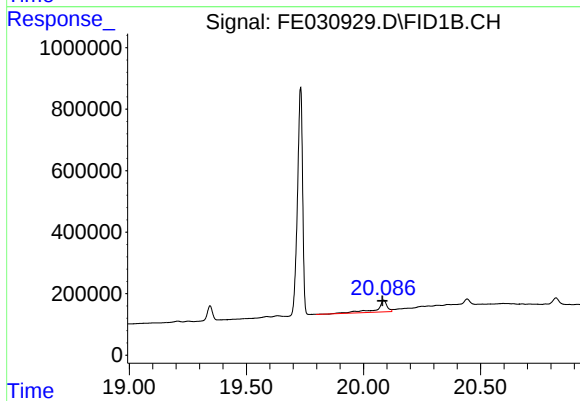


#16 N-HEXATRIACONTANE

R.T.: 20.086 min
Delta R.T.: 0.005 min
Response: 1226687
Conc: 4.47 ug/ml

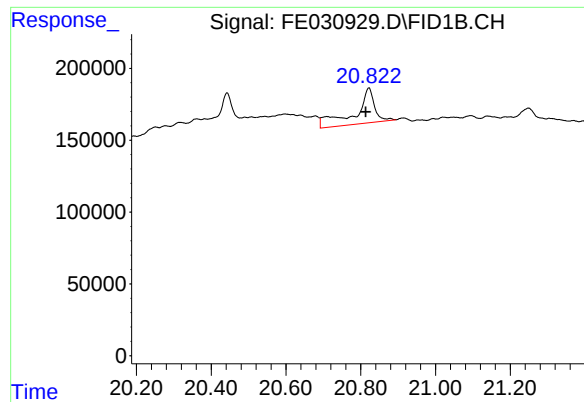

#17 N-OCTATRIACONTANE

R.T.: 20.822 min
Delta R.T.: 0.008 min
Response: 887150
Conc: 3.51 ug/ml

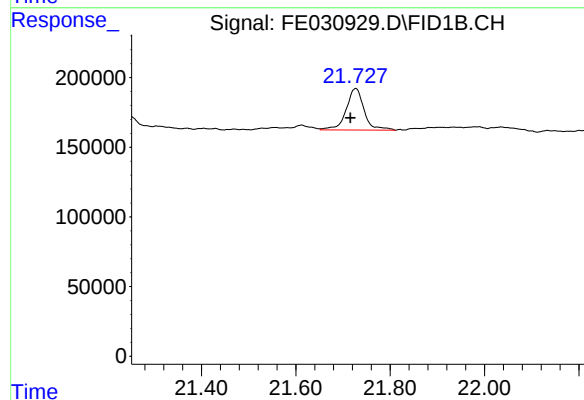

#18 N-TETRACONTANE

R.T.: 21.727 min
Delta R.T.: 0.011 min
Response: 788367
Conc: 3.00 ug/ml