

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE12223AL\
 Data File : FE045489.D
 Signal(s) : FID1B.ch
 Acq On : 22 Nov 2023 04:41
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Nov 22 22:44:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 110423.M
 Quant Title : GC Extractables
 QLast Update : Sat Nov 04 05:16:05 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	12.861	181763	1.147 ug/ml
11) T n-Heneicosane (C21)	13.481	198778	1.293 ug/ml
13) T n-Docosane (C22)	14.071	191981	1.267 ug/ml
14) T n-Tetracosane (C24)	15.176	120302	0.812 ug/ml
15) T n-Hexacosane (C26)	16.201	115907	0.795 ug/ml
16) T n-Octacosane (C28)	17.154	117288	0.803 ug/ml
17) T n-Tricontane (C30)	18.044	106443	0.701 ug/ml
18) T n-Dotriacontane (C32)	18.877	257884	1.651 ug/ml
19) T n-Tetratriacontane (C34)	19.664	92535	0.593 ug/ml
20) T n-Hexatriacontane (C36)	20.408	59405	0.366 ug/ml
21) T n-Octatriacontane (C38)	21.140	299034	1.800 ug/ml
22) T n-Tetracontane (C40)	22.055	357896	2.095 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE122223AL\
Data File : FE045489.D
Signal(s) : FID1B.ch
Acq On : 22 Nov 2023 04:41
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Nov 22 22:44:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 110423.M
Quant Title : GC Extractables
QLast Update : Sat Nov 04 05:16:05 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

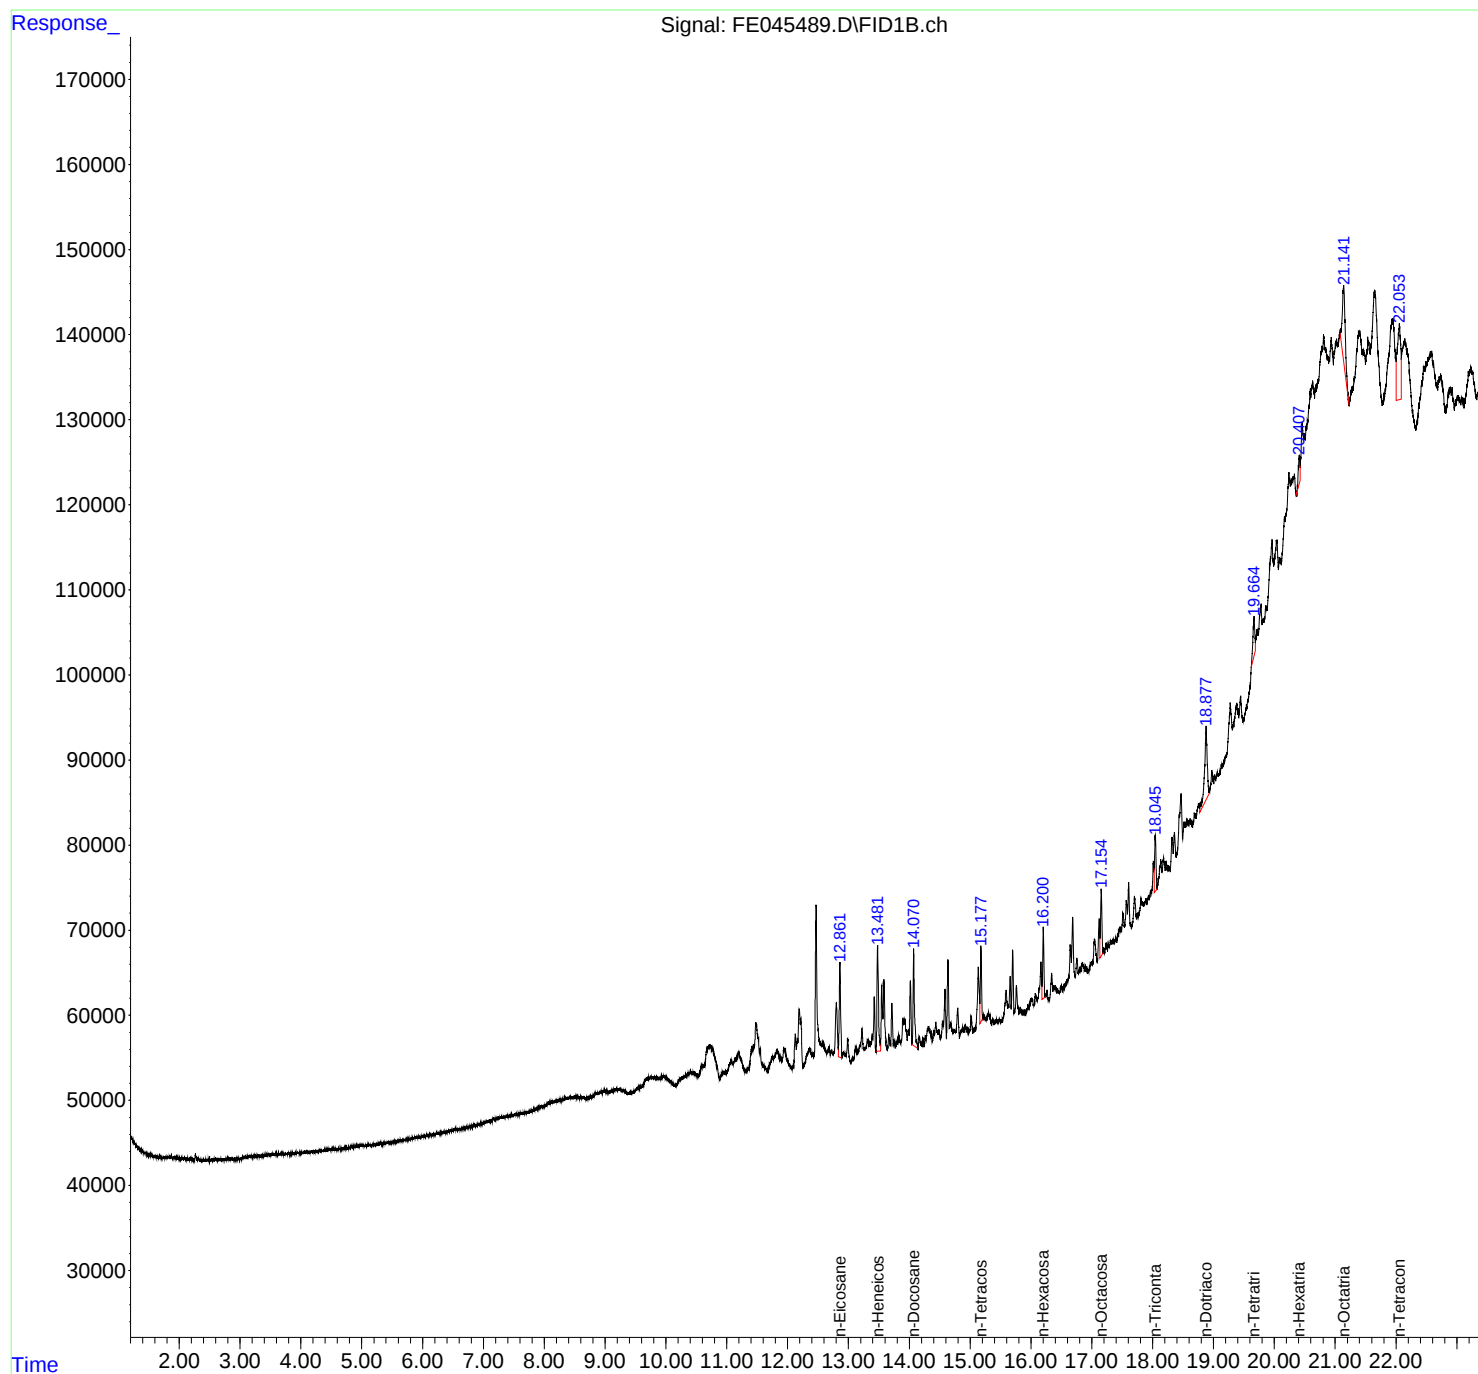


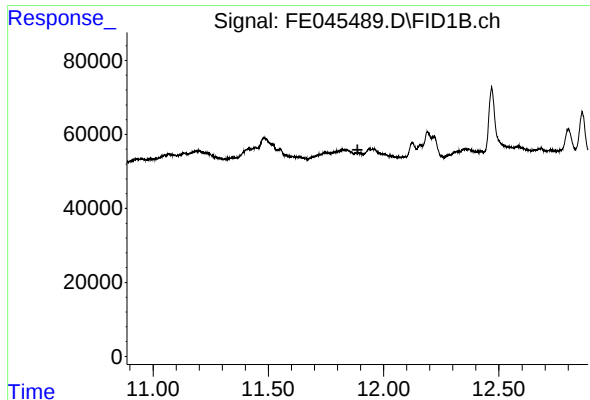

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.887 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

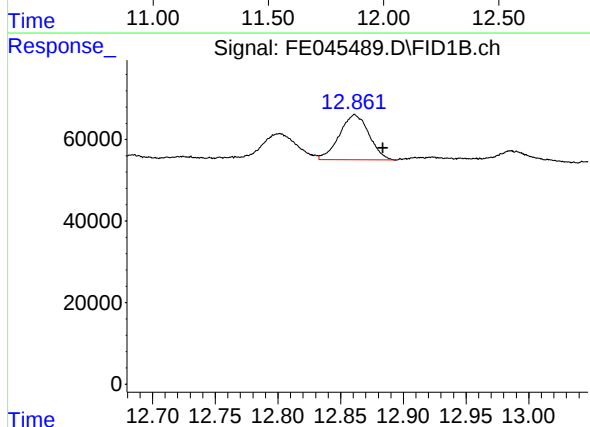


#10 n-Eicosane (C20)

R.T.: 12.861 min
Delta R.T.: -0.023 min
Response: 181763
Conc: 1.15 ug/ml

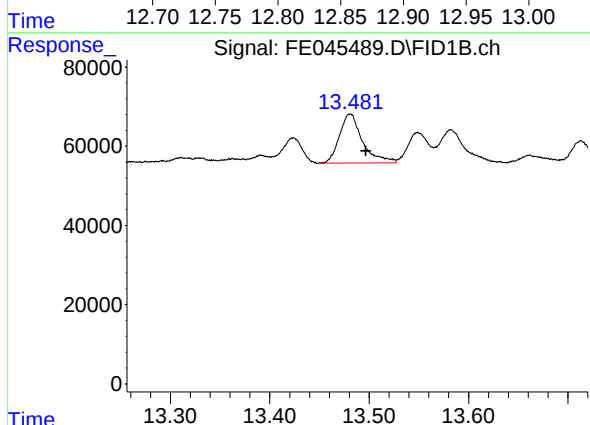


#11 n-Heneicosane (C21)

R.T.: 13.481 min
Delta R.T.: -0.016 min
Response: 198778
Conc: 1.29 ug/ml

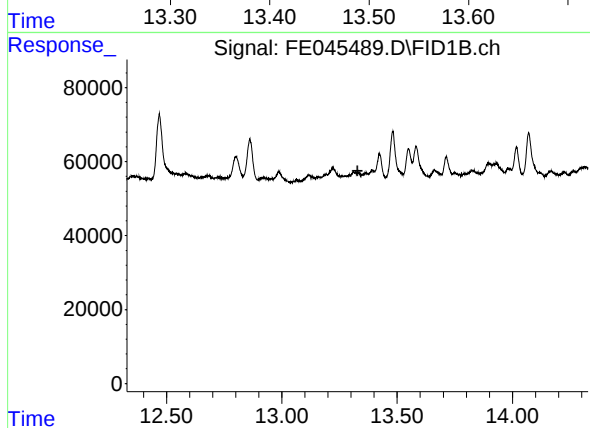

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.328 min
Response: 0
Conc: N.D.

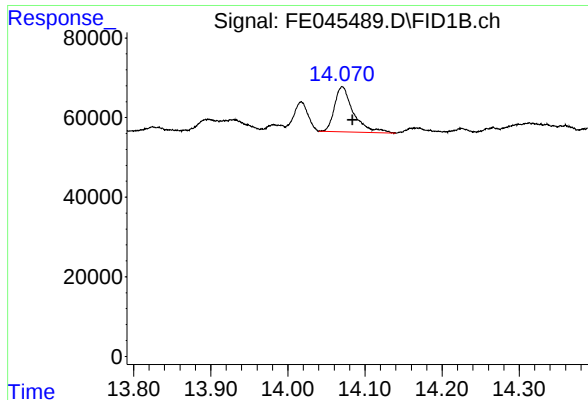

#13 n-Docosane (C22)


R.T.: 14.071 min
Delta R.T.: -0.013 min
Response: 191981
Conc: 1.27 ug/ml

Instrument :
FID_E
ClientSampleId :

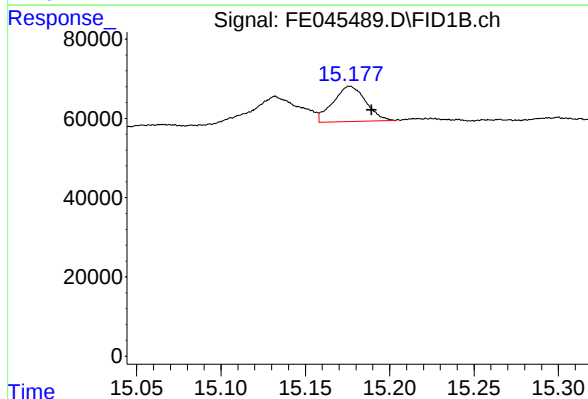


#14 n-Tetracosane (C24)

R.T.: 15.176 min
Delta R.T.: -0.013 min
Response: 120302
Conc: 0.81 ug/ml

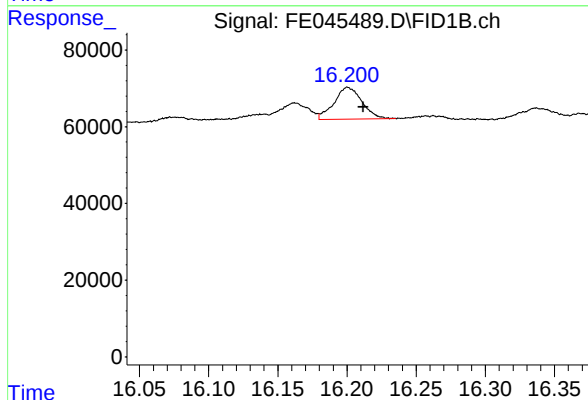


#15 n-Hexacosane (C26)

R.T.: 16.201 min
Delta R.T.: -0.011 min
Response: 115907
Conc: 0.80 ug/ml

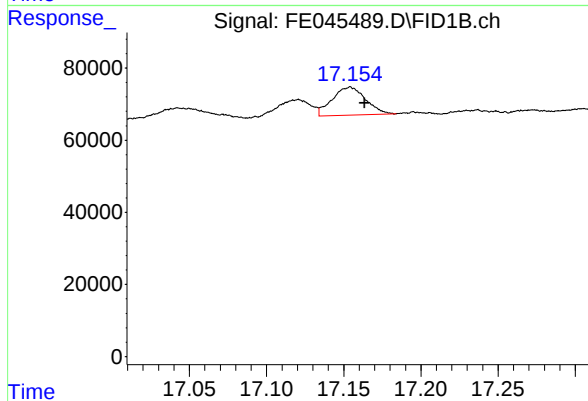

#16 n-Octacosane (C28)


R.T.: 17.154 min
Delta R.T.: -0.009 min
Response: 117288
Conc: 0.80 ug/ml

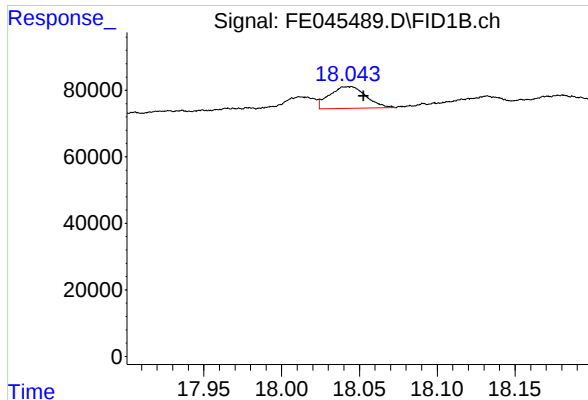

#17 n-Tricontane (C30)


R.T.: 18.044 min
Delta R.T.: -0.009 min
Response: 106443
Conc: 0.70 ug/ml

Instrument :
FID_E
ClientSampleId :

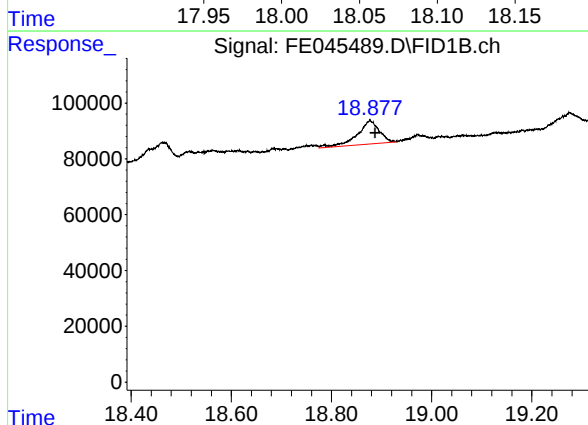


#18 n-Dotriacontane (C32)

R.T.: 18.877 min
Delta R.T.: -0.011 min
Response: 257884
Conc: 1.65 ug/ml

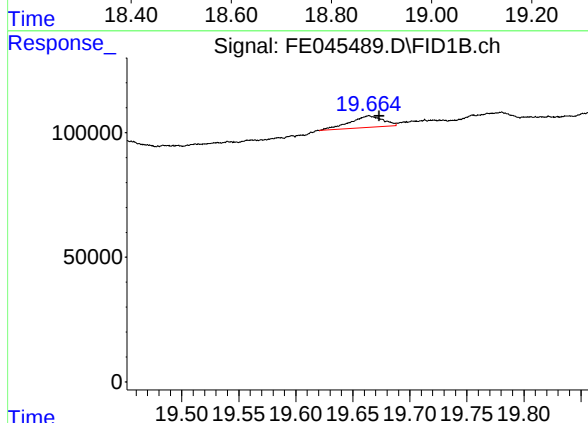


#19 n-Tetratriacontane (C34)

R.T.: 19.664 min
Delta R.T.: -0.009 min
Response: 92535
Conc: 0.59 ug/ml

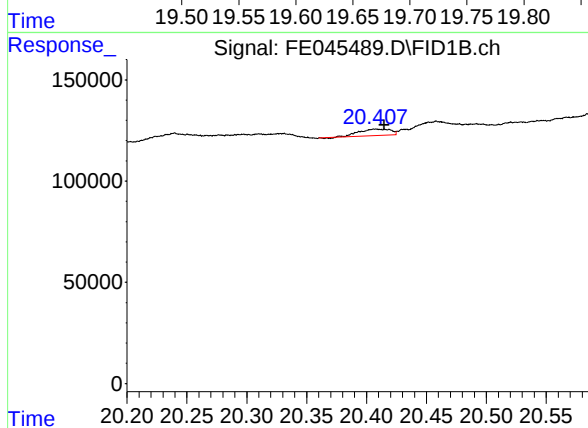

#20 n-Hexatriacontane (C36)


R.T.: 20.408 min
Delta R.T.: -0.007 min
Response: 59405
Conc: 0.37 ug/ml

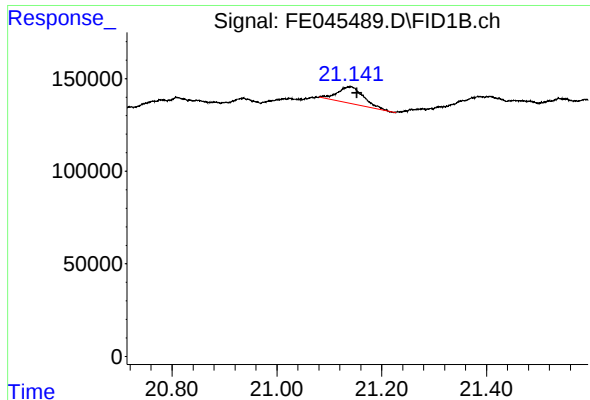

#21 n-Octatriacontane (C38)

R.T.: 21.140 min
Delta R.T.: -0.013 min
Response: 299034
Conc: 1.80 ug/ml

Instrument :
FID_E
ClientSampleId :

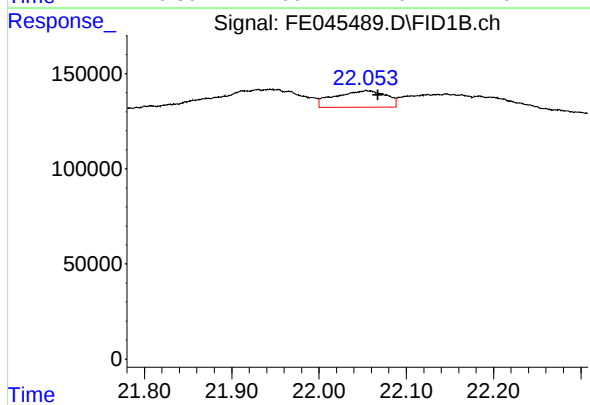

#22 n-Tetracontane (C40)

R.T.: 22.055 min
Delta R.T.: -0.013 min
Response: 357896
Conc: 2.10 ug/ml