

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112320\
Data File : FE033165.D
Signal(s) : FID1B.CH
Acq On : 23 Nov 2020 15:03
Operator : DD\AJ
Sample : L4800-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
KENS-B1-111820-0-1

Integration File: autoint1.e
Quant Time: Nov 24 00:11:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE110220.M
Quant Title :
QLast Update : Tue Nov 03 00:53:10 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.613	4372850	13.847 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112320\
Data File : FE033165.D
Signal(s) : FID1B.CH
Acq On : 23 Nov 2020 15:03
Operator : DD\AJ
Sample : L4800-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
KENS-B1-111820-0-1

Integration File: autoint1.e
Quant Time: Nov 24 00:11:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE110220.M
Quant Title :
QLast Update : Tue Nov 03 00:53:10 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

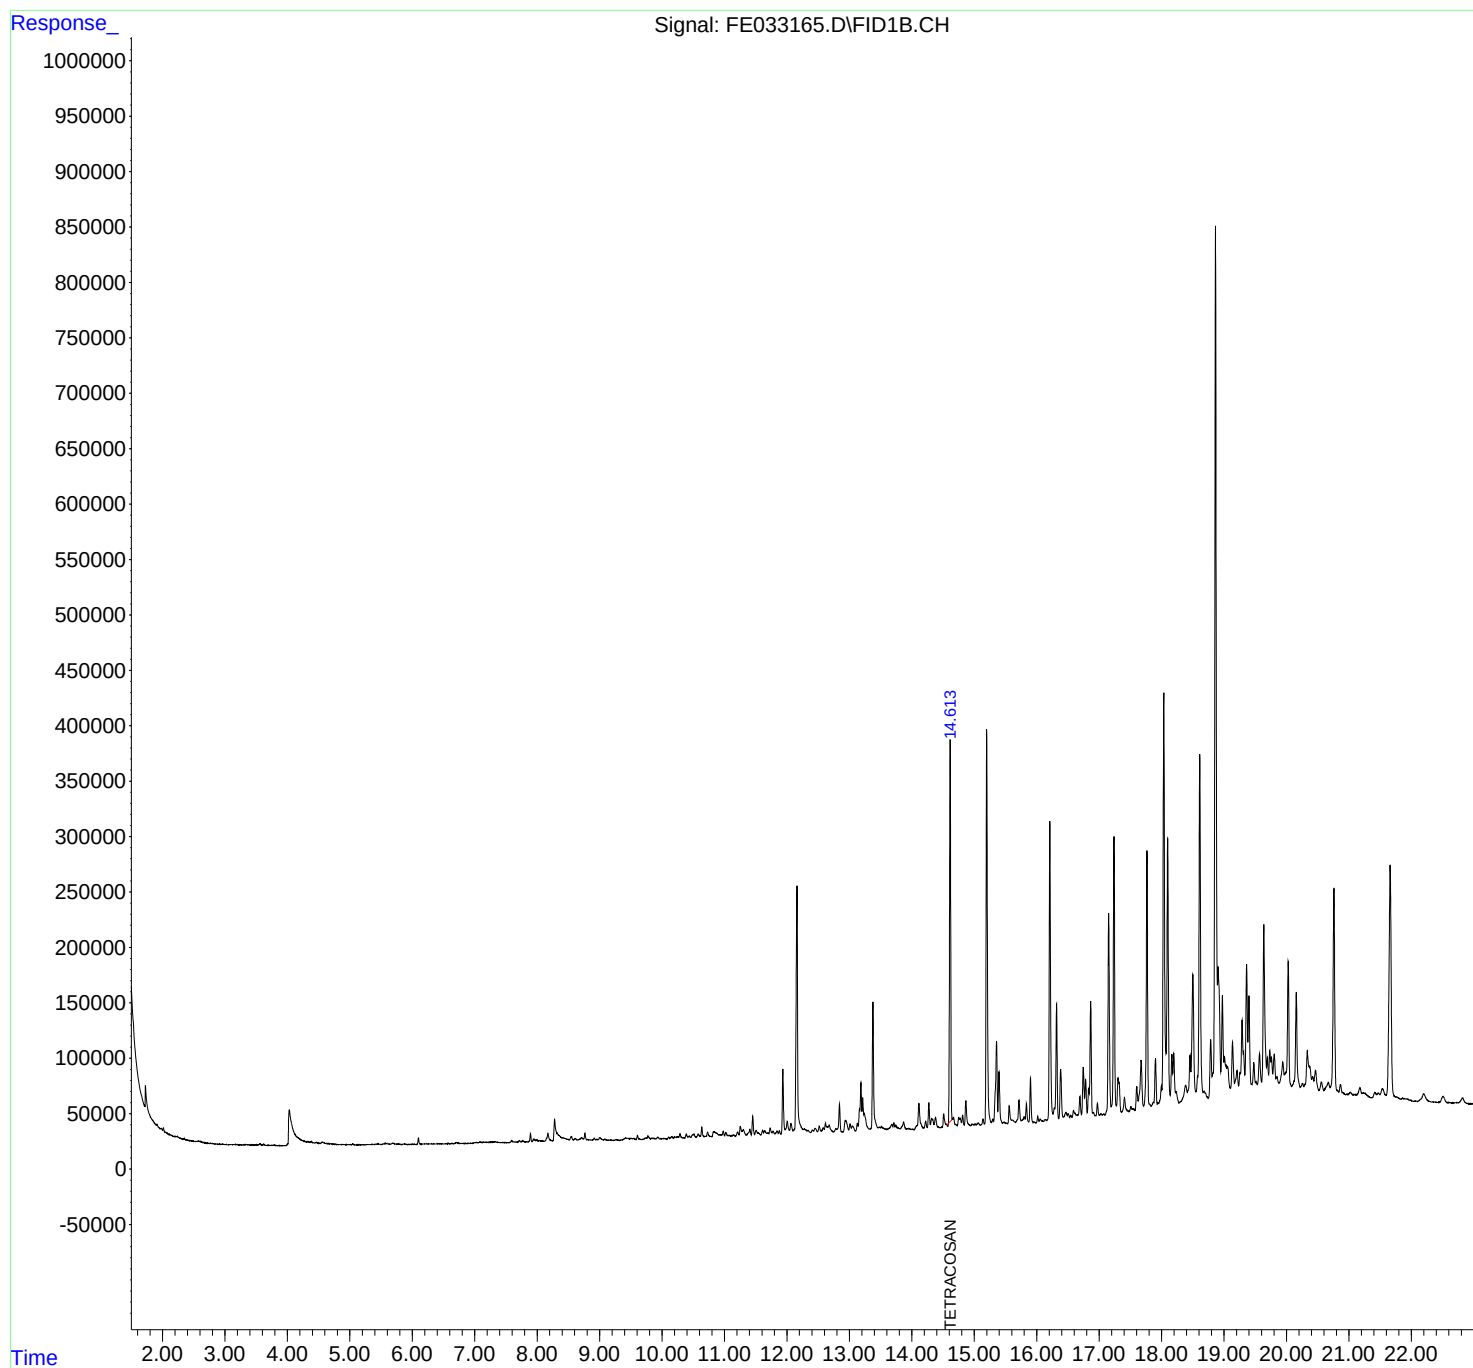

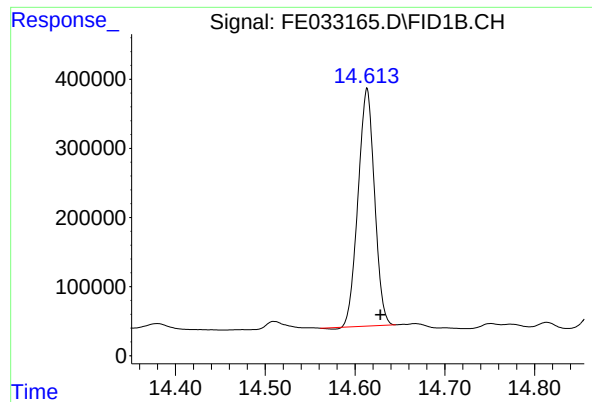

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.613 min
Delta R.T.: -0.015 min
Response: 4372850
Conc: 13.85 ug/ml

Instrument :
FID_E
ClientSampleId :
KENS-B1-111820-0-1