

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112320\
Data File : FE033168.D
Signal(s) : FID1B.CH
Acq On : 23 Nov 2020 16:44
Operator : DD\AJ
Sample : L4838-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
KENS-B2-111920-6-8

Integration File: autoint1.e
Quant Time: Nov 24 00:11:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE110220.M
Quant Title :
QLast Update : Tue Nov 03 00:53:10 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.615	4974559	15.752 ug/ml

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE112320\
Data File : FE033168.D
Signal(s) : FID1B.CH
Acq On : 23 Nov 2020 16:44
Operator : DD\AJ
Sample : L4838-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
KENS-B2-111920-6-8

Integration File: autoint1.e
Quant Time: Nov 24 00:11:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE110220.M
Quant Title :
QLast Update : Tue Nov 03 00:53:10 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

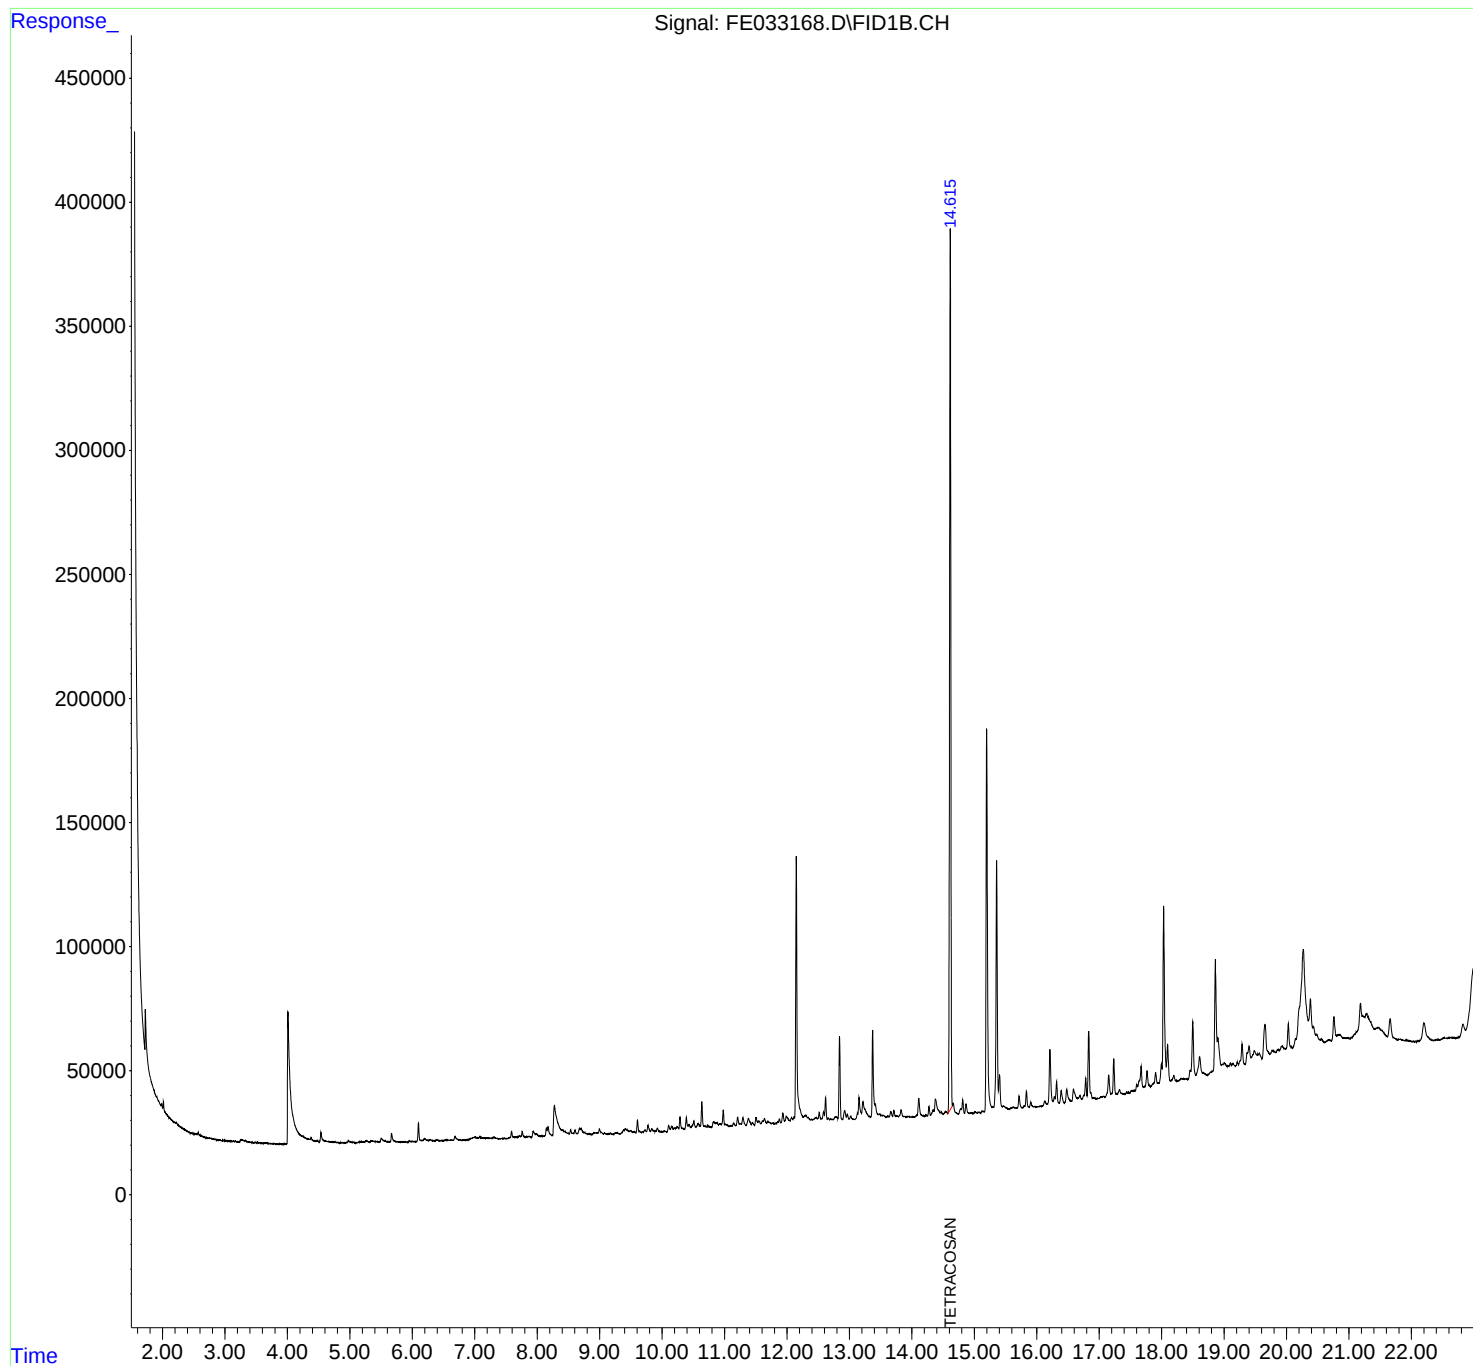

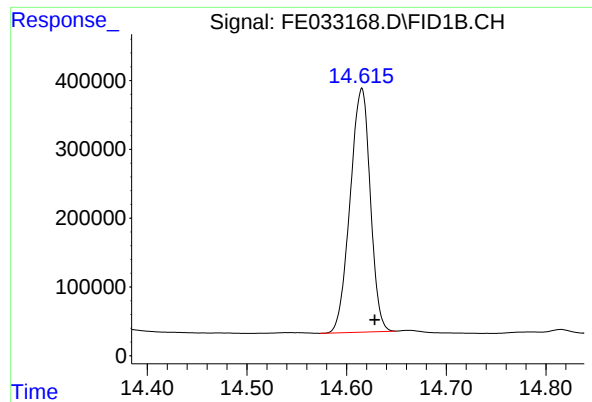

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.615 min
Delta R.T.: -0.013 min
Response: 4974559
Conc: 15.75 ug/ml

Instrument :
FID_E
ClientSampleId :
KENS-B2-111920-6-8